

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011398.D
 Acq On : 11 Aug 2022 21:58
 Operator : CG/JU
 Sample : PB146871BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK871

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	26	rVB	35811	49151	2.31%	0.221%
2	3.493	82	86	106	rBV	364180	572935	26.95%	2.572%
3	3.799	135	138	142	rVB	7544	9131	0.43%	0.041%
4	6.764	635	642	656	rBV	397813	642901	30.25%	2.886%
5	6.928	663	670	685	rVB	314621	492808	23.18%	2.212%
6	7.111	694	701	712	rBV	450614	680924	32.03%	3.056%
7	7.575	773	780	790	rBV	322206	513990	24.18%	2.307%
8	8.299	896	903	914	rBV	461795	751178	35.34%	3.372%
9	8.740	971	978	991	rBV	384237	633375	29.80%	2.843%
10	9.158	1045	1049	1052	rVV5	1578	2319	0.11%	0.010%
11	9.463	1093	1101	1114	rBV	297889	513307	24.15%	2.304%
12	9.999	1181	1192	1204	rBV	404627	719755	33.86%	3.231%
13	10.369	1248	1255	1268	rBV	428263	704136	33.13%	3.160%
14	10.522	1274	1281	1297	rBV	383655	701781	33.02%	3.150%
15	11.652	1469	1473	1483	rVB	1444	3258	0.15%	0.015%
16	11.981	1523	1529	1537	rBV6	7222	16175	0.76%	0.073%
17	12.199	1561	1566	1570	rBV8	1553	3006	0.14%	0.013%
18	13.228	1736	1741	1743	rBV5	1732	2706	0.13%	0.012%
19	13.675	1810	1817	1830	rBV	794391	1115649	52.49%	5.008%
20	13.940	1856	1862	1879	rBV	830381	1222060	57.49%	5.485%
21	14.251	1909	1915	1926	rBV	581875	842521	39.64%	3.782%
22	14.487	1949	1955	1973	rBV	185222	451263	21.23%	2.025%
23	15.257	2077	2086	2103	rBV	1042036	1545670	72.72%	6.938%
24	15.387	2103	2108	2123	rVV	330036	523559	24.63%	2.350%
25	15.504	2123	2128	2141	rVB5	13660	34186	1.61%	0.153%
26	15.916	2196	2198	2202	rBV5	1464	2330	0.11%	0.010%
27	16.051	2216	2221	2227	rBB9	3783	5622	0.26%	0.025%
28	16.704	2328	2332	2336	rVB7	2145	2720	0.13%	0.012%
29	16.816	2346	2351	2355	rBV6	2813	5754	0.27%	0.026%
30	17.022	2380	2386	2397	rBV	726364	1043171	49.08%	4.682%
31	17.122	2397	2403	2424	rVB	1200205	1791441	84.28%	8.041%
32	17.716	2501	2504	2508	rBV6	2515	2406	0.11%	0.011%
33	18.963	2711	2716	2722	rBV5	17028	26347	1.24%	0.118%
34	19.034	2723	2728	2733	rVV	16986	26001	1.22%	0.117%
35	19.386	2782	2788	2799	rBV	1626717	2072497	97.50%	9.302%
36	21.151	3084	3088	3097	rBV	897362	1184610	55.73%	5.317%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011398.D
Acq On : 11 Aug 2022 21:58
Operator : CG/JU
Sample : PB146871BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	23.310	3449	3455	3463	rBV	1174450	2125580	100.00%	9.541%
38	23.457	3474	3480	3490	rVB2	633224	1243048	58.48%	5.579%




Sum of corrected areas: 22279271

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011398.D
Acq On : 11 Aug 2022 21:58
Operator : CG/JU
Sample : PB146871BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

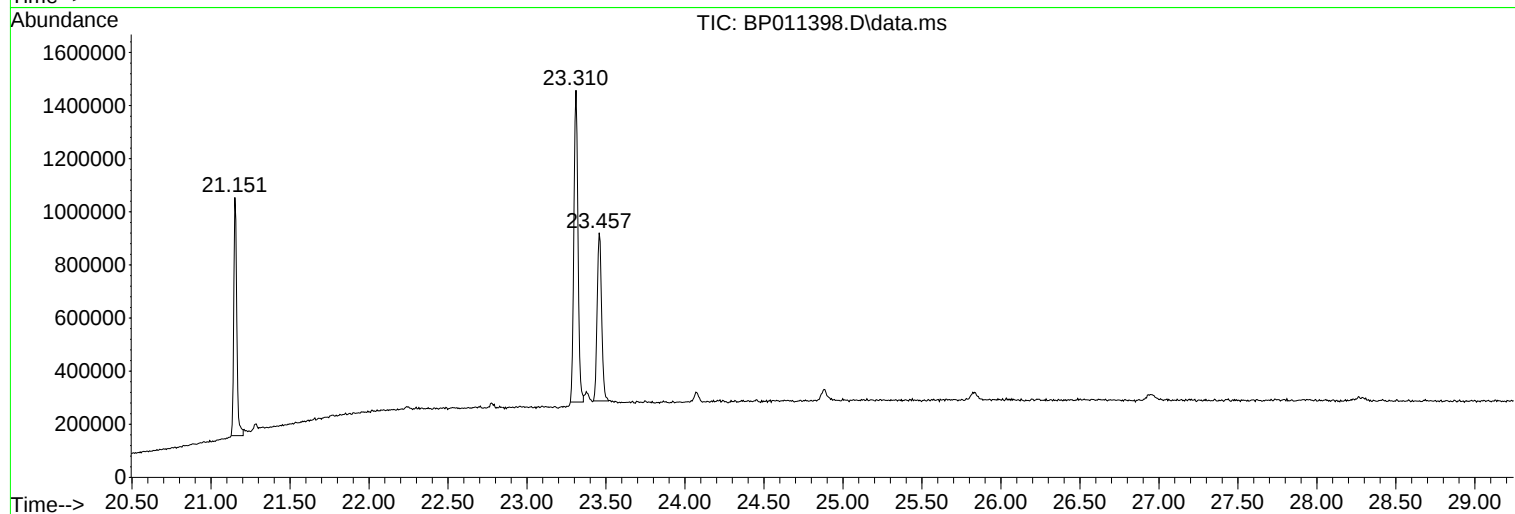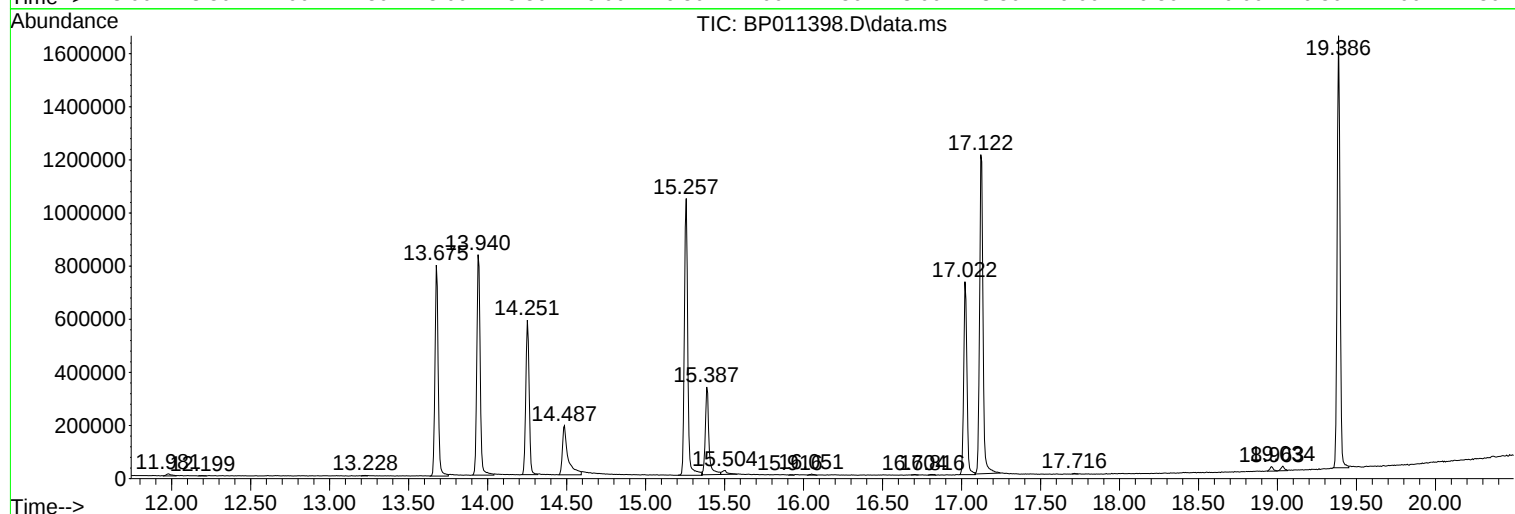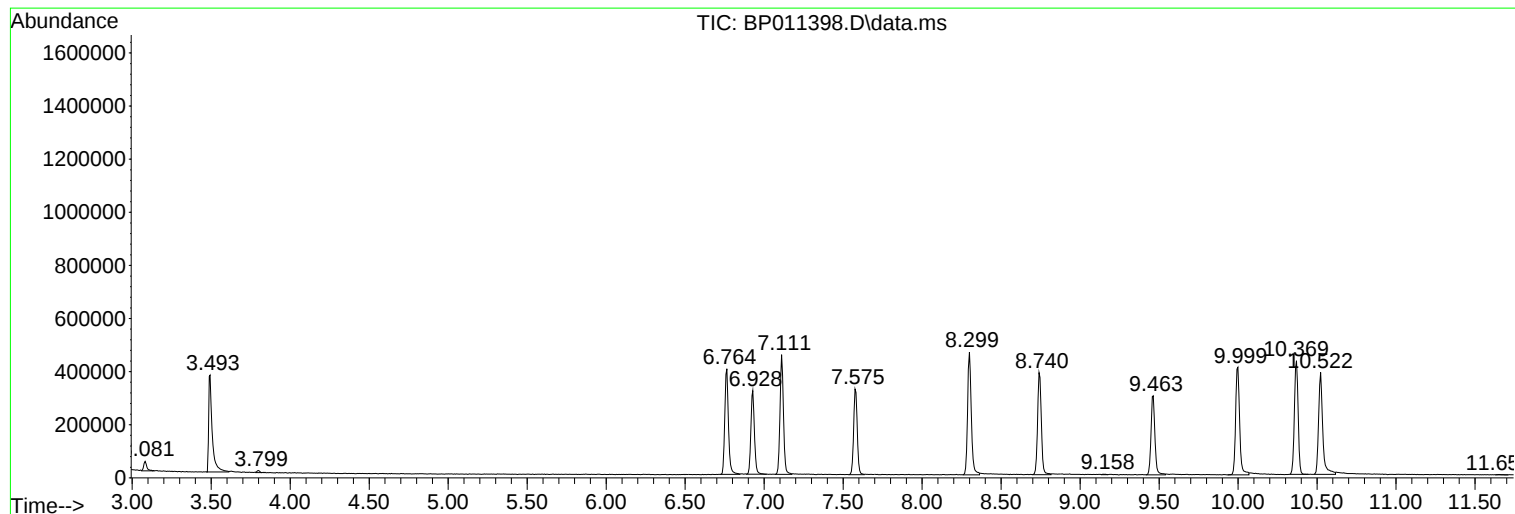

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011398.D
Acq On : 11 Aug 2022 21:58
Operator : CG/JU
Sample : PB146871BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011398.D
Acq On : 11 Aug 2022 21:58
Operator : CG/JU
Sample : PB146871BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc