

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011400.D
 Acq On : 11 Aug 2022 23:07
 Operator : CG/JU
 Sample : N4128-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	23	rBV	28790	33348	1.10%	0.122%
2	3.499	85	87	103	rBV	121982	194365	6.38%	0.709%
3	3.705	118	122	128	rVB3	14322	21854	0.72%	0.080%
4	3.799	134	138	142	rVB	10418	13297	0.44%	0.049%
5	4.234	208	212	219	rVB	23119	32063	1.05%	0.117%
6	4.711	291	293	297	rVB3	3015	3215	0.11%	0.012%
7	4.828	310	313	316	rVB4	3897	4704	0.15%	0.017%
8	5.593	441	443	449	rVB6	2282	3426	0.11%	0.012%
9	6.711	628	633	637	rBV2	12910	20027	0.66%	0.073%
10	6.764	637	642	653	rVB	101121	162237	5.33%	0.592%
11	6.928	662	670	685	rBV	369105	587387	19.29%	2.143%
12	7.111	694	701	712	rBV	400695	627995	20.62%	2.291%
13	7.193	712	715	725	rVB9	5226	12391	0.41%	0.045%
14	7.575	773	780	790	rBV	446597	699869	22.98%	2.553%
15	8.299	895	903	922	rBV	278830	472245	15.51%	1.723%
16	8.740	971	978	995	rBV	467864	781200	25.65%	2.850%
17	8.875	997	1001	1005	rVB6	3403	5983	0.20%	0.022%
18	9.152	1043	1048	1053	rVB2	13715	21677	0.71%	0.079%
19	9.458	1093	1100	1119	rBV	364994	610378	20.04%	2.227%
20	9.993	1184	1191	1215	rBV	463790	817301	26.84%	2.982%
21	10.369	1247	1255	1264	rBV	588562	957975	31.46%	3.495%
22	10.522	1274	1281	1297	rBV	391958	724035	23.78%	2.641%
23	11.216	1397	1399	1407	rVB9	1787	3647	0.12%	0.013%
24	11.652	1468	1473	1480	rVB4	9540	15803	0.52%	0.058%
25	11.981	1523	1529	1533	rBV2	9018	15298	0.50%	0.056%
26	12.193	1561	1565	1570	rVB8	1969	3126	0.10%	0.011%
27	13.163	1724	1730	1734	rBV9	1695	3150	0.10%	0.011%
28	13.228	1734	1741	1746	rVV9	3386	5844	0.19%	0.021%
29	13.675	1811	1817	1834	rBV	1008339	1445912	47.48%	5.275%
30	13.940	1855	1862	1875	rBV	1038335	1546544	50.79%	5.642%
31	14.251	1908	1915	1924	rBV	826029	1202098	39.48%	4.385%
32	14.493	1950	1956	1967	rBV2	29563	80701	2.65%	0.294%
33	15.010	2037	2044	2045	rBV6	4090	7531	0.25%	0.027%
34	15.257	2079	2086	2102	rBV	1412934	2031188	66.70%	7.410%
35	15.387	2102	2108	2123	rVV	461415	701744	23.04%	2.560%
36	15.498	2123	2127	2135	rVB3	16099	32731	1.07%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011400.D
 Acq On : 11 Aug 2022 23:07
 Operator : CG/JU
 Sample : N4128-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.828	2178	2183	2188	rBV8	2554	5776	0.19%	0.021%
38	15.993	2207	2211	2216	rVV5	6521	10369	0.34%	0.038%
39	16.051	2216	2221	2225	rVB7	4424	7295	0.24%	0.027%
40	16.163	2236	2240	2242	rBV5	2172	3111	0.10%	0.011%
41	16.510	2295	2299	2305	rVB3	7786	9820	0.32%	0.036%
42	16.698	2329	2331	2338	rVB8	2667	3914	0.13%	0.014%
43	16.804	2345	2349	2355	rBV8	3960	6631	0.22%	0.024%
44	16.975	2374	2378	2379	rBV4	2939	3306	0.11%	0.012%
45	17.022	2380	2386	2397	rBV	1001791	1479438	48.58%	5.397%
46	17.128	2397	2404	2415	rBV	1700194	2437644	80.05%	8.893%
47	17.592	2478	2483	2490	rVB8	7175	12448	0.41%	0.045%
48	17.716	2500	2504	2505	rBV4	4715	5645	0.19%	0.021%
49	17.945	2538	2543	2547	rBV8	4422	6978	0.23%	0.025%
50	18.016	2552	2555	2559	rVB2	4445	6264	0.21%	0.023%
51	18.404	2618	2621	2622	rBV3	3317	3842	0.13%	0.014%
52	18.516	2637	2640	2644	rBV6	6680	7834	0.26%	0.029%
53	18.963	2712	2716	2721	rVB5	21816	29142	0.96%	0.106%
54	19.034	2724	2728	2732	rBV	19485	27621	0.91%	0.101%
55	19.339	2778	2780	2782	rBV3	5696	3884	0.13%	0.014%
56	19.386	2782	2788	2798	rBV	2240727	2900857	95.26%	10.582%
57	21.157	3084	3089	3099	rBV	1279617	1698587	55.78%	6.196%
58	23.316	3449	3456	3464	rBV2	1664595	3045144	100.00%	11.109%
59	23.463	3475	3481	3492	rVB2	950831	1794429	58.93%	6.546%




Sum of corrected areas: 27412268

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011400.D
Acq On : 11 Aug 2022 23:07
Operator : CG/JU
Sample : N4128-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

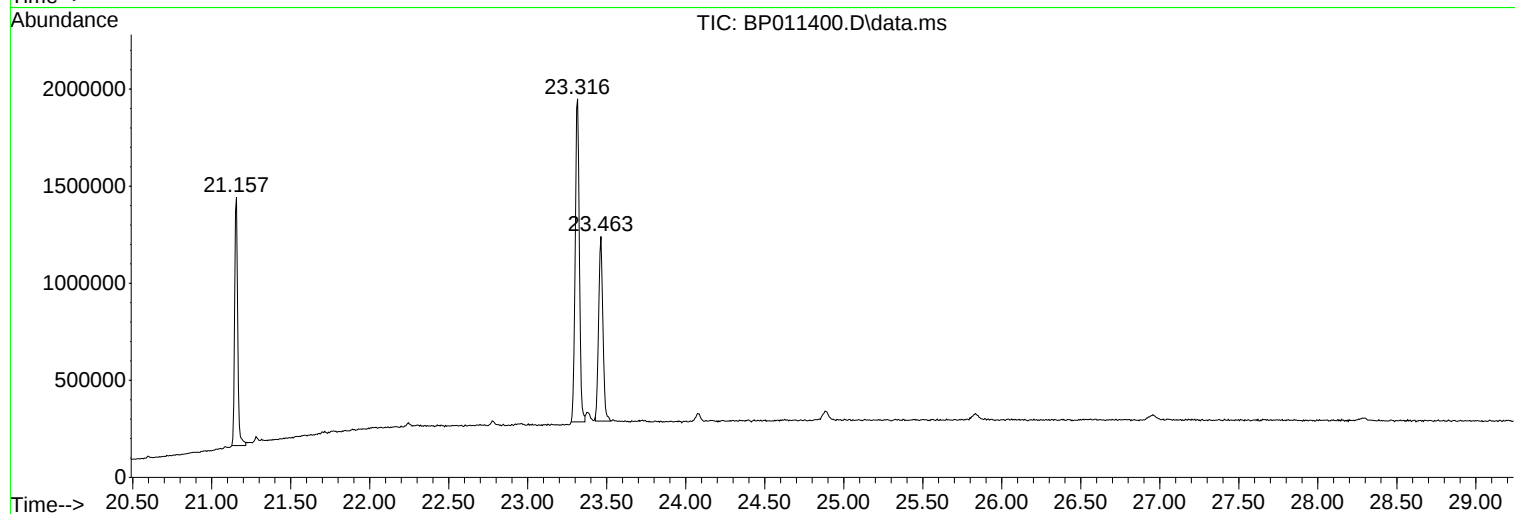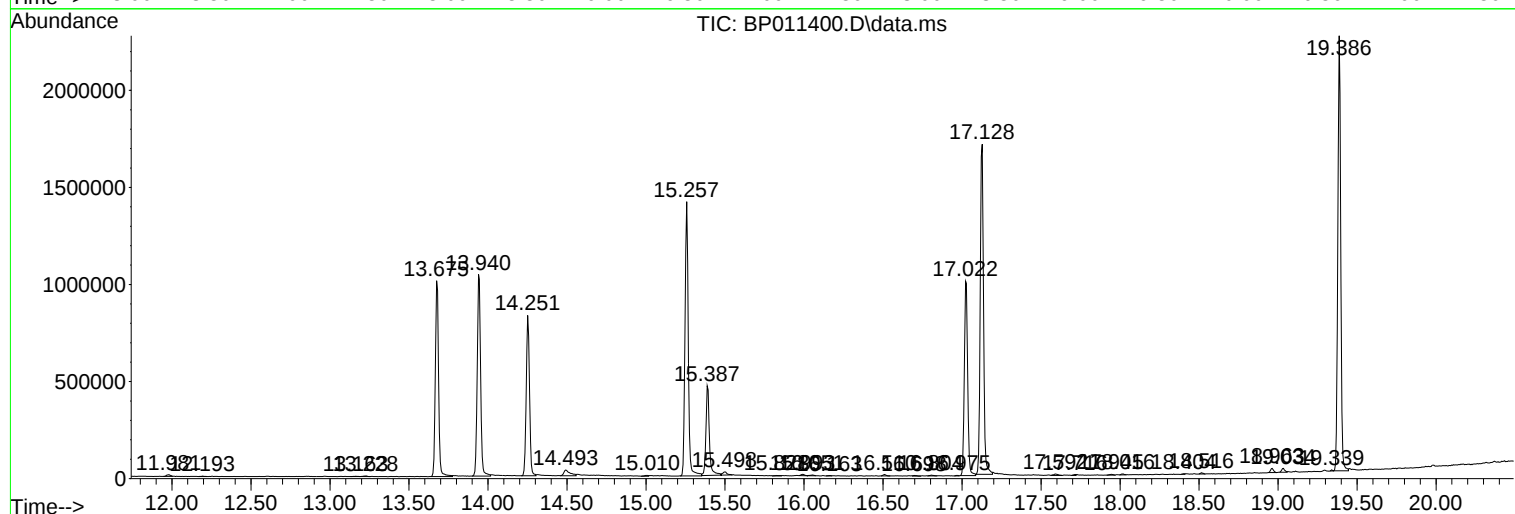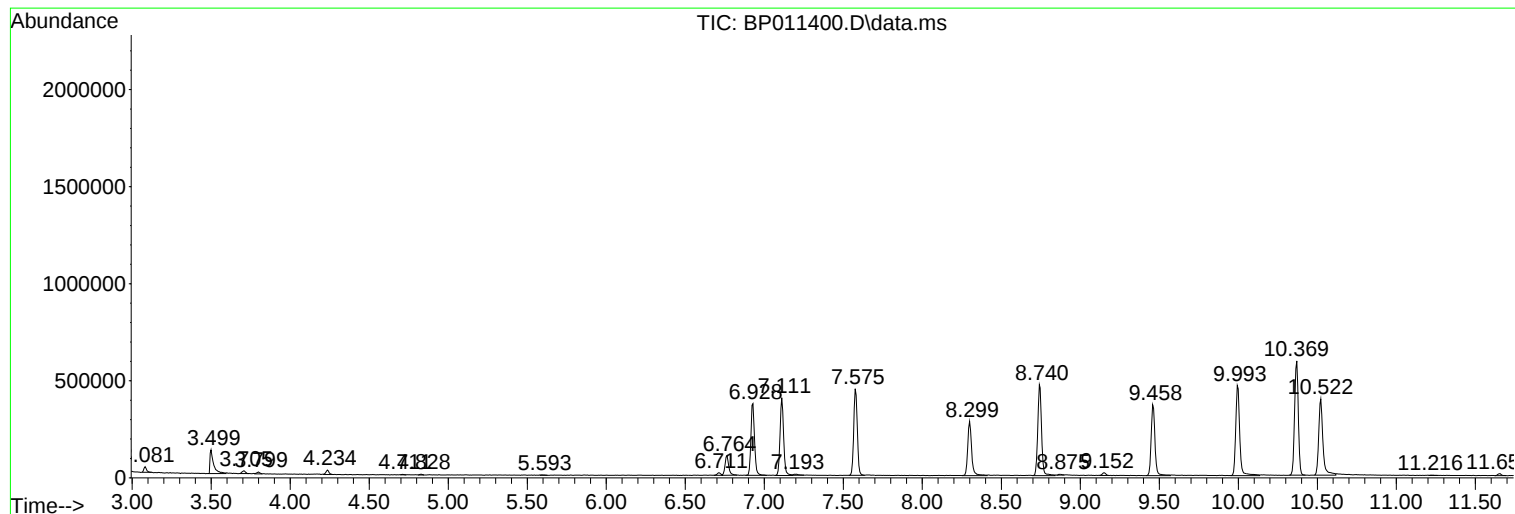

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011400.D
Acq On : 11 Aug 2022 23:07
Operator : CG/JU
Sample : N4128-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011400.D
Acq On : 11 Aug 2022 23:07
Operator : CG/JU
Sample : N4128-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc