

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011401.D
 Acq On : 11 Aug 2022 23:41
 Operator : CG/JU
 Sample : N4128-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	23	rVB	29486	36864	1.47%	0.166%
2	3.499	84	87	106	rVB	96228	156139	6.25%	0.702%
3	3.705	117	122	128	rVB2	14956	24041	0.96%	0.108%
4	3.799	134	138	142	rBV3	8133	9297	0.37%	0.042%
5	4.234	207	212	218	rVB	20515	29265	1.17%	0.132%
6	4.340	226	230	232	rBV5	1838	2604	0.10%	0.012%
7	4.828	310	313	319	rVB8	3838	4559	0.18%	0.020%
8	6.711	629	633	636	rBV	11349	15095	0.60%	0.068%
9	6.764	636	642	652	rVB	84338	138874	5.55%	0.624%
10	6.928	664	670	681	rBV	279133	452951	18.12%	2.036%
11	7.111	693	701	713	rBV	314455	496611	19.86%	2.232%
12	7.199	713	716	723	rVB7	4083	7321	0.29%	0.033%
13	7.575	772	780	789	rBV	368089	576331	23.05%	2.591%
14	7.663	789	795	802	rVB	3149	8547	0.34%	0.038%
15	8.299	896	903	914	rBV	230297	377132	15.08%	1.695%
16	8.740	971	978	993	rBV	357033	590446	23.62%	2.654%
17	8.916	1005	1008	1014	rVB7	1924	2862	0.11%	0.013%
18	9.146	1040	1047	1053	rBV	12999	21524	0.86%	0.097%
19	9.457	1093	1100	1111	rBV	266541	451025	18.04%	2.028%
20	9.993	1184	1191	1204	rBV	353350	621943	24.88%	2.796%
21	10.369	1246	1255	1263	rBV	473221	798096	31.92%	3.588%
22	10.522	1273	1281	1291	rBV	273278	504462	20.18%	2.268%
23	11.652	1466	1473	1479	rVB	11136	17844	0.71%	0.080%
24	11.975	1522	1528	1533	rBV5	7123	13804	0.55%	0.062%
25	12.599	1628	1634	1640	rBV5	1937	3578	0.14%	0.016%
26	12.863	1675	1679	1683	rVB7	2226	3520	0.14%	0.016%
27	13.228	1736	1741	1745	rVB8	2354	3899	0.16%	0.018%
28	13.675	1811	1817	1834	rBV	793583	1120288	44.81%	5.036%
29	13.940	1852	1862	1872	rBV	813901	1201247	48.05%	5.400%
30	14.251	1908	1915	1924	rBV	680893	979581	39.18%	4.404%
31	14.493	1951	1956	1972	rBV2	23699	77233	3.09%	0.347%
32	15.128	2061	2064	2067	rVB4	2556	3013	0.12%	0.014%
33	15.257	2077	2086	2102	rBV	1092536	1601972	64.07%	7.201%
34	15.387	2102	2108	2123	rVV	350926	554099	22.16%	2.491%
35	15.498	2124	2127	2138	rVV4	15398	33955	1.36%	0.153%
36	15.998	2208	2212	2218	rVV9	3857	6726	0.27%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011401.D
 Acq On : 11 Aug 2022 23:41
 Operator : CG/JU
 Sample : N4128-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.051	2218	2221	2225	rVB6	4844	6137	0.25%	0.028%
38	16.169	2238	2241	2248	rVB9	2278	3524	0.14%	0.016%
39	16.510	2294	2299	2303	rBV5	6133	9611	0.38%	0.043%
40	16.804	2345	2349	2355	rVV9	3886	6895	0.28%	0.031%
41	16.845	2355	2356	2364	rVB7	2547	3469	0.14%	0.016%
42	17.022	2380	2386	2397	rBV	843269	1208786	48.35%	5.434%
43	17.122	2397	2403	2423	rVV	1326112	2008261	80.32%	9.028%
44	17.416	2451	2453	2455	rBV3	2835	2704	0.11%	0.012%
45	17.592	2479	2483	2490	rVB8	7151	10570	0.42%	0.048%
46	17.692	2497	2500	2501	rBV3	2995	3121	0.12%	0.014%
47	17.722	2501	2505	2510	rVV8	5872	11309	0.45%	0.051%
48	17.939	2538	2542	2546	rBV6	9462	14422	0.58%	0.065%
49	18.016	2551	2555	2559	rVB4	4974	7388	0.30%	0.033%
50	18.516	2637	2640	2644	rVB5	5801	7182	0.29%	0.032%
51	18.963	2712	2716	2722	rBV4	16949	23577	0.94%	0.106%
52	19.033	2724	2728	2731	rVB	15272	19883	0.80%	0.089%
53	19.386	2782	2788	2798	rBV	1865626	2382611	95.30%	10.711%
54	20.886	3040	3043	3050	rBV4	57487	92123	3.68%	0.414%
55	21.080	3073	3076	3081	rBV	60698	67696	2.71%	0.304%
56	21.151	3084	3088	3101	rVV	1058616	1433240	57.32%	6.443%
57	23.310	3449	3455	3463	rBV2	1310251	2500207	100.00%	11.239%
58	23.457	3474	3480	3491	rVB2	751924	1475717	59.02%	6.634%




Sum of corrected areas: 22245181

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011401.D
Acq On : 11 Aug 2022 23:41
Operator : CG/JU
Sample : N4128-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

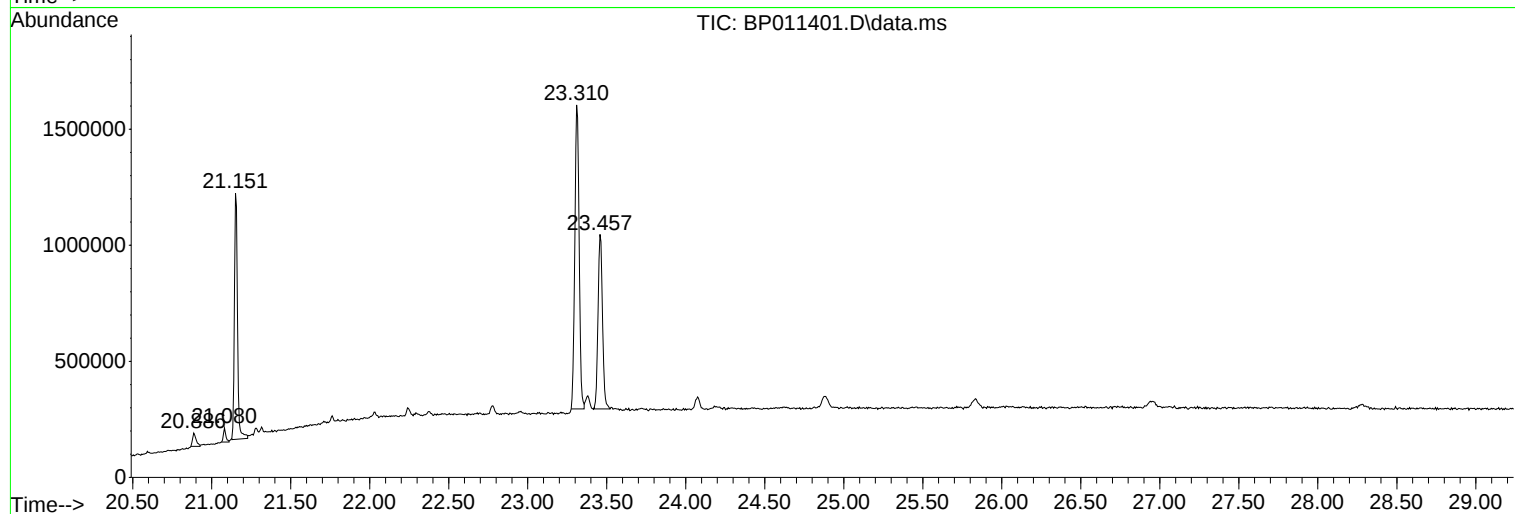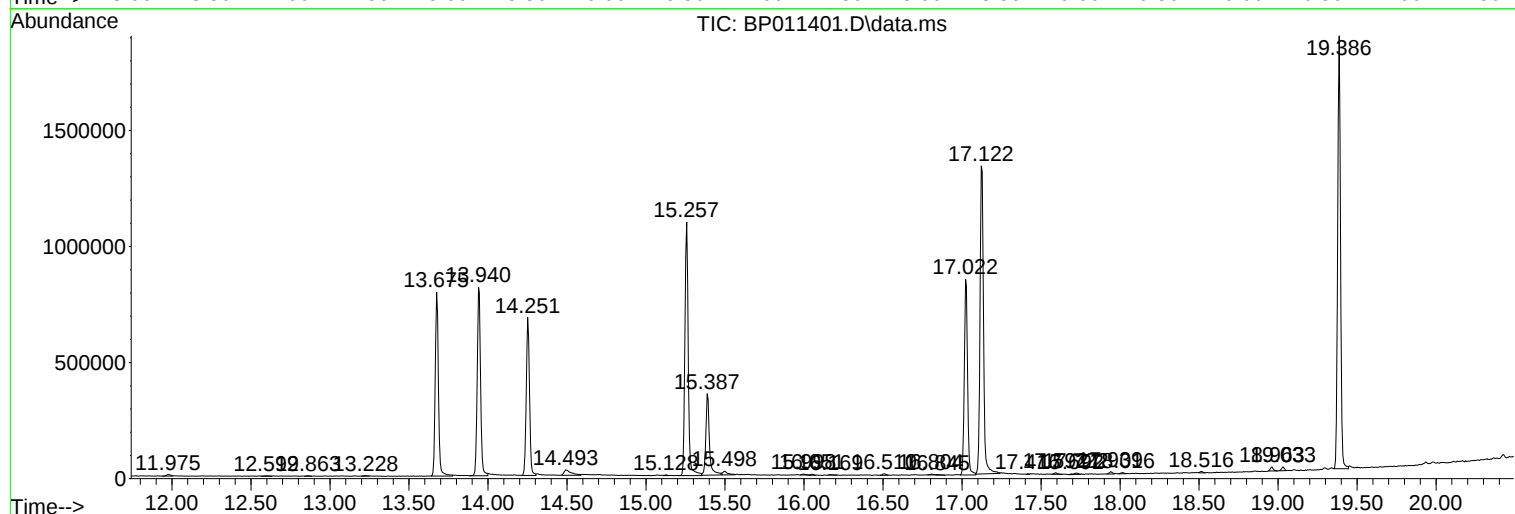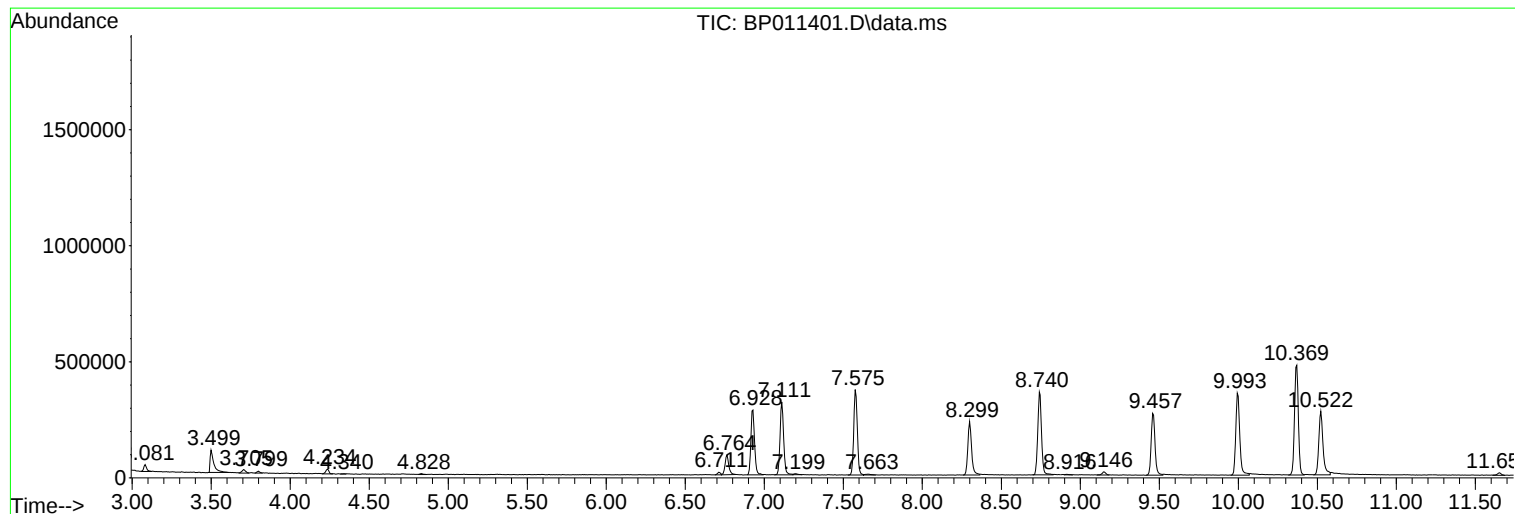

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011401.D
Acq On : 11 Aug 2022 23:41
Operator : CG/JU
Sample : N4128-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011401.D
Acq On : 11 Aug 2022 23:41
Operator : CG/JU
Sample : N4128-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc