

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011402.D
 Acq On : 12 Aug 2022 00:16
 Operator : CG/JU
 Sample : N4128-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	24	rVB	28029	34939	1.35%	0.146%
2	3.499	84	87	101	rBV	89021	144942	5.61%	0.606%
3	3.711	118	123	127	rBV	12339	18374	0.71%	0.077%
4	3.799	134	138	142	rVB	8454	11839	0.46%	0.049%
5	4.234	208	212	218	rVB	21277	28705	1.11%	0.120%
6	4.881	318	322	328	rVB5	4255	6108	0.24%	0.026%
7	6.711	627	633	637	rBV3	11216	18909	0.73%	0.079%
8	6.764	637	642	651	rVB	70886	117114	4.53%	0.489%
9	6.928	663	670	684	rBV	316137	504521	19.53%	2.108%
10	7.111	694	701	710	rBV	326072	507743	19.66%	2.121%
11	7.193	713	715	723	rVB9	3949	7620	0.29%	0.032%
12	7.575	773	780	791	rBV	432594	680206	26.33%	2.842%
13	8.299	897	903	919	rBV	215305	360833	13.97%	1.508%
14	8.740	971	978	986	rBV	399326	649470	25.14%	2.714%
15	8.911	1005	1007	1011	rVB5	2853	3048	0.12%	0.013%
16	9.152	1041	1048	1053	rBV3	11703	18574	0.72%	0.078%
17	9.458	1092	1100	1117	rBV	297150	507276	19.64%	2.119%
18	9.993	1184	1191	1203	rBV	372443	645952	25.01%	2.699%
19	10.369	1245	1255	1264	rBV	573488	944866	36.58%	3.948%
20	10.522	1272	1281	1299	rBV	328180	624440	24.17%	2.609%
21	11.652	1467	1473	1478	rVB4	8198	14221	0.55%	0.059%
22	11.822	1498	1502	1509	rVB9	1368	3192	0.12%	0.013%
23	11.975	1522	1528	1533	rBV7	6972	14012	0.54%	0.059%
24	12.975	1693	1698	1703	rBV8	1622	2941	0.11%	0.012%
25	13.675	1810	1817	1833	rBV	881573	1205301	46.66%	5.036%
26	13.940	1855	1862	1880	rBV	869506	1304348	50.49%	5.450%
27	14.251	1908	1915	1923	rBV	794107	1163668	45.05%	4.862%
28	14.498	1952	1957	1971	rBV7	14678	52047	2.01%	0.217%
29	15.257	2079	2086	2101	rBV	1141243	1705812	66.03%	7.127%
30	15.387	2103	2108	2121	rVV	347645	536684	20.78%	2.242%
31	15.498	2123	2127	2132	rVB4	12405	21442	0.83%	0.090%
32	16.045	2217	2220	2225	rVB7	3518	6425	0.25%	0.027%
33	16.163	2235	2240	2246	rBV10	1781	4434	0.17%	0.019%
34	16.510	2294	2299	2305	rVB3	6458	10058	0.39%	0.042%
35	16.810	2345	2350	2355	rBV8	3686	6173	0.24%	0.026%
36	17.022	2379	2386	2397	rBV	969350	1441886	55.82%	6.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011402.D
 Acq On : 12 Aug 2022 00:16
 Operator : CG/JU
 Sample : N4128-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	17.122	2397	2403	2427	rVB	1403915	2093647	81.05%	8.748%
38	17.592	2478	2483	2486	rBV6	6121	9167	0.35%	0.038%
39	17.716	2501	2504	2510	rVB7	5218	6467	0.25%	0.027%
40	17.939	2538	2542	2547	rBV8	3664	5625	0.22%	0.024%
41	18.016	2552	2555	2560	rVB3	4207	5994	0.23%	0.025%
42	18.516	2637	2640	2646	rVB7	4508	6284	0.24%	0.026%
43	18.963	2712	2716	2720	rVB2	17363	22130	0.86%	0.092%
44	19.034	2723	2728	2731	rBV2	17320	24441	0.95%	0.102%
45	19.386	2782	2788	2804	rBV	1900294	2455135	95.04%	10.258%
46	21.157	3084	3089	3100	rBV	1252703	1643664	63.63%	6.867%
47	23.316	3449	3456	3465	rBV	1383356	2583251	100.00%	10.793%
48	23.463	3475	3481	3497	rVB2	911476	1750217	67.75%	7.313%




Sum of corrected areas: 23934145

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011402.D
Acq On : 12 Aug 2022 00:16
Operator : CG/JU
Sample : N4128-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

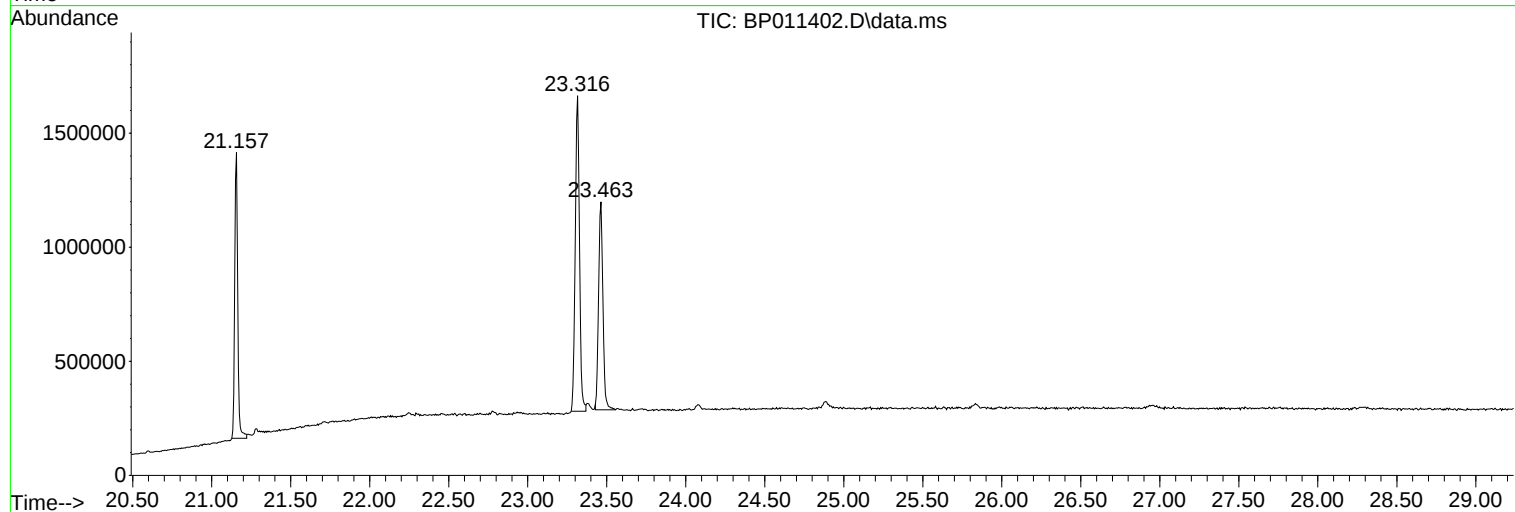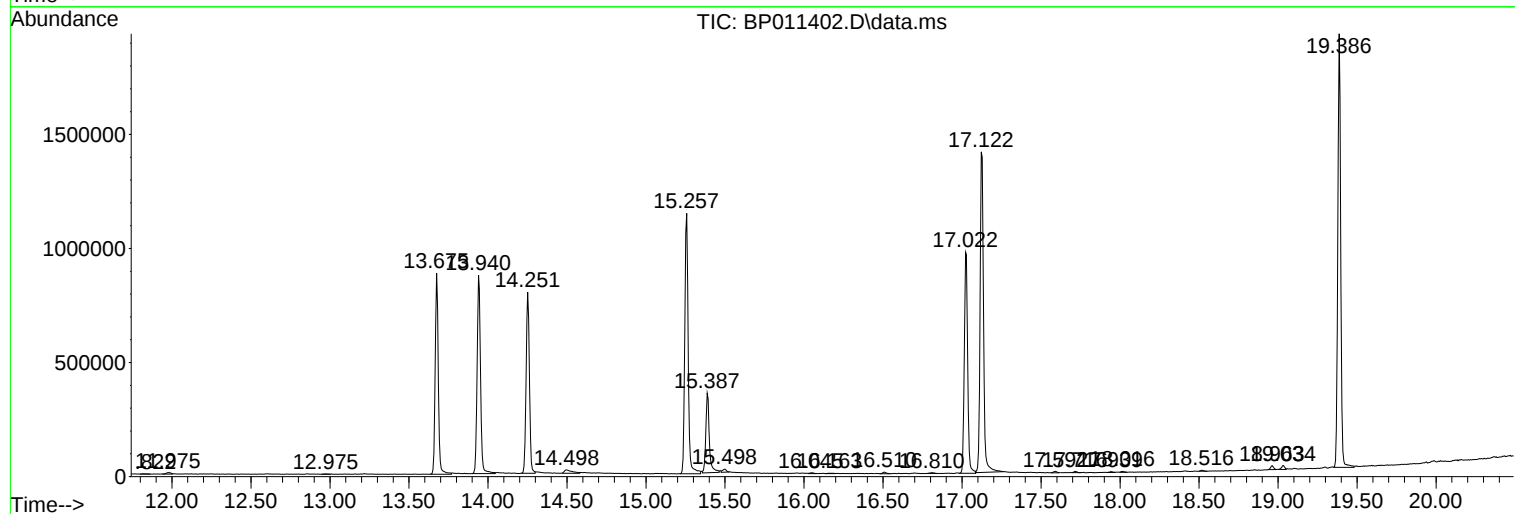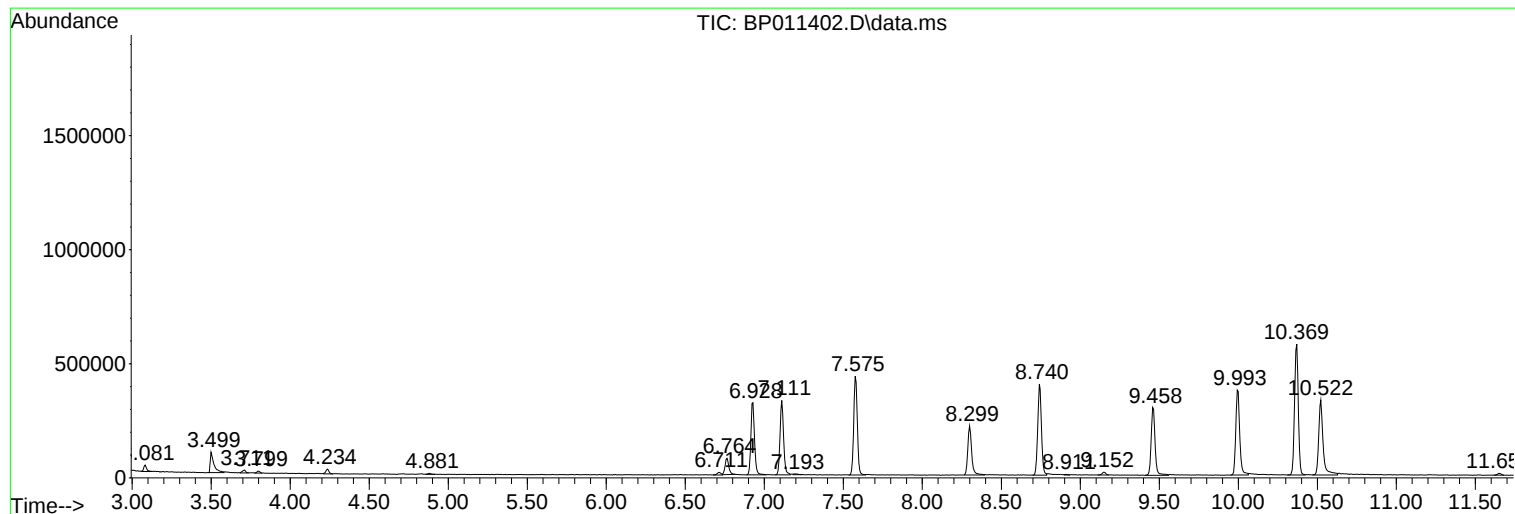

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011402.D
Acq On : 12 Aug 2022 00:16
Operator : CG/JU
Sample : N4128-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011402.D
Acq On : 12 Aug 2022 00:16
Operator : CG/JU
Sample : N4128-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc