

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011406.D
 Acq On : 12 Aug 2022 02:33
 Operator : CG/JU
 Sample : N4128-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	21	rVB	25755	31088	1.36%	0.140%
2	3.499	84	87	99	rBV	101681	164930	7.20%	0.743%
3	3.705	118	122	128	rVB	15241	22179	0.97%	0.100%
4	3.793	135	137	146	rVB2	8854	13989	0.61%	0.063%
5	4.234	208	212	216	rVB2	20055	26962	1.18%	0.121%
6	4.705	290	292	295	rBV3	2083	2359	0.10%	0.011%
7	4.822	309	312	317	rBV7	2372	3770	0.16%	0.017%
8	5.134	361	365	369	rVB6	1490	2693	0.12%	0.012%
9	6.710	628	633	636	rBV2	10669	15267	0.67%	0.069%
10	6.763	636	642	652	rVB	94737	156862	6.85%	0.707%
11	6.922	662	669	683	rBV	331712	533011	23.27%	2.401%
12	7.110	694	701	712	rBV	361492	566774	24.74%	2.553%
13	7.199	713	716	720	rVB6	4168	6235	0.27%	0.028%
14	7.575	773	780	789	rBV	368805	573316	25.03%	2.583%
15	8.299	896	903	920	rBV	261751	436794	19.07%	1.968%
16	8.740	972	978	986	rBV	427644	681248	29.74%	3.069%
17	8.875	998	1001	1007	rVB8	1594	2507	0.11%	0.011%
18	9.146	1042	1047	1055	rVB	12825	22052	0.96%	0.099%
19	9.457	1093	1100	1111	rBV	325640	528672	23.08%	2.382%
20	9.993	1184	1191	1205	rBV	419326	711420	31.06%	3.205%
21	10.363	1247	1254	1264	rBV	474141	788492	34.42%	3.552%
22	10.516	1273	1280	1297	rBV	334778	635676	27.75%	2.864%
23	11.645	1467	1472	1480	rBV2	7831	13596	0.59%	0.061%
24	11.981	1520	1529	1533	rBV5	6808	13994	0.61%	0.063%
25	12.851	1675	1677	1683	rVB6	1581	2541	0.11%	0.011%
26	13.222	1736	1740	1744	rVV5	1885	3150	0.14%	0.014%
27	13.675	1809	1817	1829	rBV	883419	1226931	53.56%	5.527%
28	13.787	1833	1836	1839	rVV5	5581	8937	0.39%	0.040%
29	13.939	1856	1862	1876	rBV	902697	1307691	57.09%	5.891%
30	14.251	1909	1915	1920	rBV	667404	948024	41.39%	4.271%
31	14.492	1950	1956	1961	rBV2	25594	56756	2.48%	0.256%
32	14.892	2021	2024	2029	rVB7	1782	2647	0.12%	0.012%
33	15.257	2078	2086	2101	rBV	1116169	1690418	73.79%	7.615%
34	15.386	2102	2108	2122	rVV	399985	584857	25.53%	2.635%
35	15.498	2123	2127	2135	rVB3	13465	26703	1.17%	0.120%
36	15.957	2199	2205	2208	rBV8	1752	3219	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011406.D
 Acq On : 12 Aug 2022 02:33
 Operator : CG/JU
 Sample : N4128-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.992	2208	2211	2217	rVV8	2486	4611	0.20%	0.021%
38	16.051	2217	2221	2227	rVB8	3664	5712	0.25%	0.026%
39	16.163	2237	2240	2244	rVB5	2680	3017	0.13%	0.014%
40	16.281	2259	2260	2266	rBV6	1475	2679	0.12%	0.012%
41	16.345	2266	2271	2276	rVV9	1964	4854	0.21%	0.022%
42	16.510	2293	2299	2306	rVB3	5582	10822	0.47%	0.049%
43	16.798	2343	2348	2354	rBV6	7850	13947	0.61%	0.063%
44	16.969	2374	2377	2380	rBV5	1949	2401	0.10%	0.011%
45	17.022	2380	2386	2397	rBV	809828	1142497	49.87%	5.147%
46	17.122	2397	2403	2428	rVB	1369462	2022325	88.28%	9.110%
47	17.545	2472	2475	2478	rBV4	5731	6881	0.30%	0.031%
48	17.592	2478	2483	2487	rVV6	5443	9448	0.41%	0.043%
49	17.716	2501	2504	2509	rVB6	3322	5469	0.24%	0.025%
50	17.945	2539	2543	2547	rBV6	4685	6646	0.29%	0.030%
51	18.016	2551	2555	2561	rVV	4161	6622	0.29%	0.030%
52	18.227	2587	2591	2596	rBV5	5271	7709	0.34%	0.035%
53	18.510	2637	2639	2644	rVB6	4004	6190	0.27%	0.028%
54	18.957	2711	2715	2721	rBV3	17087	26354	1.15%	0.119%
55	19.027	2724	2727	2733	rVB2	14995	22590	0.99%	0.102%
56	19.386	2782	2788	2797	rBV	1764955	2290727	100.00%	10.320%
57	21.157	3084	3089	3097	rBV	925344	1249738	54.56%	5.630%
58	23.310	3449	3455	3465	rBV	1242772	2275017	99.31%	10.249%
59	23.462	3474	3481	3489	rBV2	629894	1255949	54.83%	5.658%




Sum of corrected areas: 22197965

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011406.D
Acq On : 12 Aug 2022 02:33
Operator : CG/JU
Sample : N4128-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

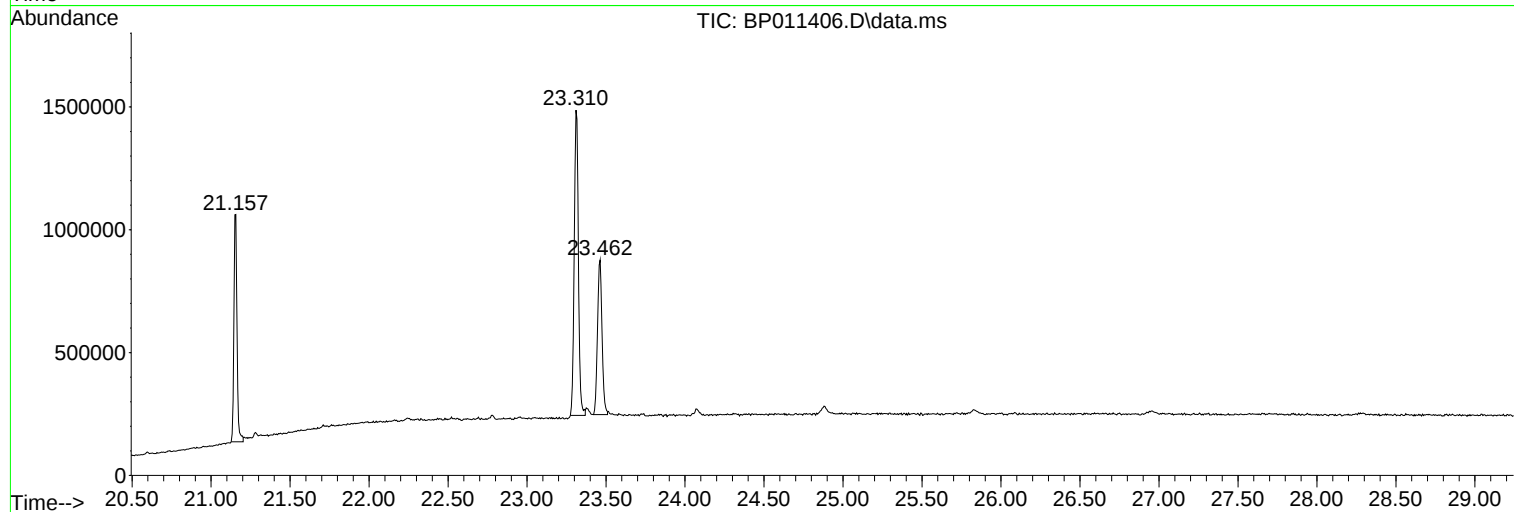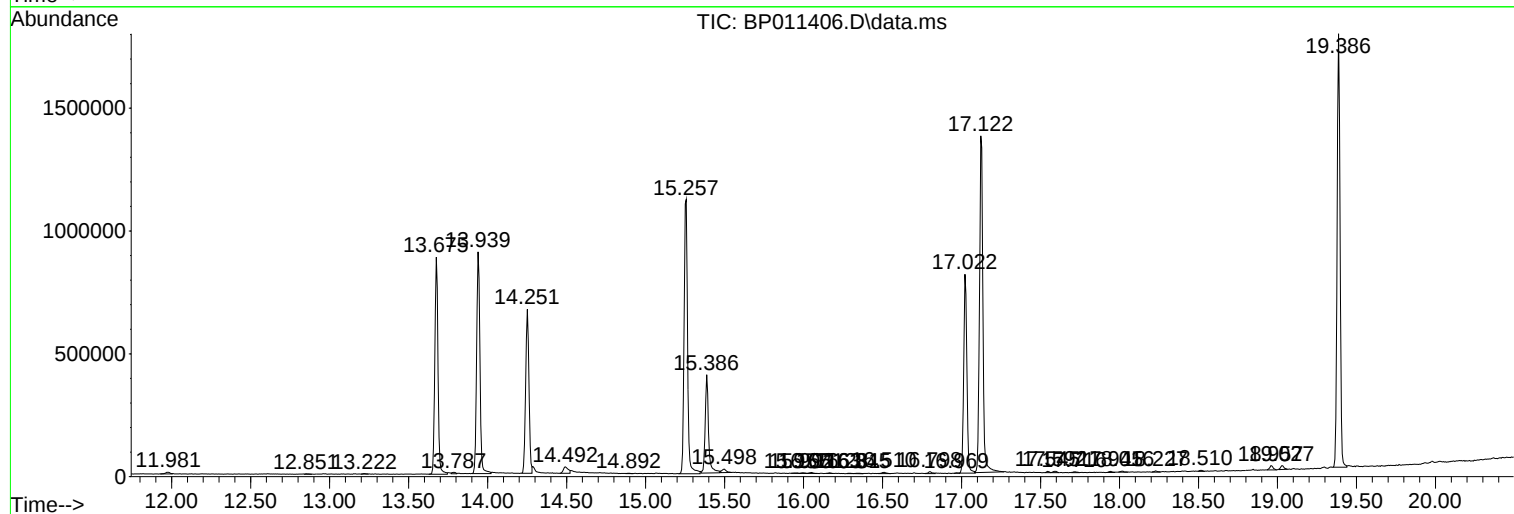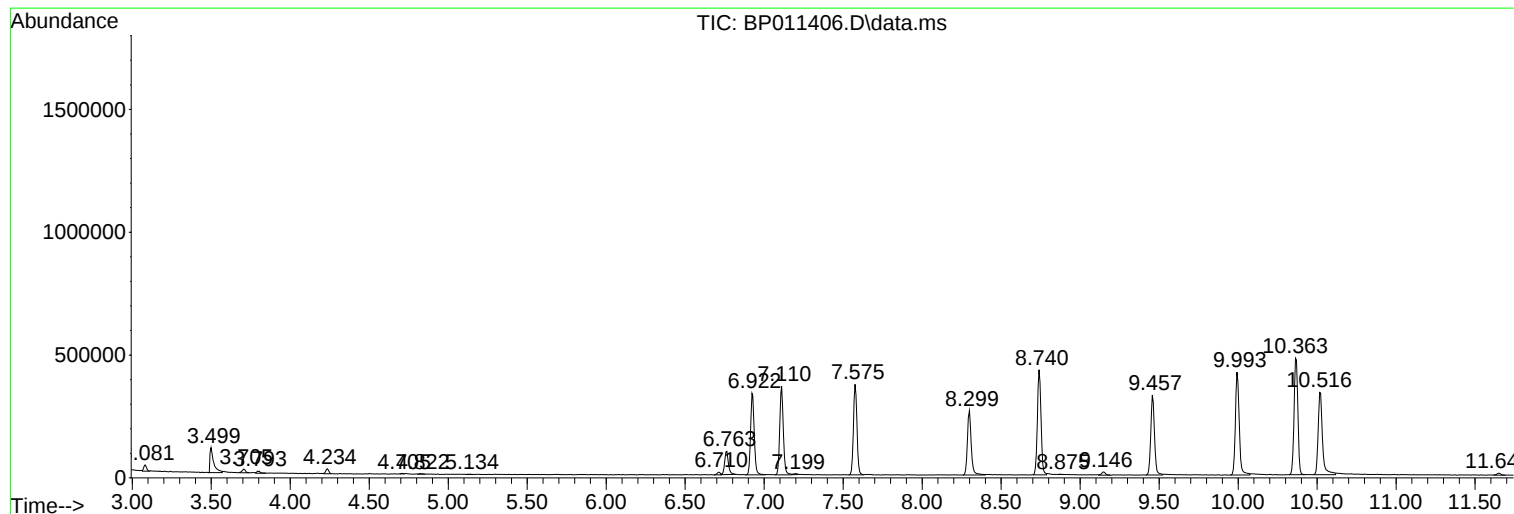

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011406.D
Acq On : 12 Aug 2022 02:33
Operator : CG/JU
Sample : N4128-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011406.D
Acq On : 12 Aug 2022 02:33
Operator : CG/JU
Sample : N4128-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc