

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011407.D
 Acq On : 12 Aug 2022 03:08
 Operator : CG/JU
 Sample : N4128-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	24	rVB	31922	38863	1.40%	0.153%
2	3.499	84	87	103	rBV	104814	170650	6.16%	0.670%
3	3.705	117	122	126	rBV	14356	21473	0.78%	0.084%
4	3.799	135	138	144	rVB	8779	11459	0.41%	0.045%
5	4.234	207	212	219	rVB	22260	30821	1.11%	0.121%
6	4.705	288	292	298	rBV5	2847	4328	0.16%	0.017%
7	4.828	309	313	317	rVB7	3190	4650	0.17%	0.018%
8	6.711	628	633	637	rBV	12384	18251	0.66%	0.072%
9	6.758	637	641	652	rVB	100345	165002	5.96%	0.647%
10	6.922	663	669	682	rBV	364898	570079	20.59%	2.237%
11	7.111	694	701	712	rBV	387784	610149	22.03%	2.394%
12	7.199	712	716	721	rVB7	4787	8000	0.29%	0.031%
13	7.575	773	780	789	rBV	434416	666728	24.08%	2.616%
14	8.299	896	903	916	rBV2	273464	459935	16.61%	1.805%
15	8.740	971	978	996	rBV	469152	759141	27.41%	2.979%
16	9.146	1042	1047	1053	rVB2	13396	21122	0.76%	0.083%
17	9.457	1092	1100	1116	rBV	362046	598441	21.61%	2.348%
18	9.993	1184	1191	1201	rBV	461529	771893	27.87%	3.029%
19	10.363	1248	1254	1265	rBV	543893	912575	32.95%	3.581%
20	10.516	1271	1280	1296	rBV	397883	734968	26.54%	2.884%
21	11.199	1391	1396	1401	rBV9	2290	5204	0.19%	0.020%
22	11.652	1468	1473	1480	rVB	9743	15404	0.56%	0.060%
23	11.969	1521	1527	1539	rBV4	7654	17844	0.64%	0.070%
24	12.851	1672	1677	1682	rBV8	2012	3404	0.12%	0.013%
25	13.157	1724	1729	1730	rBV5	2444	3237	0.12%	0.013%
26	13.216	1736	1739	1742	rBV5	2415	2951	0.11%	0.012%
27	13.675	1810	1817	1830	rBV	986007	1367187	49.37%	5.365%
28	13.940	1855	1862	1881	rBV	1027590	1482646	53.54%	5.818%
29	14.251	1903	1915	1925	rBV	768386	1119910	40.44%	4.395%
30	14.493	1949	1956	1968	rBV2	30167	87118	3.15%	0.342%
31	15.257	2079	2086	2102	rBV	1275579	1917870	69.26%	7.526%
32	15.387	2102	2108	2123	rVV	485437	687029	24.81%	2.696%
33	15.498	2123	2127	2134	rVB2	14499	24910	0.90%	0.098%
34	16.051	2217	2221	2225	rVB7	3997	5021	0.18%	0.020%
35	16.504	2295	2298	2304	rBV4	5662	8627	0.31%	0.034%
36	16.804	2345	2349	2353	rBV7	4440	7292	0.26%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011407.D
Acq On : 12 Aug 2022 03:08
Operator : CG/JU
Sample : N4128-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	16.963	2373	2376	2380	rBV6	2593	3645	0.13%	0.014%
38	17.022	2380	2386	2396	rBV	951300	1324968	47.85%	5.199%
39	17.122	2397	2403	2428	rVB	1629518	2355165	85.05%	9.242%
40	17.586	2479	2482	2485	rBV	5356	6571	0.24%	0.026%
41	17.710	2500	2503	2510	rBV8	5901	9729	0.35%	0.038%
42	17.939	2539	2542	2544	rBV4	3956	5211	0.19%	0.020%
43	18.010	2551	2554	2559	rBV	6334	7571	0.27%	0.030%
44	18.516	2637	2640	2643	rVB5	5368	7014	0.25%	0.028%
45	18.957	2711	2715	2721	rBV4	20807	32237	1.16%	0.126%
46	19.028	2724	2727	2732	rVV2	19853	25088	0.91%	0.098%
47	19.386	2782	2788	2797	rBV	2060626	2649051	95.66%	10.395%
48	21.151	3083	3088	3099	rBV	1126418	1487921	53.73%	5.839%
49	23.316	3448	3456	3464	rBV2	1444485	2769272	100.00%	10.867%
50	23.463	3474	3481	3490	rVB2	746141	1466216	52.95%	5.754%




Sum of corrected areas: 25483841

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011407.D
Acq On : 12 Aug 2022 03:08
Operator : CG/JU
Sample : N4128-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

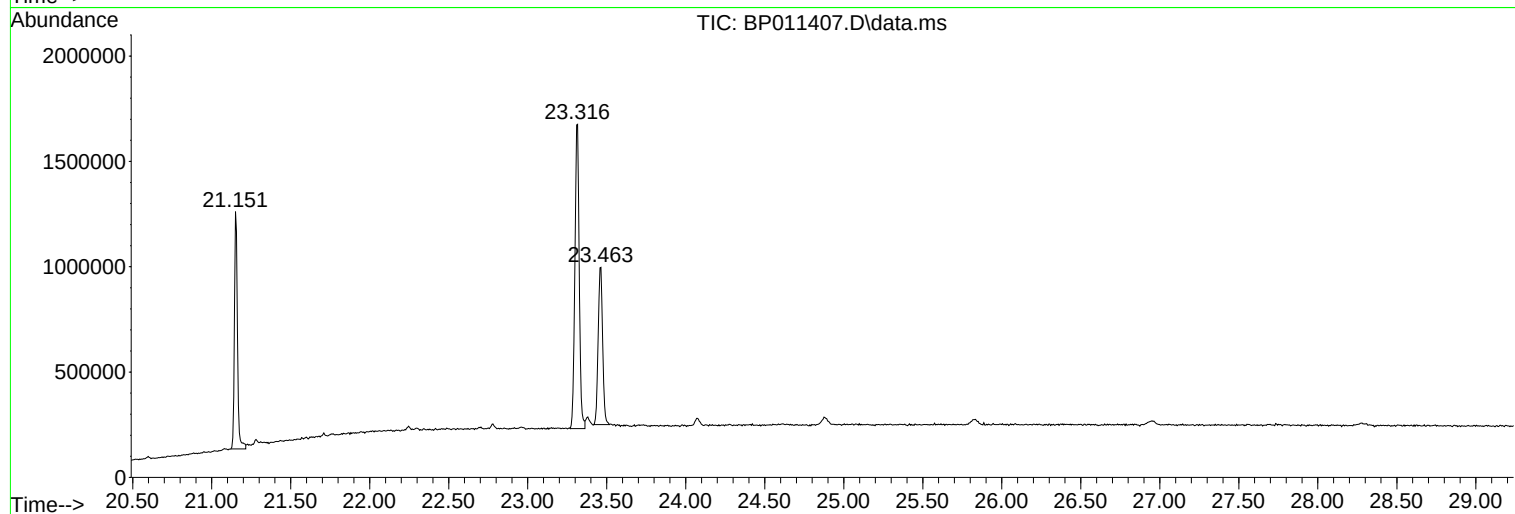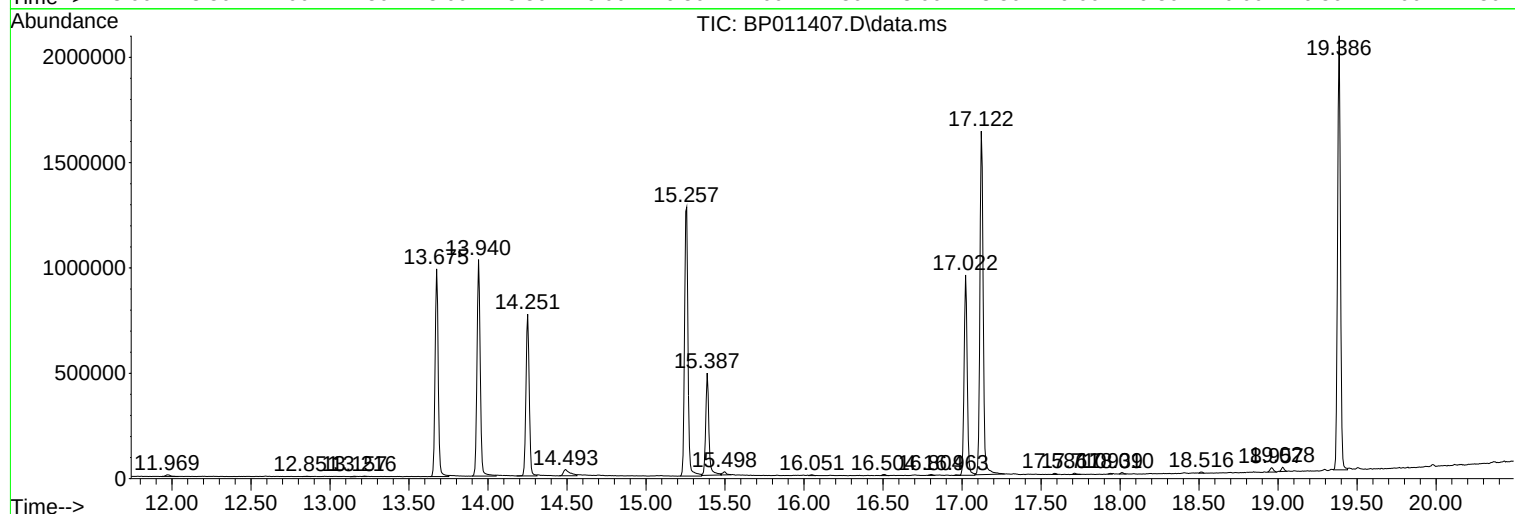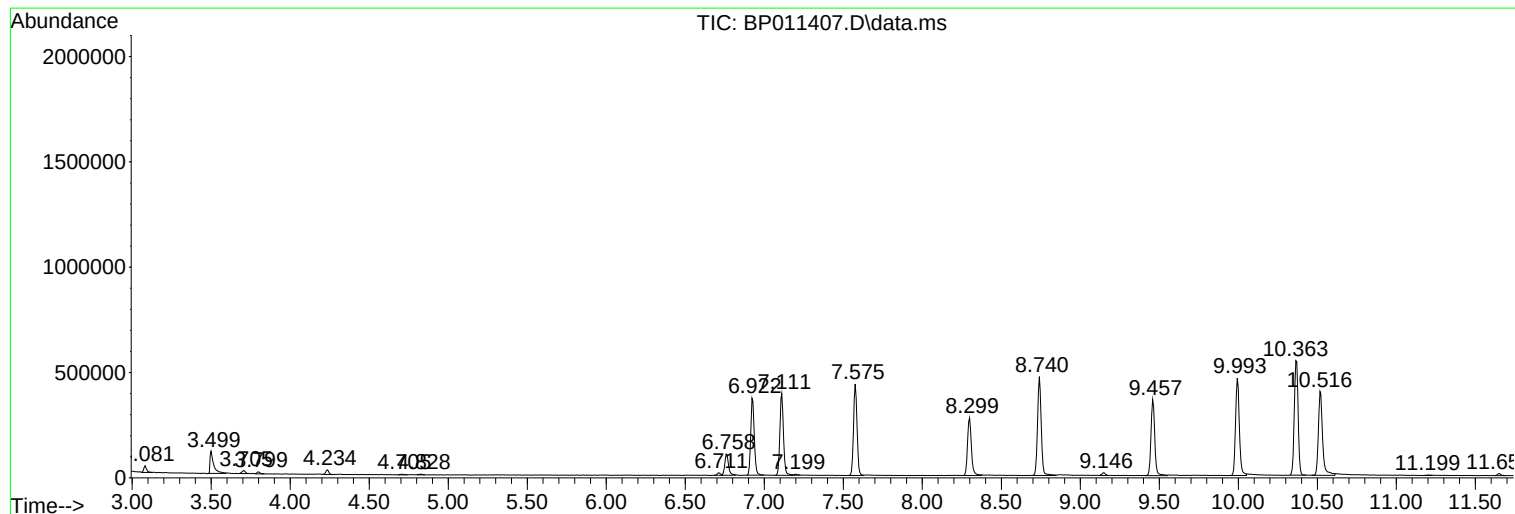

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011407.D
Acq On : 12 Aug 2022 03:08
Operator : CG/JU
Sample : N4128-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011407.D
Acq On : 12 Aug 2022 03:08
Operator : CG/JU
Sample : N4128-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------