

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011409.D
 Acq On : 12 Aug 2022 04:16
 Operator : CG/JU
 Sample : N4129-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	20	rBV	29267	31766	1.20%	0.126%
2	3.499	84	87	102	rBV	112297	179688	6.77%	0.715%
3	3.705	117	122	128	rVB	16159	23696	0.89%	0.094%
4	3.793	135	137	142	rVB2	8725	9369	0.35%	0.037%
5	4.234	208	212	217	rVB	20256	26056	0.98%	0.104%
6	4.705	289	292	295	rVB5	2219	2690	0.10%	0.011%
7	4.828	309	313	319	rVB7	4110	6329	0.24%	0.025%
8	5.722	461	465	470	rBV8	1558	3283	0.12%	0.013%
9	6.710	629	633	636	rBV2	10582	13918	0.52%	0.055%
10	6.757	636	641	653	rVB	94751	157271	5.93%	0.626%
11	6.922	663	669	679	rBV	367108	571300	21.52%	2.273%
12	7.110	693	701	713	rBV	382214	600942	22.64%	2.391%
13	7.193	713	715	725	rVB	4856	9896	0.37%	0.039%
14	7.575	773	780	791	rBV	421393	649373	24.46%	2.584%
15	8.299	896	903	916	rBV	277955	458023	17.26%	1.822%
16	8.740	971	978	986	rBV	476293	757385	28.53%	3.013%
17	8.910	1005	1007	1013	rVB7	2325	3561	0.13%	0.014%
18	9.146	1041	1047	1053	rVB3	13246	22448	0.85%	0.089%
19	9.457	1093	1100	1111	rBV	360753	579137	21.82%	2.304%
20	9.993	1184	1191	1204	rBV	465470	772044	29.09%	3.072%
21	10.363	1246	1254	1265	rBV	548318	900894	33.94%	3.584%
22	10.522	1272	1281	1298	rBV	381332	716130	26.98%	2.849%
23	11.651	1467	1473	1477	rVB2	9148	14172	0.53%	0.056%
24	11.975	1520	1528	1536	rBV4	7268	15981	0.60%	0.064%
25	12.851	1672	1677	1682	rVB9	1928	4286	0.16%	0.017%
26	13.222	1732	1740	1741	rVV7	1943	2989	0.11%	0.012%
27	13.675	1810	1817	1829	rBV	1026574	1402339	52.83%	5.579%
28	13.939	1855	1862	1881	rBV	1044352	1503059	56.63%	5.980%
29	14.251	1908	1915	1923	rBV	763492	1099287	41.41%	4.374%
30	14.492	1949	1956	1974	rBV2	27144	93025	3.50%	0.370%
31	15.257	2078	2086	2103	rBV	1283234	1929085	72.68%	7.675%
32	15.386	2103	2108	2121	rVV	461110	665478	25.07%	2.648%
33	15.498	2123	2127	2136	rVB3	16289	29417	1.11%	0.117%
34	15.992	2208	2211	2215	rVV6	2765	3755	0.14%	0.015%
35	16.045	2217	2220	2229	rVB9	6313	9263	0.35%	0.037%
36	16.510	2294	2299	2302	rBV2	5624	7790	0.29%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011409.D
 Acq On : 12 Aug 2022 04:16
 Operator : CG/JU
 Sample : N4129-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.704	2327	2332	2336	rVB8	3086	4328	0.16%	0.017%
38	16.804	2345	2349	2353	rBV6	5560	9219	0.35%	0.037%
39	16.963	2371	2376	2377	rBV5	2836	2839	0.11%	0.011%
40	17.022	2380	2386	2396	rBV	922749	1309726	49.34%	5.211%
41	17.122	2397	2403	2421	rVV	1624777	2297195	86.54%	9.139%
42	17.539	2472	2474	2478	rBV4	3765	4782	0.18%	0.019%
43	17.586	2479	2482	2488	rVB4	6581	8916	0.34%	0.035%
44	17.710	2500	2503	2508	rBV5	4384	6450	0.24%	0.026%
45	17.945	2539	2543	2546	rBV6	4619	7194	0.27%	0.029%
46	18.010	2552	2554	2558	rVB4	3160	4139	0.16%	0.016%
47	18.227	2588	2591	2597	rBV8	3840	5676	0.21%	0.023%
48	18.516	2637	2640	2645	rVB5	4414	5824	0.22%	0.023%
49	18.963	2711	2716	2722	rBV3	20017	29552	1.11%	0.118%
50	19.027	2723	2727	2733	rBV	18669	27882	1.05%	0.111%
51	19.386	2782	2788	2797	rBV	2018714	2599799	97.94%	10.343%
52	21.151	3083	3088	3099	rBV	1066840	1460780	55.03%	5.812%
53	23.310	3448	3455	3463	rBV2	1413866	2654352	100.00%	10.560%
54	23.457	3474	3480	3490	rVB2	728662	1421033	53.54%	5.654%




Sum of corrected areas: 25134811

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011409.D
Acq On : 12 Aug 2022 04:16
Operator : CG/JU
Sample : N4129-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

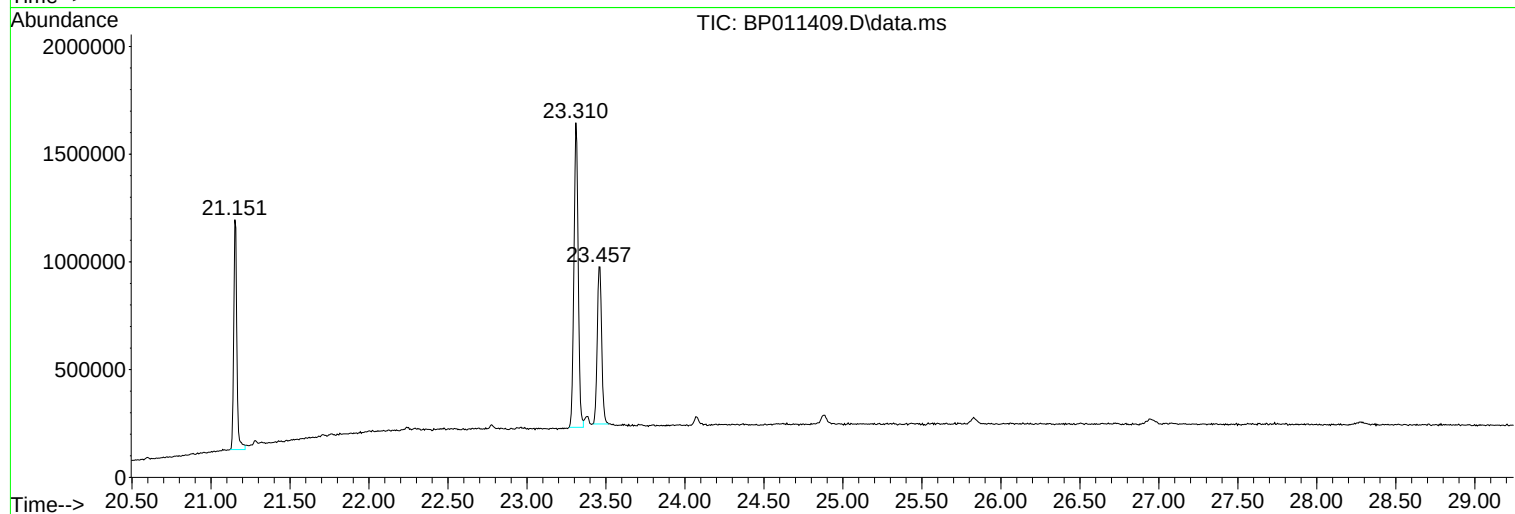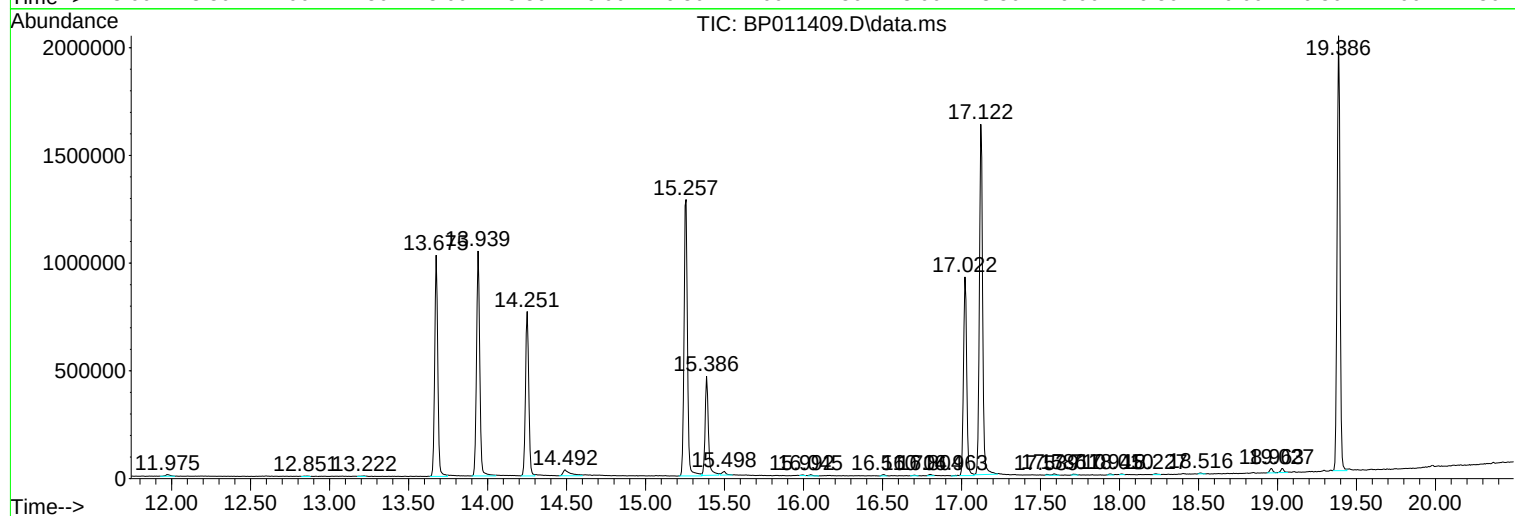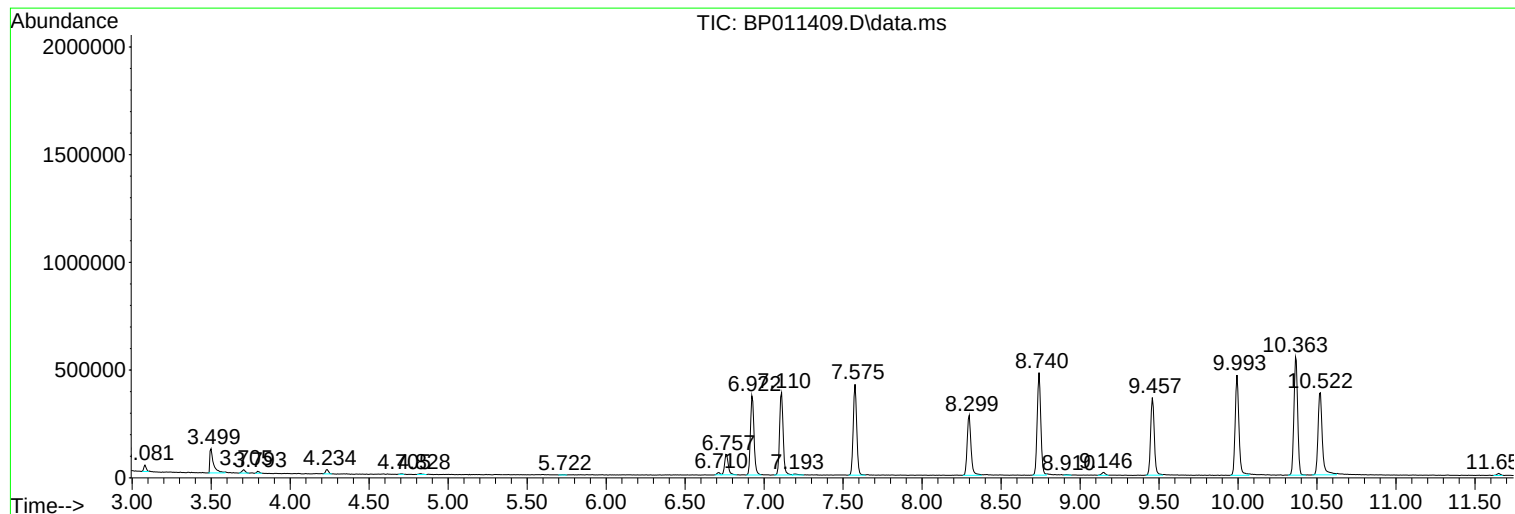

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011409.D
Acq On : 12 Aug 2022 04:16
Operator : CG/JU
Sample : N4129-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011409.D
Acq On : 12 Aug 2022 04:16
Operator : CG/JU
Sample : N4129-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc