

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011411.D
 Acq On : 12 Aug 2022 05:25
 Operator : CG/JU
 Sample : N4129-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	23	rVB	27450	34271	1.33%	0.146%
2	3.499	84	87	105	rBV	103584	169992	6.62%	0.722%
3	3.705	117	122	129	rVB	14383	21960	0.85%	0.093%
4	3.793	135	137	142	rVB3	8122	10952	0.43%	0.047%
5	4.234	207	212	218	rVB	22249	28705	1.12%	0.122%
6	4.705	289	292	297	rVB6	2463	3567	0.14%	0.015%
7	4.822	309	312	316	rBV6	3207	4217	0.16%	0.018%
8	5.299	389	393	402	rBV9	1388	4431	0.17%	0.019%
9	6.710	627	633	636	rBV	12343	17809	0.69%	0.076%
10	6.758	636	641	651	rVB	87164	143770	5.60%	0.611%
11	6.922	663	669	682	rBV	364193	563348	21.92%	2.393%
12	7.110	693	701	712	rBV	356640	576497	22.44%	2.449%
13	7.199	712	716	719	rVB4	3893	5284	0.21%	0.022%
14	7.575	773	780	790	rBV	367540	561028	21.83%	2.384%
15	8.299	896	903	913	rBV	246604	418831	16.30%	1.779%
16	8.740	971	978	993	rBV	465274	747631	29.10%	3.176%
17	9.146	1042	1047	1053	rVB2	12825	20647	0.80%	0.088%
18	9.457	1093	1100	1116	rBV	353829	581211	22.62%	2.469%
19	9.993	1184	1191	1203	rBV	451680	744227	28.96%	3.162%
20	10.363	1246	1254	1265	rBV	475027	783881	30.51%	3.330%
21	10.516	1273	1280	1291	rBV	363357	653691	25.44%	2.777%
22	11.651	1466	1473	1481	rVB3	8698	16102	0.63%	0.068%
23	11.975	1521	1528	1535	rBV3	7536	15057	0.59%	0.064%
24	13.222	1734	1740	1744	rBV8	2113	4453	0.17%	0.019%
25	13.675	1809	1817	1832	rBV	959945	1351463	52.60%	5.742%
26	13.939	1854	1862	1880	rBV	1022653	1466381	57.07%	6.230%
27	14.251	1908	1915	1924	rBV	656496	945411	36.79%	4.017%
28	14.492	1951	1956	1975	rBV3	23046	79172	3.08%	0.336%
29	15.075	2052	2055	2058	rBV4	2135	2805	0.11%	0.012%
30	15.128	2058	2064	2068	rVB9	2171	4254	0.17%	0.018%
31	15.257	2078	2086	2103	rBV	1221609	1864551	72.56%	7.922%
32	15.386	2103	2108	2122	rVV	445411	641232	24.96%	2.724%
33	15.492	2123	2126	2137	rVB2	15175	31228	1.22%	0.133%
34	16.045	2217	2220	2224	rVB5	4075	6656	0.26%	0.028%
35	16.157	2236	2239	2245	rBV8	1830	3413	0.13%	0.015%
36	16.504	2293	2298	2302	rBV4	5802	9091	0.35%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011411.D
 Acq On : 12 Aug 2022 05:25
 Operator : CG/JU
 Sample : N4129-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.698	2327	2331	2335	rBV7	2625	4331	0.17%	0.018%
38	16.810	2345	2350	2353	rBV7	4181	8174	0.32%	0.035%
39	17.022	2379	2386	2397	rBV	811232	1125205	43.79%	4.781%
40	17.122	2397	2403	2419	rVV	1548288	2179757	84.83%	9.261%
41	17.592	2479	2483	2486	rVB4	6041	7053	0.27%	0.030%
42	17.716	2501	2504	2513	rVB4	4010	7533	0.29%	0.032%
43	17.939	2538	2542	2546	rBV7	8190	10415	0.41%	0.044%
44	18.010	2550	2554	2560	rVV2	5314	7426	0.29%	0.032%
45	18.963	2711	2716	2720	rBV2	18832	26340	1.03%	0.112%
46	19.027	2723	2727	2734	rVV	18743	25952	1.01%	0.110%
47	19.339	2776	2780	2782	rBV5	7477	9387	0.37%	0.040%
48	19.386	2782	2788	2797	rBV	1953448	2527519	98.37%	10.739%
49	21.151	3083	3088	3098	rBV	974850	1260526	49.06%	5.356%
50	23.310	3448	3455	3462	rBV2	1382224	2569502	100.00%	10.917%
51	23.457	3474	3480	3492	rVB2	628587	1230285	47.88%	5.227%




Sum of corrected areas: 23536624

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011411.D
Acq On : 12 Aug 2022 05:25
Operator : CG/JU
Sample : N4129-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

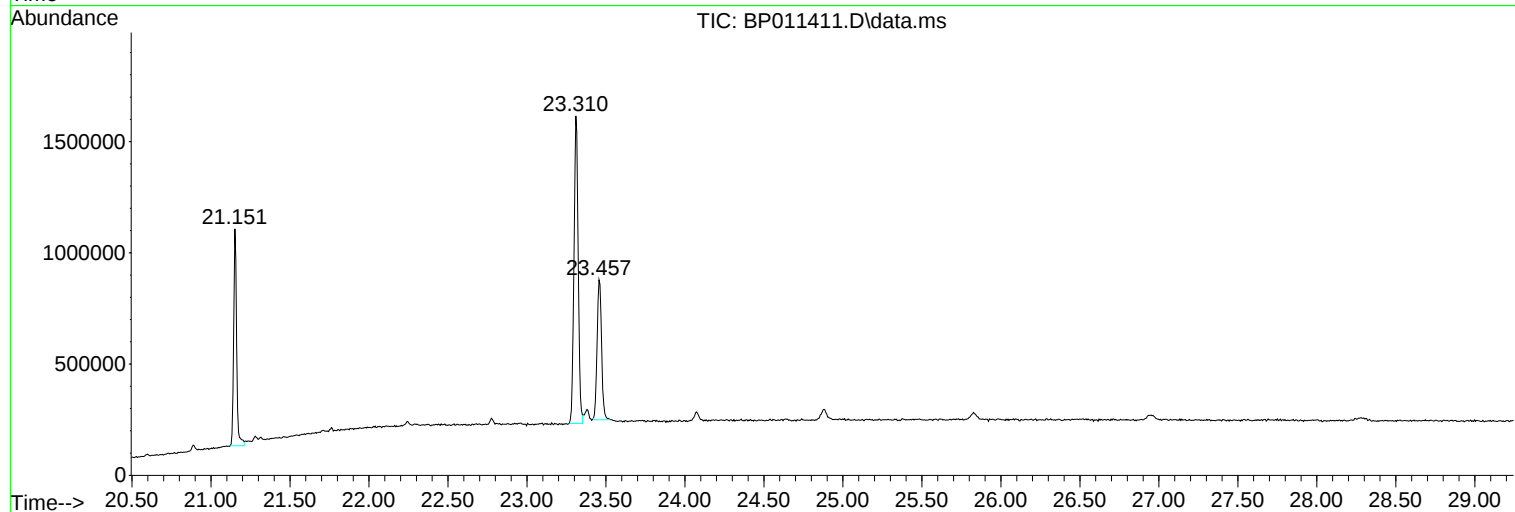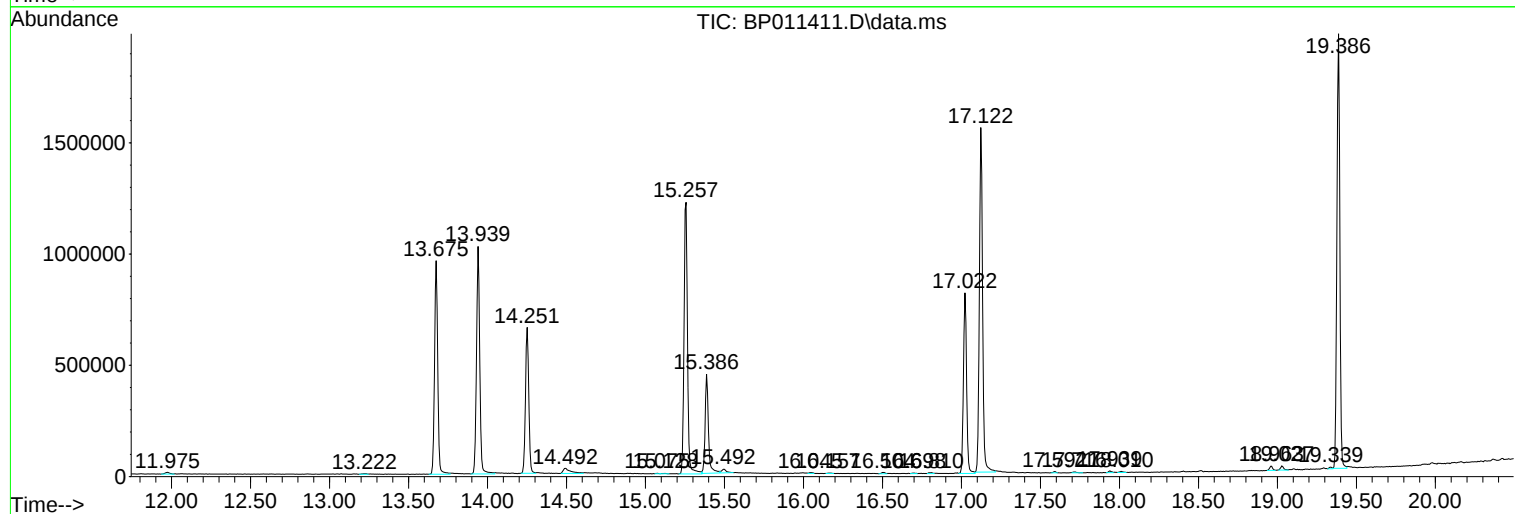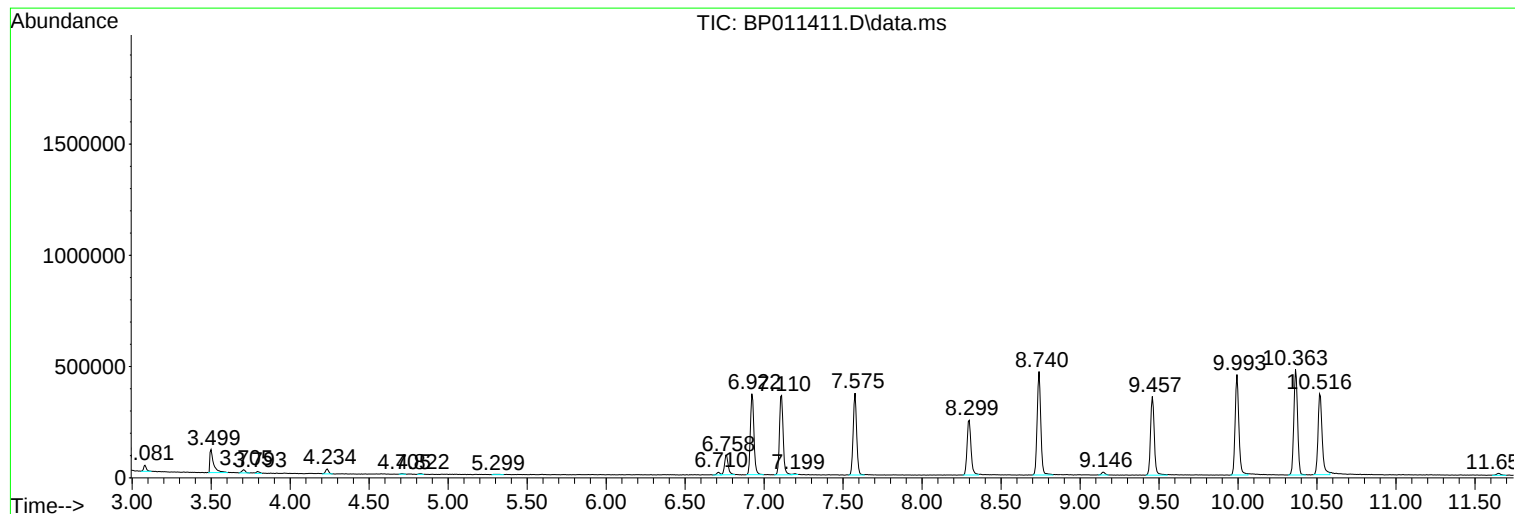

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011411.D
Acq On : 12 Aug 2022 05:25
Operator : CG/JU
Sample : N4129-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011411.D
Acq On : 12 Aug 2022 05:25
Operator : CG/JU
Sample : N4129-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc