

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011413.D
 Acq On : 12 Aug 2022 06:33
 Operator : CG/JU
 Sample : N4129-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	23	rVB	27531	35932	1.60%	0.165%
2	3.499	84	87	108	rVB	104748	177036	7.88%	0.815%
3	3.705	117	122	129	rVB	14646	24167	1.08%	0.111%
4	3.799	135	138	143	rVB3	8396	10457	0.47%	0.048%
5	4.234	207	212	218	rVB	20503	28278	1.26%	0.130%
6	4.711	290	293	297	rVB6	3818	4378	0.19%	0.020%
7	5.411	411	412	417	rBV5	1883	2837	0.13%	0.013%
8	5.593	440	443	450	rVB9	1405	2689	0.12%	0.012%
9	6.252	552	555	559	rVB5	1886	2587	0.12%	0.012%
10	6.711	628	633	636	rBV4	10163	14372	0.64%	0.066%
11	6.758	636	641	652	rVB	81093	136655	6.08%	0.629%
12	6.922	663	669	679	rBV	341552	529268	23.57%	2.436%
13	7.111	693	701	712	rBV	340038	545450	24.29%	2.510%
14	7.193	712	715	719	rVB5	3084	4183	0.19%	0.019%
15	7.575	773	780	791	rBV	352568	542172	24.14%	2.495%
16	8.299	895	903	914	rBV	233600	400185	17.82%	1.842%
17	8.740	971	978	990	rBV	435839	715459	31.86%	3.293%
18	8.910	1005	1007	1012	rVB6	1815	2462	0.11%	0.011%
19	9.146	1042	1047	1053	rVB	11338	18465	0.82%	0.085%
20	9.458	1092	1100	1119	rBV	333423	548582	24.43%	2.525%
21	9.993	1183	1191	1204	rBV	414371	699974	31.17%	3.222%
22	10.363	1247	1254	1263	rBV	456402	749065	33.35%	3.447%
23	10.516	1274	1280	1308	rBV	340600	641013	28.54%	2.950%
24	10.928	1345	1350	1352	rBV5	1631	2251	0.10%	0.010%
25	11.646	1467	1472	1478	rVB3	8134	12889	0.57%	0.059%
26	11.975	1522	1528	1535	rVB5	8142	16263	0.72%	0.075%
27	12.593	1629	1633	1639	rBV9	2486	5569	0.25%	0.026%
28	12.857	1674	1678	1681	rBV5	2908	4016	0.18%	0.018%
29	13.151	1724	1728	1731	rBV6	1811	2609	0.12%	0.012%
30	13.222	1734	1740	1745	rVB9	2309	4872	0.22%	0.022%
31	13.675	1811	1817	1832	rBV	880281	1220229	54.33%	5.616%
32	13.940	1855	1862	1875	rBV	927864	1350675	60.14%	6.216%
33	14.251	1908	1915	1924	rBV	605385	899975	40.07%	4.142%
34	14.493	1949	1956	1968	rBV4	18952	64727	2.88%	0.298%
35	15.069	2051	2054	2057	rVB4	3023	3306	0.15%	0.015%
36	15.251	2078	2085	2102	rBV	1146798	1698034	75.61%	7.815%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011413.D
 Acq On : 12 Aug 2022 06:33
 Operator : CG/JU
 Sample : N4129-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.387	2102	2108	2122	rVV	371749	548796	24.44%	2.526%
38	15.492	2123	2126	2132	rVB2	13004	21480	0.96%	0.099%
39	15.898	2190	2195	2197	rBV6	1311	2308	0.10%	0.011%
40	16.045	2216	2220	2226	rVB9	3912	6986	0.31%	0.032%
41	16.163	2235	2240	2245	rBV8	2356	4445	0.20%	0.020%
42	16.504	2294	2298	2303	rVB5	5006	6479	0.29%	0.030%
43	16.663	2321	2325	2328	rBV5	1455	2560	0.11%	0.012%
44	16.804	2345	2349	2355	rBV9	4313	6481	0.29%	0.030%
45	16.969	2374	2377	2379	rBV4	1843	2348	0.10%	0.011%
46	17.022	2380	2386	2397	rBV	738110	1067787	47.54%	4.914%
47	17.122	2397	2403	2423	rVV	1398519	1973268	87.86%	9.082%
48	17.534	2471	2473	2477	rBV5	2419	3451	0.15%	0.016%
49	17.587	2479	2482	2487	rVV6	5934	8724	0.39%	0.040%
50	17.710	2500	2503	2509	rVV7	4216	7109	0.32%	0.033%
51	17.822	2518	2522	2525	rBV6	1845	2380	0.11%	0.011%
52	17.939	2539	2542	2546	rVB5	2887	4315	0.19%	0.020%
53	18.010	2551	2554	2558	rBV2	4368	5885	0.26%	0.027%
54	18.516	2636	2640	2644	rVB5	5347	6776	0.30%	0.031%
55	18.957	2711	2715	2721	rBV4	15940	24693	1.10%	0.114%
56	19.028	2723	2727	2731	rVV	16754	22338	0.99%	0.103%
57	19.386	2782	2788	2796	rBV	1723217	2227593	99.18%	10.252%
58	21.151	3083	3088	3101	rBV	906651	1196045	53.25%	5.505%
59	23.310	3448	3455	3463	rBV2	1212321	2245912	100.00%	10.337%
60	23.457	3474	3480	3495	rVB2	591591	1208547	53.81%	5.562%




Sum of corrected areas: 21727787

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011413.D
Acq On : 12 Aug 2022 06:33
Operator : CG/JU
Sample : N4129-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

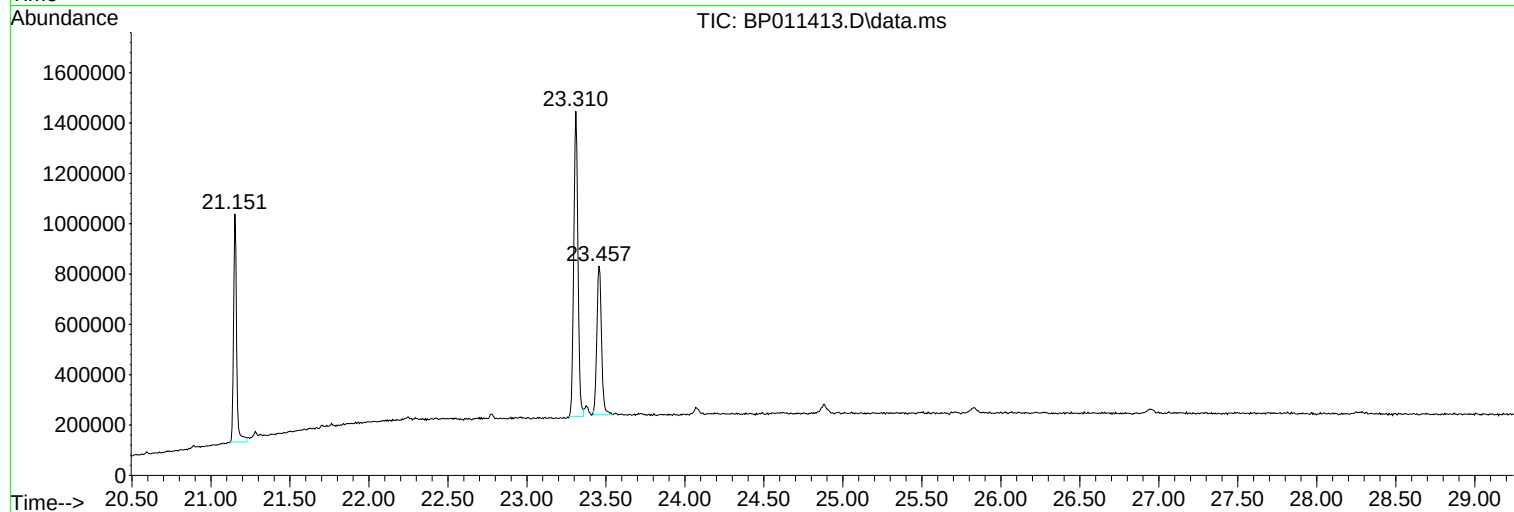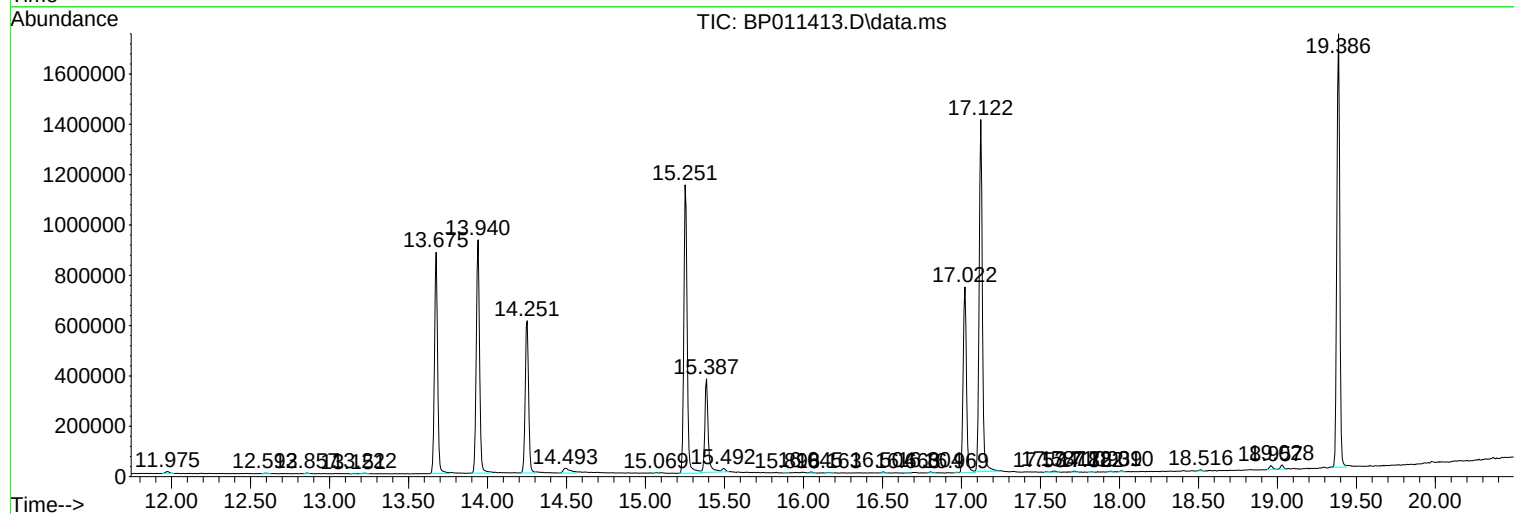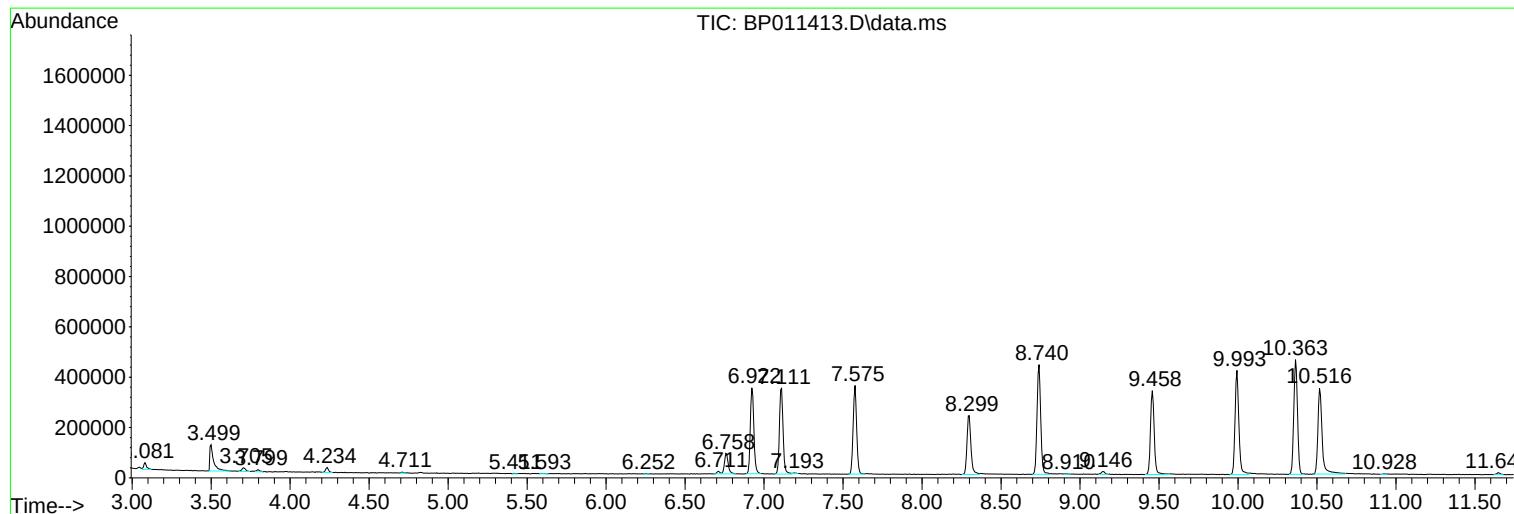

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011413.D
Acq On : 12 Aug 2022 06:33
Operator : CG/JU
Sample : N4129-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011413.D
Acq On : 12 Aug 2022 06:33
Operator : CG/JU
Sample : N4129-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc