

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011415.D
 Acq On : 12 Aug 2022 08:16
 Operator : CG/JU
 Sample : PB146917BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK917

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	20	rBV	41772	48946	1.92%	0.171%
2	3.487	83	85	104	rBV	457754	682047	26.73%	2.383%
3	3.799	134	138	142	rBV3	10688	13798	0.54%	0.048%
4	6.758	634	641	651	rBV	517271	798333	31.29%	2.789%
5	6.922	662	669	682	rVV	420390	638303	25.02%	2.230%
6	7.105	694	700	712	rBV	541767	845815	33.15%	2.955%
7	7.575	772	780	790	rBV	448800	691747	27.11%	2.417%
8	8.293	895	902	923	rBV	604294	988739	38.76%	3.455%
9	8.740	971	978	992	rBV	516304	833370	32.67%	2.912%
10	9.457	1093	1100	1121	rVV	409650	673684	26.41%	2.354%
11	9.993	1183	1191	1205	rBV	534227	923683	36.21%	3.227%
12	10.363	1246	1254	1262	rBV	599076	972376	38.11%	3.398%
13	10.516	1272	1280	1294	rBV	462911	836547	32.79%	2.923%
14	11.975	1522	1528	1534	rBV5	8255	18465	0.72%	0.065%
15	12.969	1693	1697	1700	rBV5	1708	3090	0.12%	0.011%
16	13.675	1810	1817	1828	rBV	1106449	1478117	57.94%	5.165%
17	13.940	1855	1862	1875	rBV	1112258	1581710	62.00%	5.527%
18	14.251	1908	1915	1930	rBV	831285	1215236	47.63%	4.246%
19	14.481	1947	1954	1973	rBV	322897	689402	27.02%	2.409%
20	15.251	2073	2085	2099	rBV	1352723	1972391	77.31%	6.892%
21	15.387	2102	2108	2121	rVV	498198	712617	27.93%	2.490%
22	15.492	2122	2126	2135	rVB	19553	35758	1.40%	0.125%
23	16.045	2217	2220	2227	rVB8	4361	7713	0.30%	0.027%
24	16.163	2238	2240	2250	rVB10	2553	5196	0.20%	0.018%
25	16.504	2295	2298	2305	rBV8	1775	4279	0.17%	0.015%
26	16.698	2326	2331	2335	rBV8	3073	5684	0.22%	0.020%
27	16.810	2346	2350	2355	rVB8	2946	4934	0.19%	0.017%
28	16.969	2373	2377	2380	rBV6	1753	3374	0.13%	0.012%
29	17.022	2380	2386	2397	rVV	1061633	1437819	56.36%	5.024%
30	17.122	2397	2403	2422	rVV2	1604119	2273621	89.12%	7.944%
31	17.710	2500	2503	2508	rVB6	4526	6931	0.27%	0.024%
32	18.957	2711	2715	2720	rBV2	17556	25036	0.98%	0.087%
33	19.027	2724	2727	2734	rVB2	17063	24503	0.96%	0.086%
34	19.386	2782	2788	2799	rBV	2035953	2551247	100.00%	8.914%
35	21.151	3083	3088	3098	rBV	1157400	1549870	60.75%	5.415%
36	23.310	3448	3455	3464	rBV	1355074	2526215	99.02%	8.827%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011415.D
Acq On : 12 Aug 2022 08:16
Operator : CG/JU
Sample : PB146917BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK917

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	23.457	3474	3480	3495	rVB2	797697	1539320	60.34%	5.378%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 28619916

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011415.D
Acq On : 12 Aug 2022 08:16
Operator : CG/JU
Sample : PB146917BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK917

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

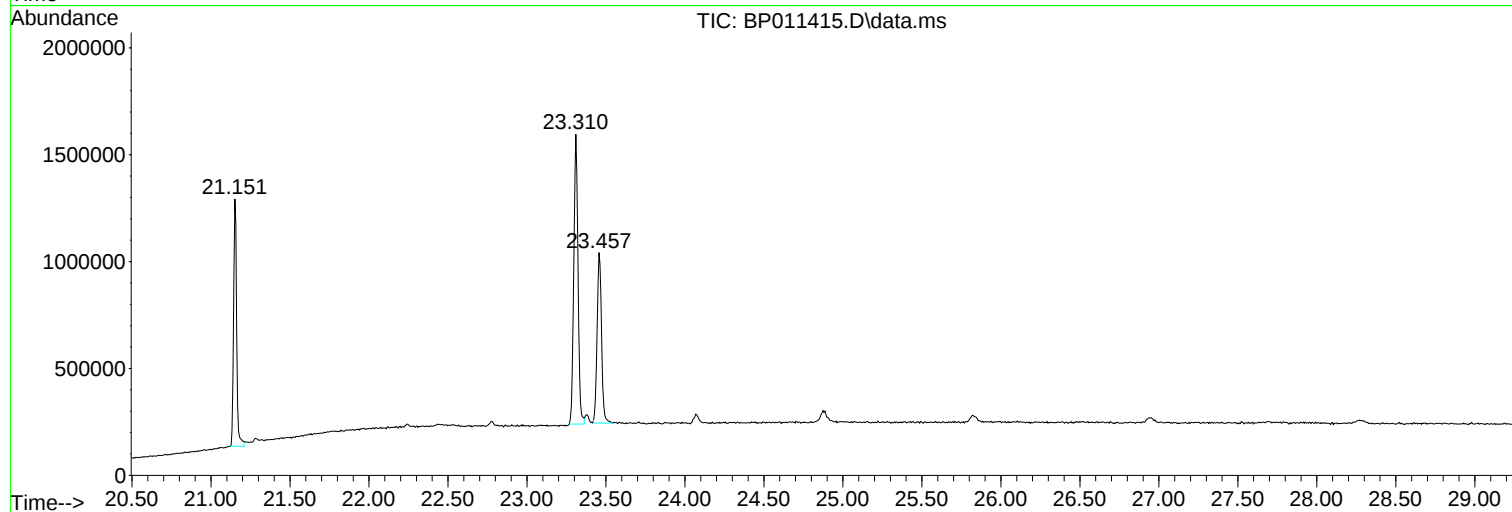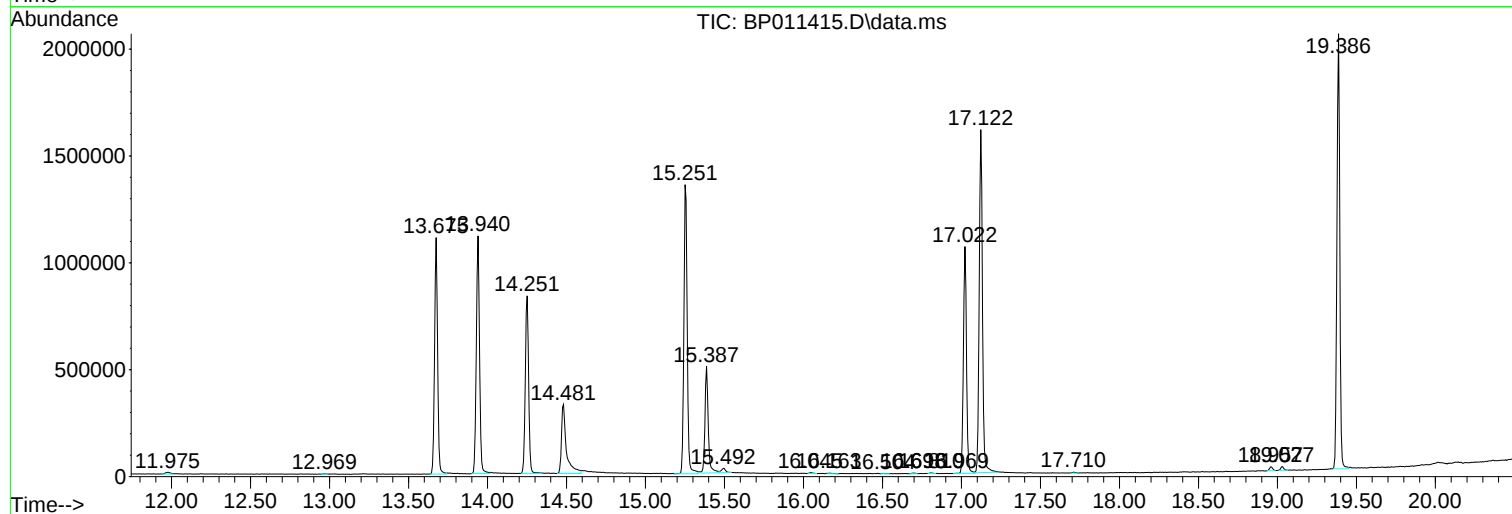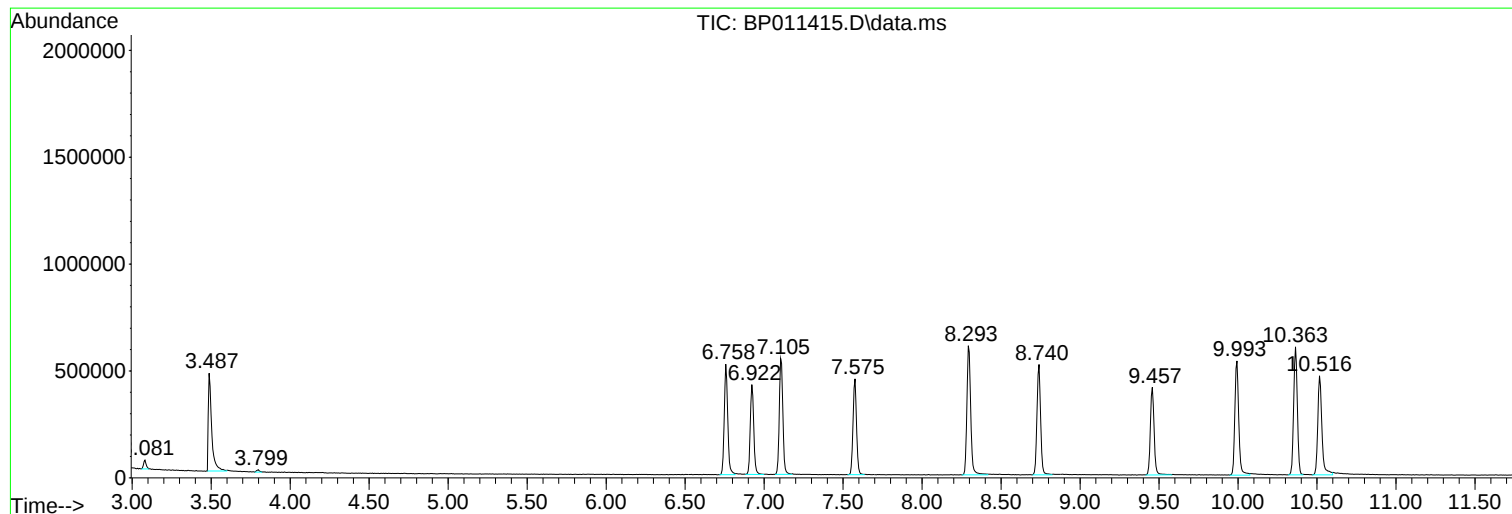

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011415.D
Acq On : 12 Aug 2022 08:16
Operator : CG/JU
Sample : PB146917BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK917

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011415.D
Acq On : 12 Aug 2022 08:16
Operator : CG/JU
Sample : PB146917BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK917

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc