

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011416.D
 Acq On : 12 Aug 2022 08:50
 Operator : CG/JU
 Sample : PB146919BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK919

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	25	rVB	38975	52250	2.50%	0.222%
2	3.487	82	85	109	rBV	422772	638744	30.53%	2.710%
3	3.793	134	137	141	rVB2	7293	9834	0.47%	0.042%
4	4.817	303	311	313	rBV9	2344	4295	0.21%	0.018%
5	6.305	561	564	567	rBV5	1527	2139	0.10%	0.009%
6	6.758	634	641	653	rBV	447538	693243	33.14%	2.941%
7	6.922	663	669	679	rBV	351550	533069	25.48%	2.262%
8	7.105	691	700	716	rBV	464812	733899	35.08%	3.114%
9	7.575	773	780	792	rVB	364735	555345	26.55%	2.356%
10	8.293	896	902	914	rBV	490075	808797	38.66%	3.432%
11	8.740	971	978	990	rBV	433751	692377	33.10%	2.938%
12	9.216	1055	1059	1062	rBV6	1402	2258	0.11%	0.010%
13	9.458	1091	1100	1112	rBV	346933	563136	26.92%	2.389%
14	9.993	1183	1191	1210	rBV	457390	798869	38.19%	3.390%
15	10.363	1247	1254	1266	rBV	481484	784421	37.50%	3.328%
16	10.516	1272	1280	1297	rBV	415859	767275	36.68%	3.256%
17	11.163	1386	1390	1394	rVB7	1561	2434	0.12%	0.010%
18	11.775	1486	1494	1496	rBV8	1555	3112	0.15%	0.013%
19	11.981	1521	1529	1537	rBV2	7927	16880	0.81%	0.072%
20	12.969	1694	1697	1700	rBV5	1749	2147	0.10%	0.009%
21	13.675	1809	1817	1830	rBV	855287	1207995	57.74%	5.126%
22	13.940	1855	1862	1875	rBV	907088	1322621	63.22%	5.612%
23	14.251	1908	1915	1926	rBV	653816	957789	45.78%	4.064%
24	14.481	1945	1954	1973	rBV	234490	530790	25.37%	2.252%
25	15.251	2077	2085	2100	rBV	1109613	1625586	77.70%	6.897%
26	15.387	2102	2108	2121	rVV	379889	556500	26.60%	2.361%
27	15.493	2123	2126	2137	rVB2	13355	25440	1.22%	0.108%
28	16.051	2217	2221	2226	rVB8	4238	7822	0.37%	0.033%
29	16.657	2321	2324	2328	rBV6	1548	2742	0.13%	0.012%
30	16.698	2328	2331	2336	rVV7	2564	4359	0.21%	0.018%
31	16.810	2347	2350	2354	rBV6	2414	3650	0.17%	0.015%
32	17.022	2379	2386	2397	rBV	820880	1141780	54.58%	4.845%
33	17.122	2397	2403	2423	rVB	1303429	1841967	88.05%	7.815%
34	17.716	2500	2504	2511	rBV10	3170	5366	0.26%	0.023%
35	18.510	2638	2639	2643	rBV4	2792	2687	0.13%	0.011%
36	18.775	2682	2684	2687	rBV4	2057	2892	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011416.D
Acq On : 12 Aug 2022 08:50
Operator : CG/JU
Sample : PB146919BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK919

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	18.957	2711	2715	2721	rBV4	14405	21771	1.04%	0.092%
38	19.034	2724	2728	2734	rVV	14219	20230	0.97%	0.086%
39	19.386	2782	2788	2804	rBV	1639799	2092065	100.00%	8.877%
40	21.151	3084	3088	3099	rBV	930069	1203138	57.51%	5.105%
41	23.310	3449	3455	3464	rBV2	1127983	2059568	98.45%	8.739%
42	23.457	3474	3480	3492	rVB2	637837	1267037	60.56%	5.376%




Sum of corrected areas: 23568319

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011416.D
Acq On : 12 Aug 2022 08:50
Operator : CG/JU
Sample : PB146919BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

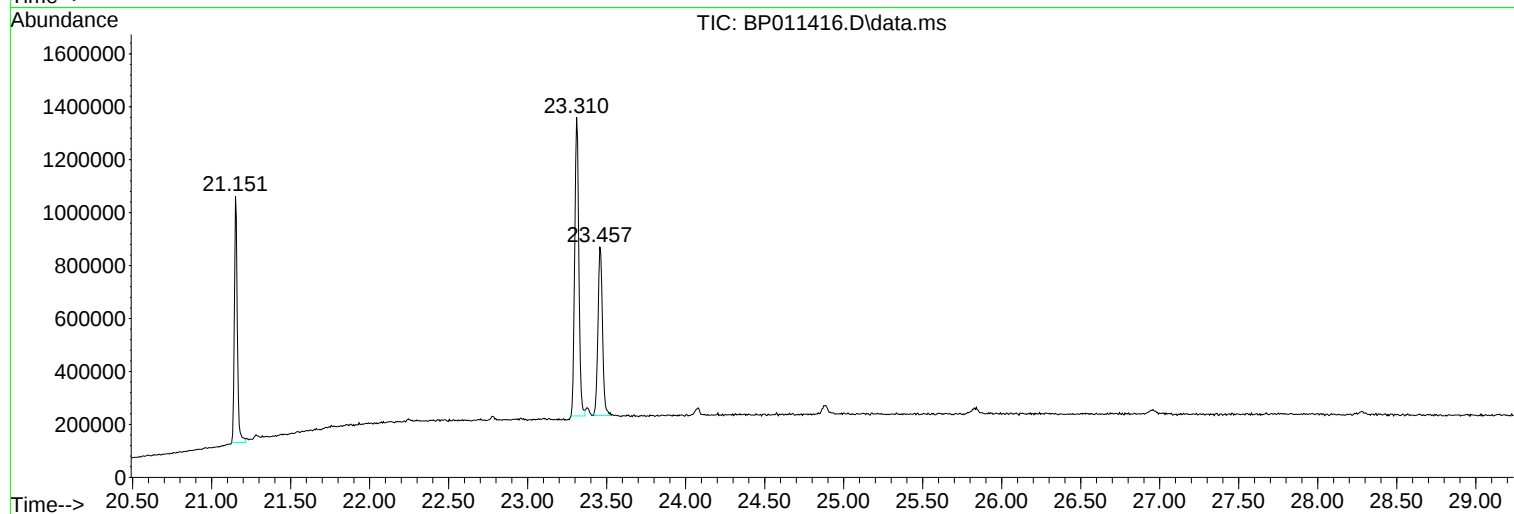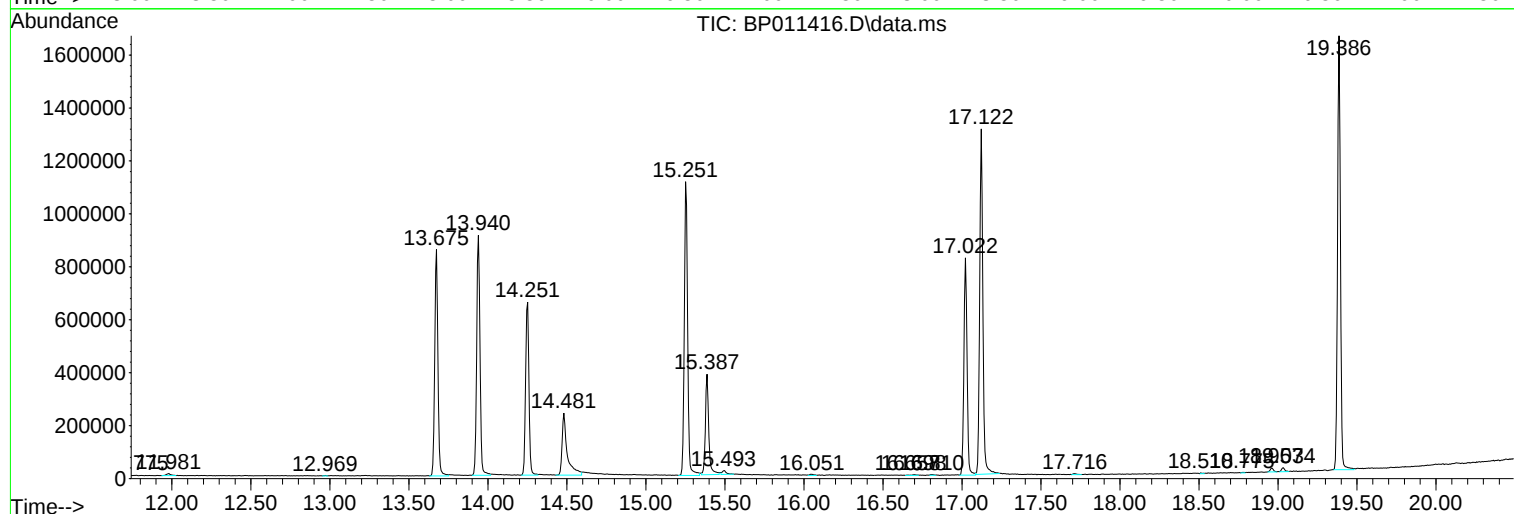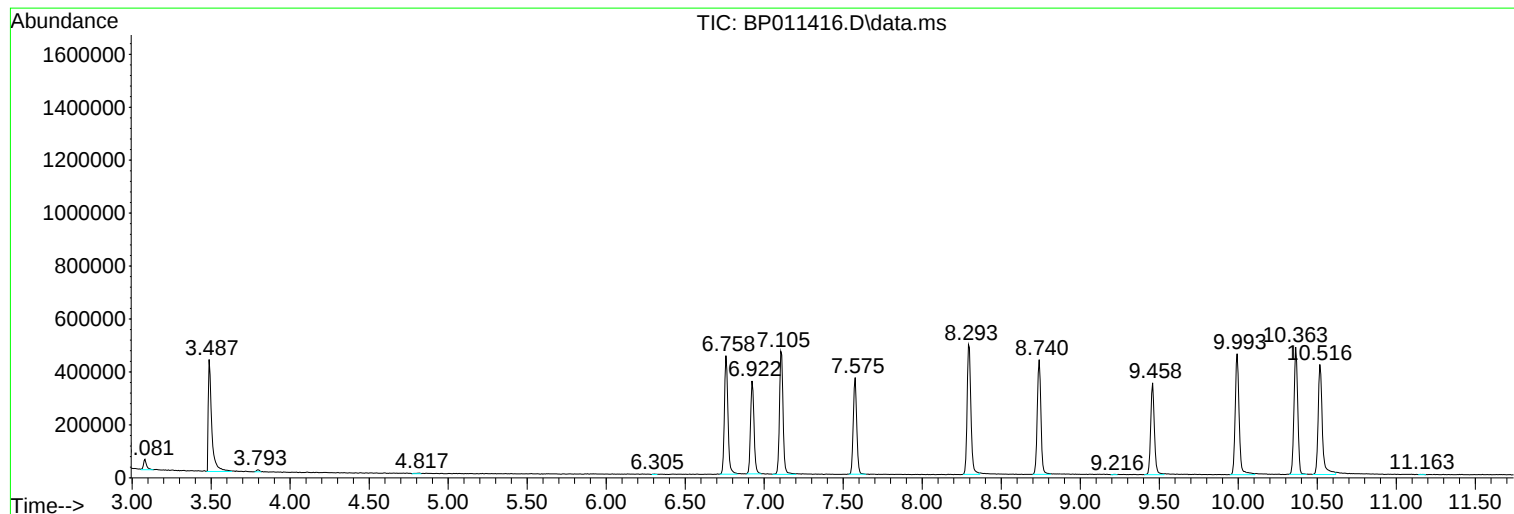

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011416.D
Acq On : 12 Aug 2022 08:50
Operator : CG/JU
Sample : PB146919BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011416.D
Acq On : 12 Aug 2022 08:50
Operator : CG/JU
Sample : PB146919BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK919

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc