

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011417.D
 Acq On : 12 Aug 2022 10:38
 Operator : CG/JU
 Sample : PB146934BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK934

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	26	rVB	43238	63468	3.08%	0.257%
2	3.487	82	85	109	rBV	455512	677286	32.91%	2.741%
3	3.799	134	138	147	rVB	10631	16800	0.82%	0.068%
4	5.728	463	466	470	rVB5	1572	2211	0.11%	0.009%
5	6.758	635	641	659	rBV	442496	713748	34.68%	2.888%
6	6.928	663	670	685	rVB	346239	545127	26.48%	2.206%
7	7.111	694	701	712	rBV	475495	734216	35.67%	2.971%
8	7.575	773	780	792	rBV	436775	683711	33.22%	2.767%
9	8.299	893	903	916	rBV	507341	827886	40.22%	3.350%
10	8.387	916	918	922	rVB5	2048	2636	0.13%	0.011%
11	8.740	970	978	992	rBV	430558	707655	34.38%	2.864%
12	8.875	998	1001	1005	rBV6	1336	2274	0.11%	0.009%
13	9.458	1094	1100	1110	rBV	334487	562230	27.32%	2.275%
14	9.993	1184	1191	1208	rBV	455784	790852	38.42%	3.200%
15	10.369	1245	1255	1266	rBV	569928	946171	45.97%	3.829%
16	10.522	1274	1281	1303	rBV	413392	786540	38.21%	3.183%
17	10.999	1359	1362	1366	rVB5	1629	2079	0.10%	0.008%
18	11.981	1524	1529	1537	rBV5	7120	16378	0.80%	0.066%
19	12.587	1628	1632	1640	rBV9	1509	3505	0.17%	0.014%
20	13.228	1734	1741	1744	rBV8	1530	3121	0.15%	0.013%
21	13.675	1811	1817	1831	rBV	813907	1180240	57.34%	4.776%
22	13.946	1855	1863	1878	rBV	884289	1296859	63.01%	5.248%
23	14.251	1908	1915	1928	rBV	774431	1149516	55.85%	4.652%
24	14.481	1948	1954	1985	rBV	223777	546217	26.54%	2.210%
25	15.257	2079	2086	2102	rBV	1116514	1596432	77.56%	6.460%
26	15.393	2103	2109	2122	rVV	352244	529713	25.74%	2.144%
27	15.498	2124	2127	2132	rVB3	11263	18803	0.91%	0.076%
28	15.822	2180	2182	2188	rVB7	1232	2062	0.10%	0.008%
29	16.051	2217	2221	2229	rVB10	2979	5291	0.26%	0.021%
30	16.816	2348	2351	2355	rVB6	1908	2299	0.11%	0.009%
31	17.028	2380	2387	2398	rBV	967908	1356057	65.88%	5.487%
32	17.128	2398	2404	2420	rVV	1256992	1798043	87.36%	7.276%
33	17.722	2501	2505	2510	rVB8	2235	4449	0.22%	0.018%
34	18.963	2712	2716	2721	rBV5	13108	19978	0.97%	0.081%
35	19.034	2725	2728	2733	rBV	12583	17435	0.85%	0.071%
36	19.392	2783	2789	2797	rBV	1572085	2006804	97.50%	8.121%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011417.D
Acq On : 12 Aug 2022 10:38
Operator : CG/JU
Sample : PB146934BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	21.157	3084	3089	3100	rBV	1136503	1491355	72.46%	6.035%
38	23.316	3450	3456	3465	rBV2	1077998	2058259	100.00%	8.329%
39	23.469	3476	3482	3498	rVB2	796675	1544715	75.05%	6.251%




Sum of corrected areas: 24712421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011417.D
Acq On : 12 Aug 2022 10:38
Operator : CG/JU
Sample : PB146934BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

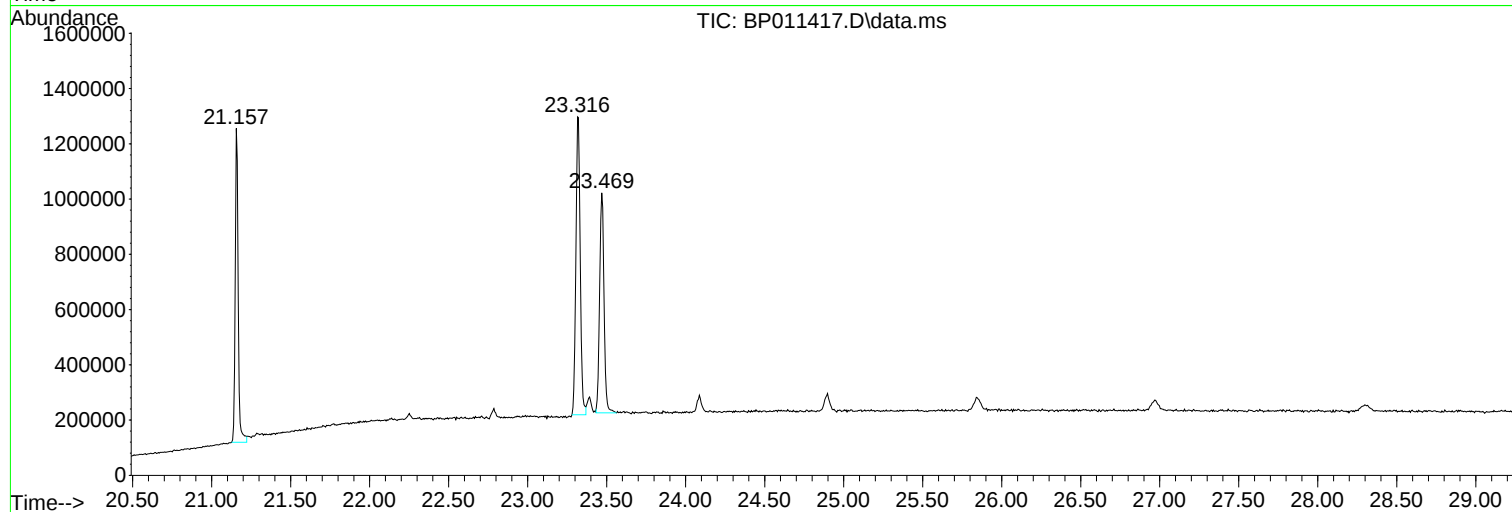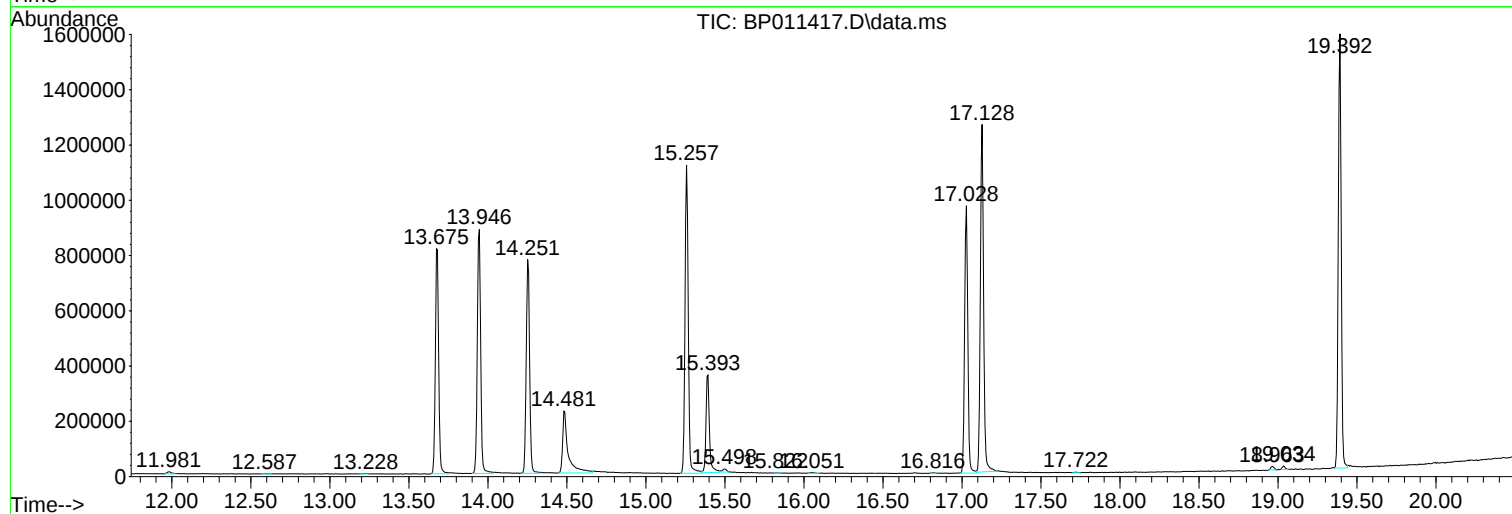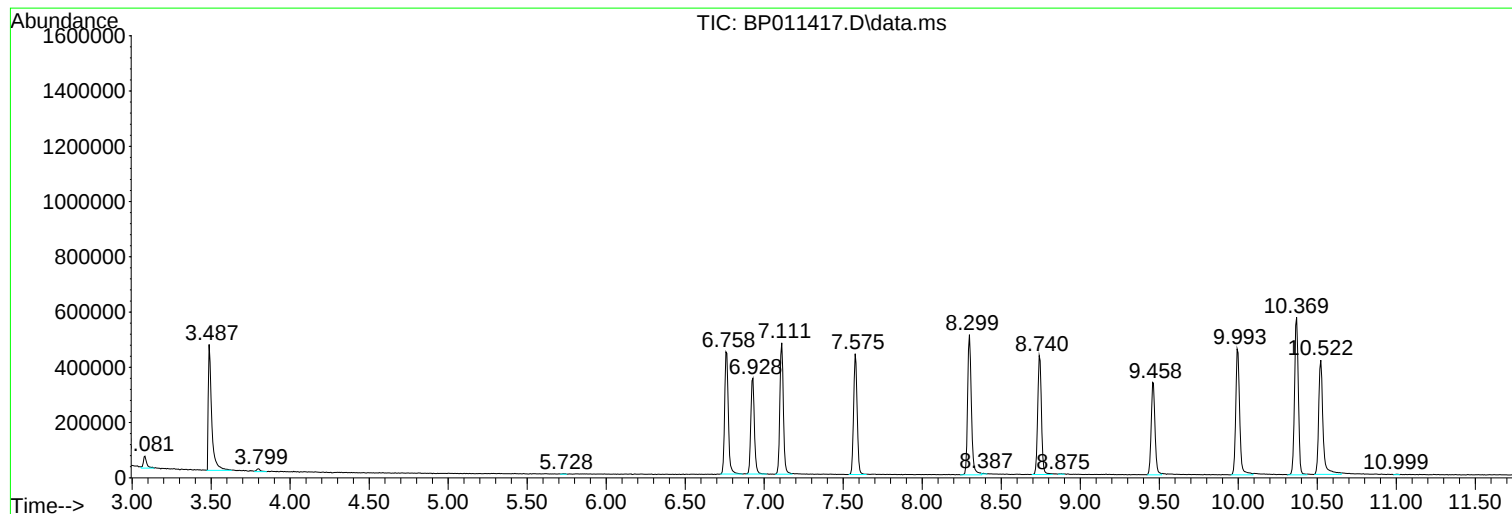

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011417.D
Acq On : 12 Aug 2022 10:38
Operator : CG/JU
Sample : PB146934BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011417.D
Acq On : 12 Aug 2022 10:38
Operator : CG/JU
Sample : PB146934BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK934

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc