

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011418.D
 Acq On : 12 Aug 2022 11:12
 Operator : CG/JU
 Sample : N4129-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	25	rBV	30342	38962	1.55%	0.173%
2	3.493	84	86	105	rBV	130753	205862	8.18%	0.912%
3	3.705	118	122	127	rVB	15918	23234	0.92%	0.103%
4	3.793	135	137	143	rVB3	8711	10244	0.41%	0.045%
5	4.234	208	212	217	rVB	17073	24123	0.96%	0.107%
6	4.581	267	271	274	rBV6	2396	3475	0.14%	0.015%
7	4.711	289	293	296	rBV5	2718	3970	0.16%	0.018%
8	6.710	628	633	636	rBV2	9726	13940	0.55%	0.062%
9	6.758	636	641	653	rVB	83533	137259	5.46%	0.608%
10	6.922	663	669	683	rBV	348478	536055	21.31%	2.374%
11	7.110	693	701	710	rBV	341026	540507	21.49%	2.393%
12	7.199	713	716	720	rVB6	3348	5206	0.21%	0.023%
13	7.575	772	780	791	rBV	326750	501674	19.94%	2.221%
14	8.293	892	902	916	rBV	233863	402605	16.00%	1.783%
15	8.740	970	978	991	rBV	442788	717846	28.54%	3.179%
16	8.869	998	1000	1006	rVB7	2107	2567	0.10%	0.011%
17	9.146	1042	1047	1053	rVB2	11815	18743	0.75%	0.083%
18	9.457	1093	1100	1116	rBV	336121	550278	21.88%	2.437%
19	9.993	1181	1191	1206	rBV	428851	723191	28.75%	3.202%
20	10.363	1247	1254	1263	rBV	432477	698730	27.78%	3.094%
21	10.516	1272	1280	1293	rBV	384255	714725	28.41%	3.165%
22	11.645	1468	1472	1478	rVB3	7996	12195	0.48%	0.054%
23	11.975	1523	1528	1535	rBV4	7251	14520	0.58%	0.064%
24	12.863	1674	1679	1685	rVB9	1490	2904	0.12%	0.013%
25	13.163	1723	1730	1733	rVB9	1911	4118	0.16%	0.018%
26	13.216	1733	1739	1743	rBV9	1926	4163	0.17%	0.018%
27	13.675	1811	1817	1829	rBV	942382	1301421	51.74%	5.763%
28	13.939	1855	1862	1879	rBV	988550	1420236	56.46%	6.289%
29	14.251	1908	1915	1927	rBV	577652	853259	33.92%	3.778%
30	14.492	1951	1956	1969	rBV3	18170	57994	2.31%	0.257%
31	15.257	2079	2086	2102	rBV	1228792	1813359	72.09%	8.030%
32	15.386	2102	2108	2123	rVV	405258	603908	24.01%	2.674%
33	15.498	2123	2127	2138	rVB4	15692	31768	1.26%	0.141%
34	16.045	2218	2220	2228	rVB8	4242	5983	0.24%	0.026%
35	16.510	2296	2299	2303	rVB3	4928	6340	0.25%	0.028%
36	16.692	2328	2330	2336	rBV7	2851	4749	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011418.D
 Acq On : 12 Aug 2022 11:12
 Operator : CG/JU
 Sample : N4129-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.804	2346	2349	2357	rVB10	2287	4547	0.18%	0.020%
38	16.975	2374	2378	2380	rBV5	2119	2676	0.11%	0.012%
39	17.022	2380	2386	2396	rVV	718091	1013903	40.31%	4.490%
40	17.122	2397	2403	2419	rVV	1486076	2182081	86.75%	9.662%
41	17.239	2420	2423	2428	rVB7	8698	16149	0.64%	0.072%
42	17.422	2451	2454	2457	rBV5	2568	3294	0.13%	0.015%
43	17.586	2479	2482	2489	rVB6	5528	7175	0.29%	0.032%
44	17.722	2503	2505	2508	rVB4	2800	3268	0.13%	0.014%
45	18.016	2552	2555	2560	rBV3	2745	3724	0.15%	0.016%
46	18.410	2620	2622	2626	rVB5	2729	2632	0.10%	0.012%
47	18.963	2712	2716	2721	rVB3	17195	23587	0.94%	0.104%
48	19.033	2723	2728	2737	rVV	16891	26519	1.05%	0.117%
49	19.339	2776	2780	2782	rBV5	7099	8980	0.36%	0.040%
50	19.386	2782	2788	2798	rBV	1921305	2482574	98.69%	10.993%
51	21.157	3084	3089	3098	rBV	845524	1138559	45.26%	5.042%
52	23.315	3449	3456	3463	rBV2	1370090	2515499	100.00%	11.139%
53	23.463	3475	3481	3494	rVB2	588224	1138266	45.25%	5.040%




Sum of corrected areas: 22583546

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011418.D
Acq On : 12 Aug 2022 11:12
Operator : CG/JU
Sample : N4129-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

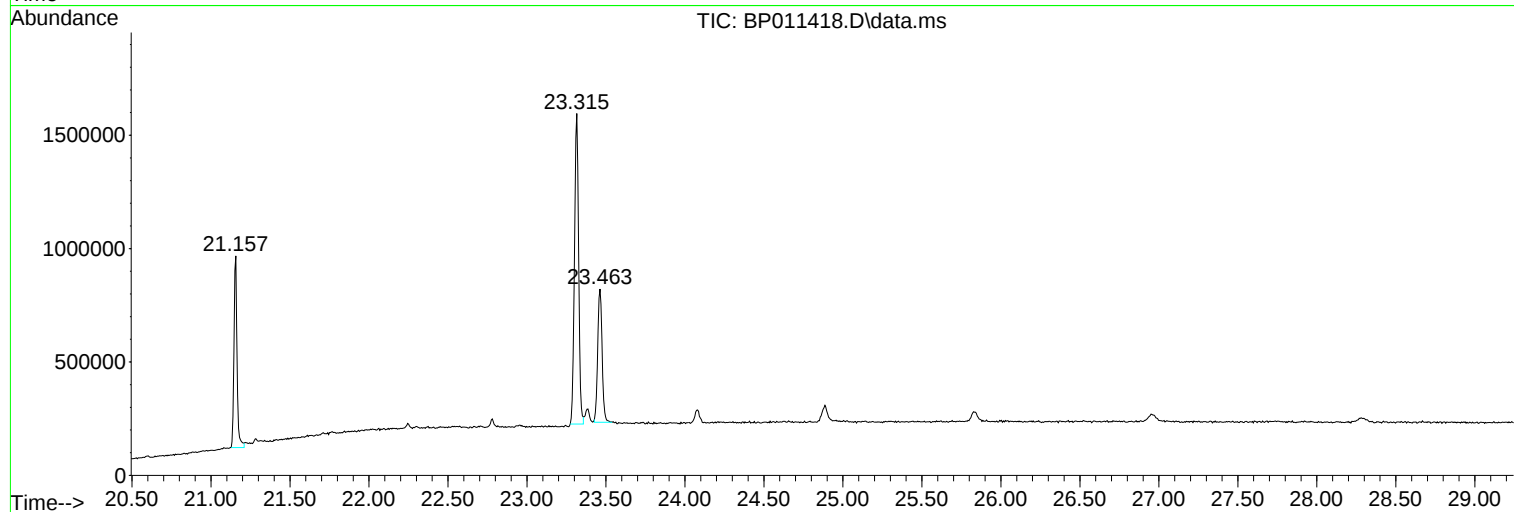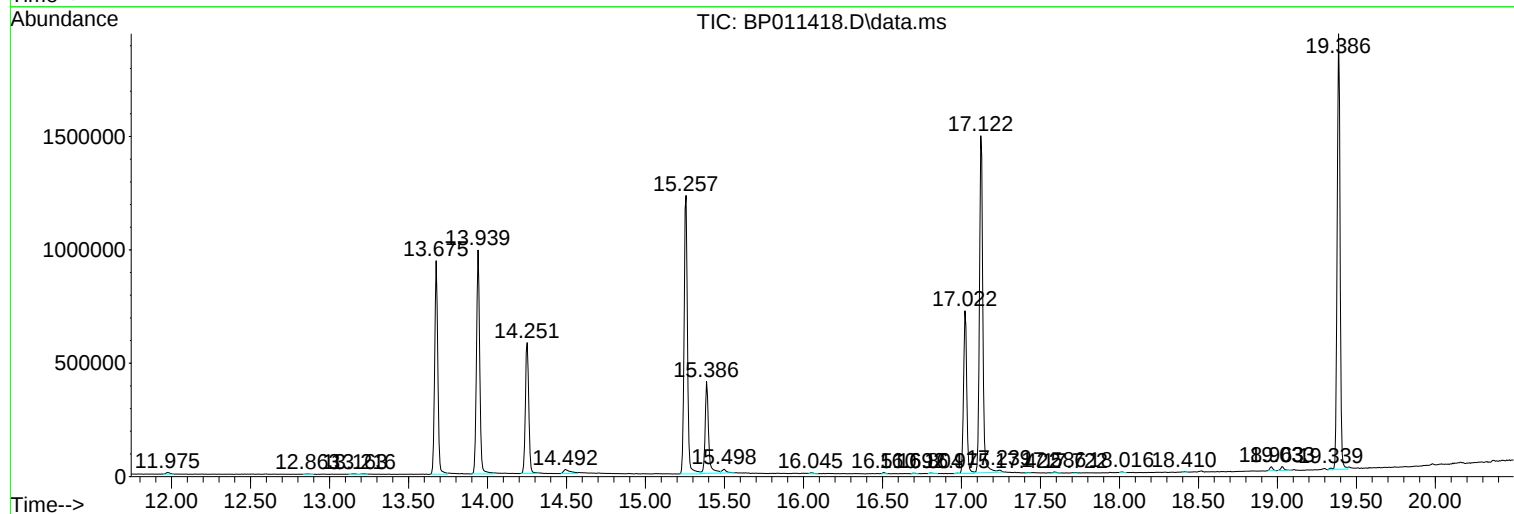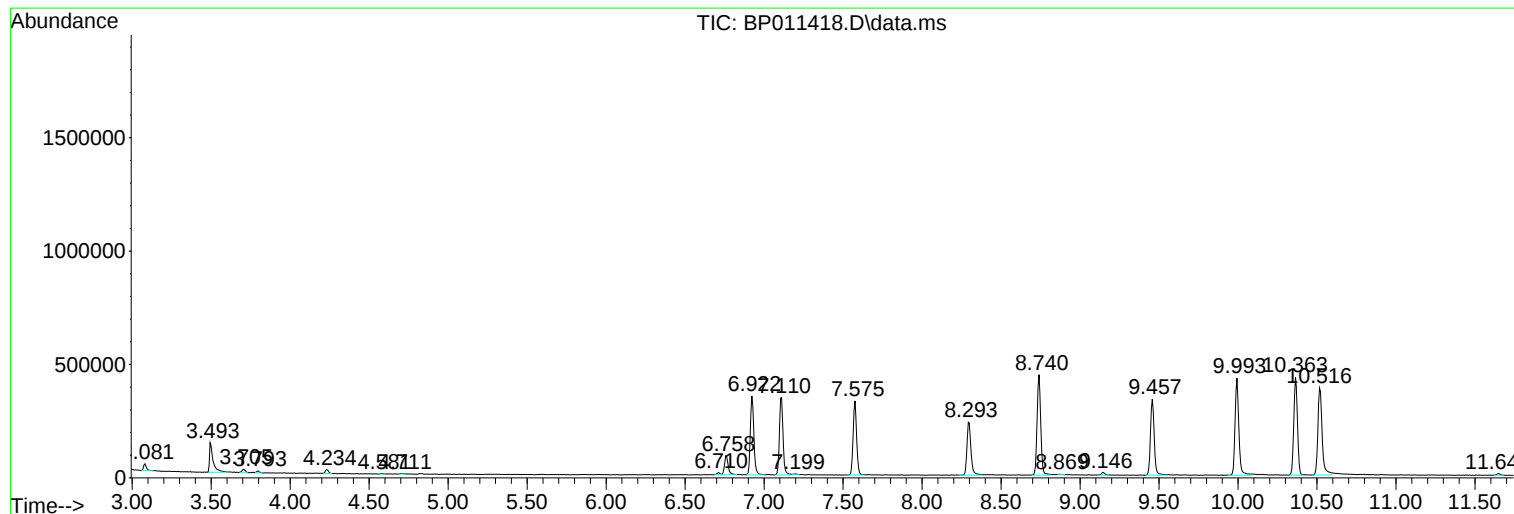

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011418.D
Acq On : 12 Aug 2022 11:12
Operator : CG/JU
Sample : N4129-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011418.D
Acq On : 12 Aug 2022 11:12
Operator : CG/JU
Sample : N4129-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBS9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc