

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011419.D
 Acq On : 12 Aug 2022 11:47
 Operator : CG/JU
 Sample : N4129-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	13	rBV	118513	150577	5.68%	0.633%
2	3.076	13	15	28	rVB	35373	52426	1.98%	0.220%
3	3.499	85	87	102	rBV	101329	161131	6.07%	0.677%
4	3.705	118	122	129	rVB2	15465	26066	0.98%	0.110%
5	3.799	134	138	145	rVB4	7621	10562	0.40%	0.044%
6	4.228	207	211	216	rVB	21866	30369	1.14%	0.128%
7	6.711	627	633	636	rBV2	11138	16224	0.61%	0.068%
8	6.758	636	641	655	rVB	103397	165468	6.24%	0.695%
9	6.922	663	669	682	rBV	349896	545075	20.55%	2.290%
10	7.105	693	700	710	rBV	367579	576056	21.72%	2.420%
11	7.193	712	715	719	rVB4	4482	6295	0.24%	0.026%
12	7.575	773	780	788	rBV	355413	545638	20.57%	2.292%
13	8.293	895	902	918	rBV	269881	453924	17.11%	1.907%
14	8.740	970	978	989	rBV	457268	733278	27.64%	3.080%
15	9.146	1042	1047	1054	rVB	12612	19676	0.74%	0.083%
16	9.458	1093	1100	1109	rBV	349731	554442	20.90%	2.329%
17	9.993	1184	1191	1209	rBV	434016	744401	28.06%	3.127%
18	10.363	1245	1254	1265	rBV	467143	763946	28.80%	3.209%
19	10.516	1271	1280	1296	rBV	369814	689564	26.00%	2.897%
20	11.646	1467	1472	1480	rBV2	8488	16703	0.63%	0.070%
21	11.975	1521	1528	1536	rVB2	6537	13548	0.51%	0.057%
22	12.199	1560	1566	1568	rBV7	2192	3652	0.14%	0.015%
23	12.593	1628	1633	1635	rBV6	1833	2972	0.11%	0.012%
24	12.857	1673	1678	1683	rBV9	1845	3156	0.12%	0.013%
25	13.675	1809	1817	1830	rBV	987291	1369367	51.62%	5.753%
26	13.781	1833	1835	1841	rVV7	4431	7791	0.29%	0.033%
27	13.940	1854	1862	1877	rBV	963706	1429081	53.87%	6.003%
28	14.251	1908	1915	1925	rBV	631016	927729	34.97%	3.897%
29	14.493	1950	1956	1966	rBV2	33889	92302	3.48%	0.388%
30	14.710	1989	1993	2003	rVB2	2371	5498	0.21%	0.023%
31	15.257	2079	2086	2102	rBV	1236278	1849079	69.71%	7.768%
32	15.387	2102	2108	2123	rVV	468297	672277	25.34%	2.824%
33	15.498	2123	2127	2134	rVB3	15350	26405	1.00%	0.111%
34	15.951	2200	2204	2208	rBV7	2243	4093	0.15%	0.017%
35	15.993	2208	2211	2215	rVV6	1978	3380	0.13%	0.014%
36	16.045	2217	2220	2226	rVB7	4262	5909	0.22%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011419.D
 Acq On : 12 Aug 2022 11:47
 Operator : CG/JU
 Sample : N4129-07
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.157	2236	2239	2244	rBV7	2194	3919	0.15%	0.016%
38	16.504	2294	2298	2302	rBV3	5207	7274	0.27%	0.031%
39	16.698	2328	2331	2336	rVB7	3357	4128	0.16%	0.017%
40	16.798	2345	2348	2353	rBV7	2931	5369	0.20%	0.023%
41	17.022	2380	2386	2397	rBV	778766	1093376	41.22%	4.593%
42	17.122	2397	2403	2417	rVV	1561168	2251706	84.88%	9.459%
43	17.334	2437	2439	2443	rVB5	2818	2899	0.11%	0.012%
44	17.587	2479	2482	2487	rVB4	6053	8900	0.34%	0.037%
45	17.710	2498	2503	2509	rBV5	17164	25865	0.98%	0.109%
46	17.945	2537	2543	2547	rBV9	6859	13041	0.49%	0.055%
47	18.016	2552	2555	2558	rVB	4248	4936	0.19%	0.021%
48	18.516	2637	2640	2643	rVB4	4878	5451	0.21%	0.023%
49	18.963	2712	2716	2720	rBV4	20147	28006	1.06%	0.118%
50	19.034	2724	2728	2733	rVV	18658	26006	0.98%	0.109%
51	19.292	2770	2772	2776	rVB3	6892	7433	0.28%	0.031%
52	19.386	2782	2788	2797	rBV	1950070	2565152	96.70%	10.776%
53	21.157	3084	3089	3103	rBV	929051	1233450	46.50%	5.182%
54	23.316	3449	3456	3465	rBV2	1408071	2652669	100.00%	11.144%
55	23.463	3475	3481	3492	rVB2	630661	1186747	44.74%	4.985%




Sum of corrected areas: 23804387

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011419.D
Acq On : 12 Aug 2022 11:47
Operator : CG/JU
Sample : N4129-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

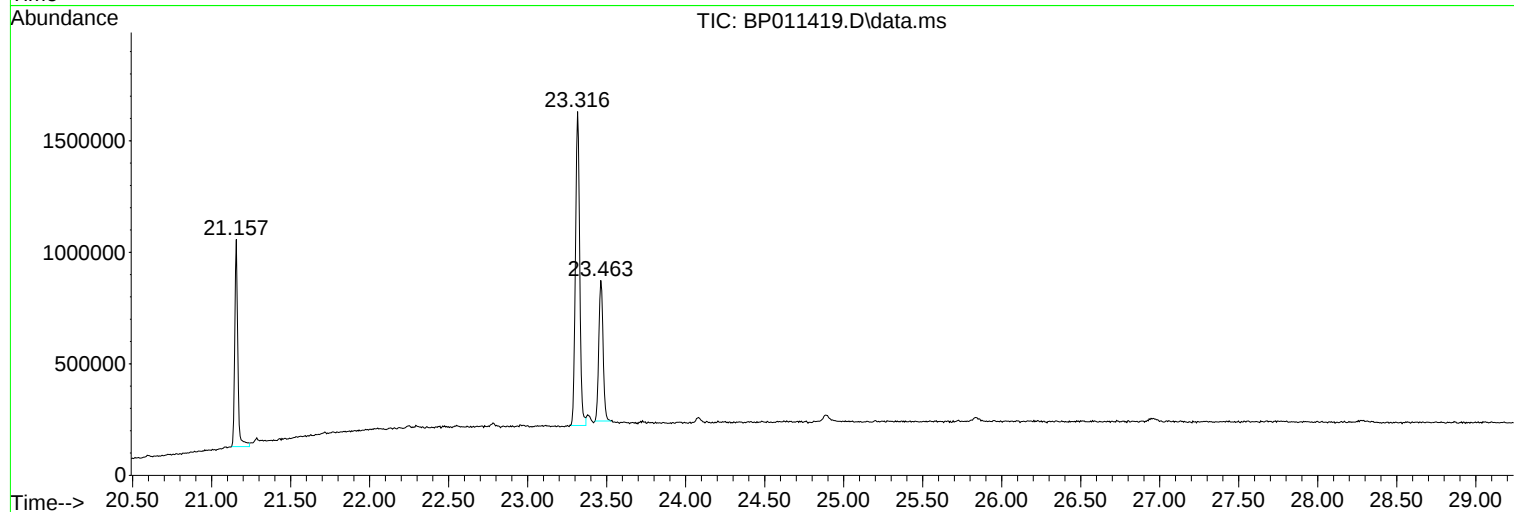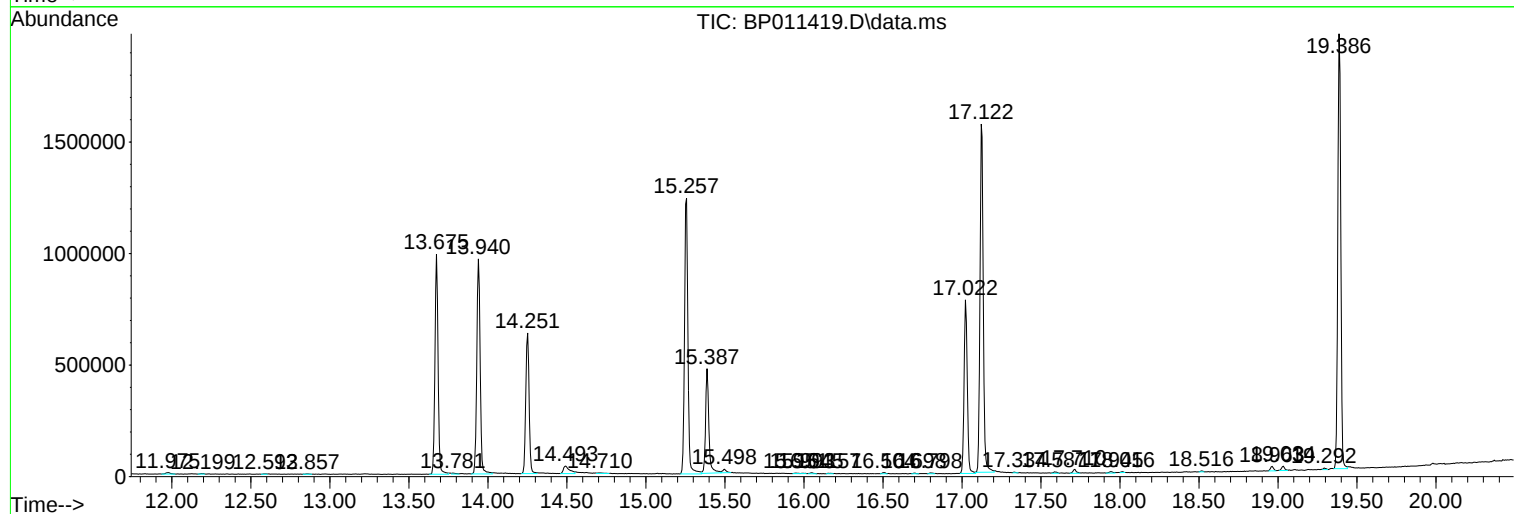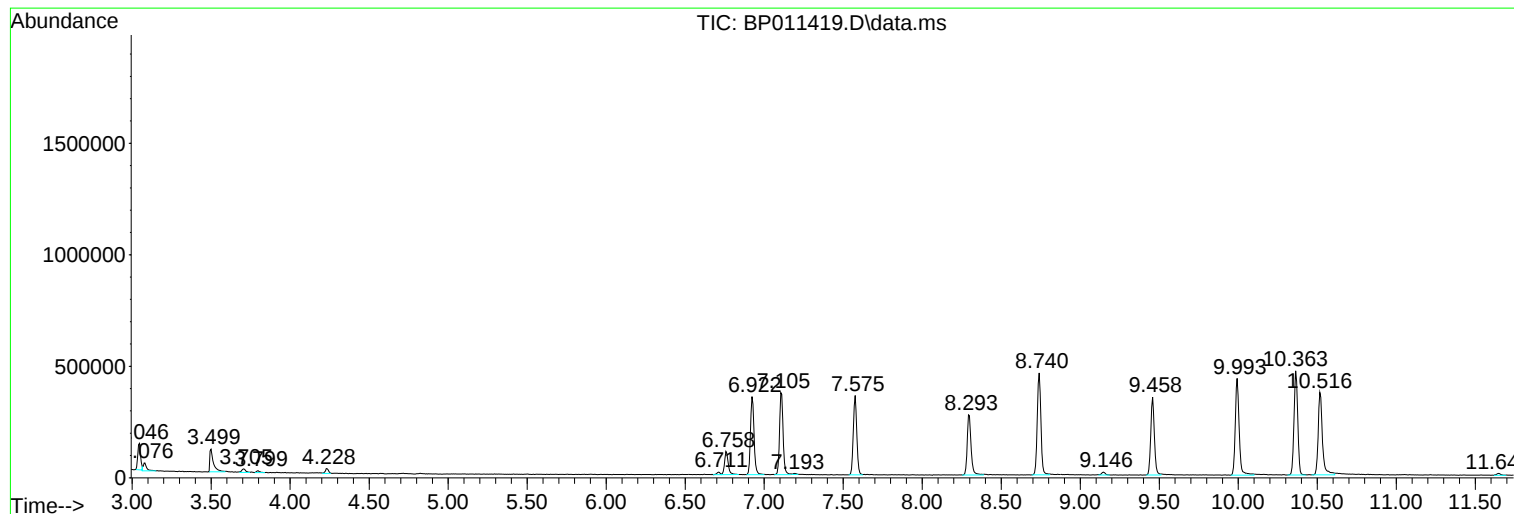

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011419.D
Acq On : 12 Aug 2022 11:47
Operator : CG/JU
Sample : N4129-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011419.D
Acq On : 12 Aug 2022 11:47
Operator : CG/JU
Sample : N4129-07
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc