

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011420.D
 Acq On : 12 Aug 2022 12:21
 Operator : CG/JU
 Sample : N4129-08
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	26	rVB	28985	37937	1.61%	0.172%
2	3.493	83	86	107	rBV	136479	218236	9.26%	0.988%
3	3.705	118	122	128	rVB	17675	24540	1.04%	0.111%
4	3.799	135	138	143	rVB3	7218	9452	0.40%	0.043%
5	4.234	208	212	217	rVB	21553	27861	1.18%	0.126%
6	4.828	310	313	316	rVB5	3419	4749	0.20%	0.022%
7	6.628	614	619	623	rVB8	1711	2724	0.12%	0.012%
8	6.710	627	633	636	rBV	10727	16409	0.70%	0.074%
9	6.757	636	641	653	rVB	87872	145446	6.17%	0.659%
10	6.922	663	669	682	rBV	340389	518876	22.02%	2.350%
11	7.110	693	701	712	rBV	341096	545060	23.13%	2.469%
12	7.199	712	716	720	rVB5	3960	6105	0.26%	0.028%
13	7.575	772	780	793	rBV	341238	528942	22.45%	2.396%
14	8.299	895	903	914	rBV	241971	405357	17.20%	1.836%
15	8.740	969	978	987	rBV	431411	694600	29.48%	3.146%
16	8.904	1004	1006	1013	rVB7	1995	3649	0.15%	0.017%
17	9.146	1042	1047	1054	rVB	14610	20899	0.89%	0.095%
18	9.457	1093	1100	1115	rBV	329873	533505	22.64%	2.416%
19	9.993	1183	1191	1207	rBV	401717	697934	29.62%	3.161%
20	10.363	1247	1254	1263	rBV	449527	725039	30.77%	3.284%
21	10.516	1273	1280	1303	rBV	382787	734022	31.15%	3.324%
22	11.128	1382	1384	1389	rVB6	1647	2689	0.11%	0.012%
23	11.651	1468	1473	1479	rVB3	9165	15109	0.64%	0.068%
24	11.975	1524	1528	1536	rVB4	7396	14412	0.61%	0.065%
25	12.604	1629	1635	1637	rBV7	2219	3612	0.15%	0.016%
26	12.851	1675	1677	1682	rVB5	2033	2781	0.12%	0.013%
27	13.222	1736	1740	1746	rBV9	2038	4544	0.19%	0.021%
28	13.675	1808	1817	1832	rBV	888535	1242519	52.74%	5.627%
29	13.939	1855	1862	1880	rBV	916447	1344424	57.06%	6.089%
30	14.251	1908	1915	1925	rBV	602757	876052	37.18%	3.968%
31	14.492	1950	1956	1968	rBV4	19727	66660	2.83%	0.302%
32	15.069	2050	2054	2059	rBV7	1585	2615	0.11%	0.012%
33	15.257	2079	2086	2102	rBV	1155359	1705225	72.37%	7.723%
34	15.386	2102	2108	2123	rVV	377610	579472	24.59%	2.624%
35	15.498	2123	2127	2135	rVB2	14472	27401	1.16%	0.124%
36	16.051	2216	2221	2226	rVB8	3728	6895	0.29%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011420.D
 Acq On : 12 Aug 2022 12:21
 Operator : CG/JU
 Sample : N4129-08
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.169	2236	2241	2246	rBV9	1801	3911	0.17%	0.018%
38	16.504	2295	2298	2304	rVB2	5961	8418	0.36%	0.038%
39	16.698	2327	2331	2336	rVB8	2632	4582	0.19%	0.021%
40	16.810	2343	2350	2355	rBV8	3629	8306	0.35%	0.038%
41	16.975	2374	2378	2380	rBV4	1590	2501	0.11%	0.011%
42	17.022	2380	2386	2397	rVV	724680	1036885	44.01%	4.696%
43	17.122	2397	2403	2420	rVV	1399862	2091968	88.79%	9.474%
44	17.239	2421	2423	2431	rVB9	9209	15693	0.67%	0.071%
45	17.592	2479	2483	2488	rBV3	5964	8306	0.35%	0.038%
46	17.716	2499	2504	2509	rBV7	3207	6871	0.29%	0.031%
47	17.933	2539	2541	2544	rBV3	3318	3624	0.15%	0.016%
48	18.010	2552	2554	2557	rBV	3029	3353	0.14%	0.015%
49	18.521	2637	2641	2644	rVB4	4056	5437	0.23%	0.025%
50	18.963	2712	2716	2721	rBV2	16367	23452	1.00%	0.106%
51	19.033	2724	2728	2732	rVV	16327	22465	0.95%	0.102%
52	19.292	2770	2772	2776	rVB5	4709	4880	0.21%	0.022%
53	19.386	2782	2788	2797	rBV	1820530	2356097	100.00%	10.671%
54	21.157	3084	3089	3101	rBV	851349	1159267	49.20%	5.250%
55	23.315	3449	3456	3464	rBV2	1244634	2350592	99.77%	10.646%
56	23.462	3475	3481	3497	rVB2	583621	1167695	49.56%	5.288%




Sum of corrected areas: 22080055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011420.D
Acq On : 12 Aug 2022 12:21
Operator : CG/JU
Sample : N4129-08
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

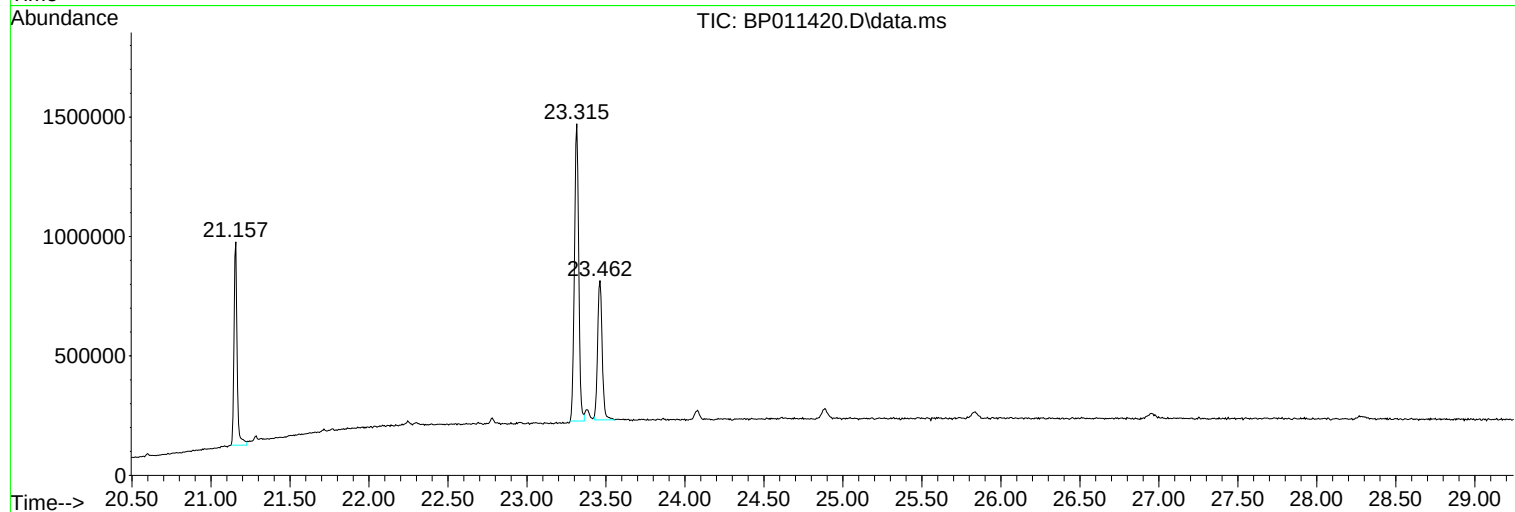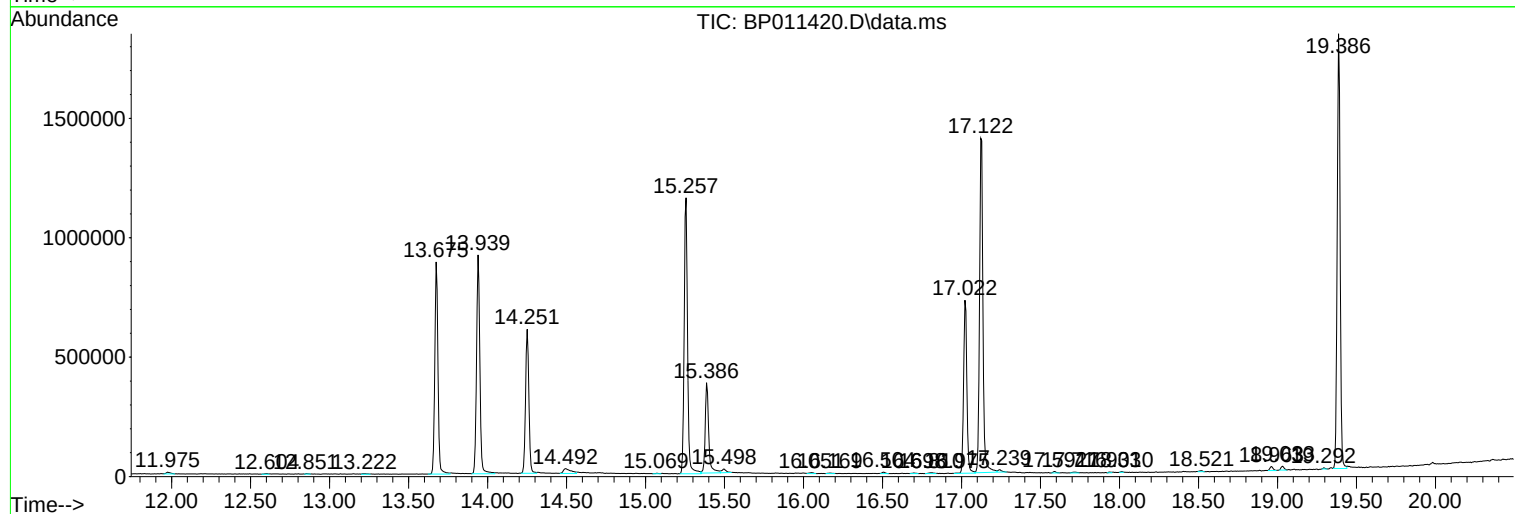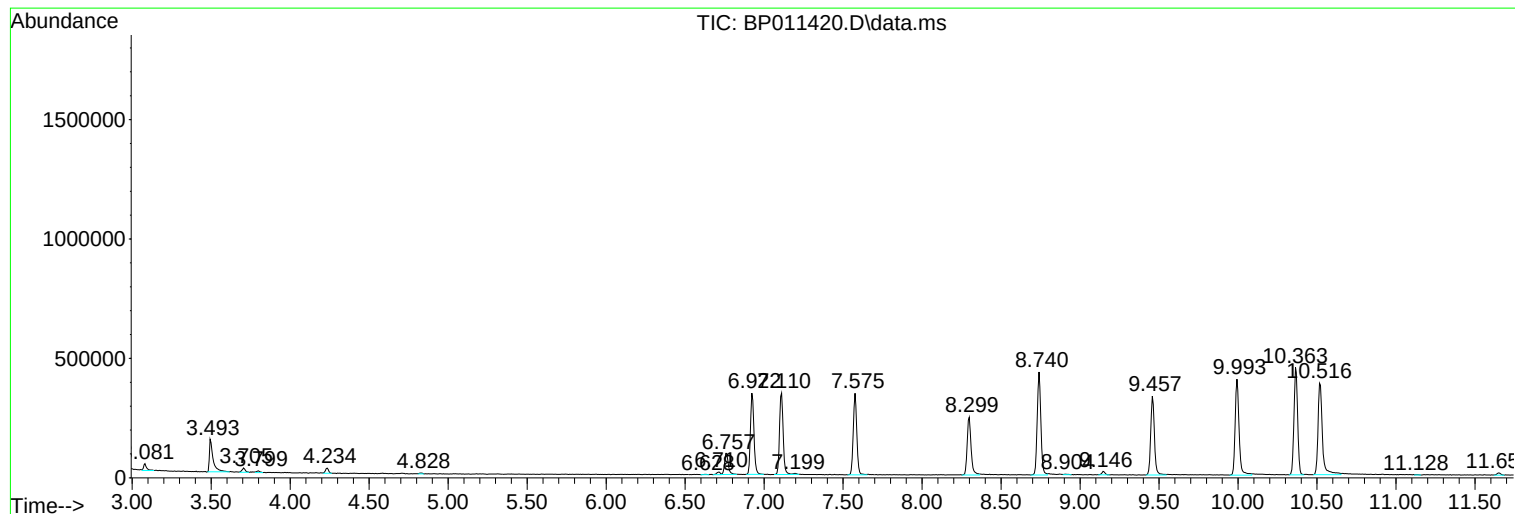

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011420.D
Acq On : 12 Aug 2022 12:21
Operator : CG/JU
Sample : N4129-08
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011420.D
Acq On : 12 Aug 2022 12:21
Operator : CG/JU
Sample : N4129-08
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc