

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011421.D
 Acq On : 12 Aug 2022 12:56
 Operator : CG/JU
 Sample : N4129-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	26	rVB	25936	35354	1.57%	0.169%
2	3.493	84	86	101	rBV	106988	168271	7.45%	0.805%
3	3.705	117	122	128	rVB	12820	17972	0.80%	0.086%
4	3.793	134	137	142	rVB	6226	7826	0.35%	0.037%
5	4.234	207	212	217	rVB	17923	25270	1.12%	0.121%
6	4.705	289	292	297	rVB7	3230	5405	0.24%	0.026%
7	4.828	309	313	316	rBV6	3386	4335	0.19%	0.021%
8	6.710	627	633	636	rBV3	10259	14225	0.63%	0.068%
9	6.757	636	641	652	rVB	78448	127857	5.66%	0.612%
10	6.922	663	669	682	rBV	321088	492912	21.83%	2.359%
11	7.105	692	700	713	rBV	313073	502686	22.26%	2.406%
12	7.199	713	716	725	rVB9	4579	8560	0.38%	0.041%
13	7.575	773	780	788	rBV	312664	490365	21.72%	2.347%
14	7.657	790	794	800	rVB6	3911	5853	0.26%	0.028%
15	8.293	896	902	918	rBV	215529	371105	16.43%	1.776%
16	8.740	971	978	987	rBV	394643	647967	28.69%	3.101%
17	8.869	996	1000	1005	rBV7	2761	3976	0.18%	0.019%
18	9.146	1043	1047	1054	rVB	12289	19315	0.86%	0.092%
19	9.457	1094	1100	1120	rVV	305145	498659	22.08%	2.387%
20	9.993	1184	1191	1204	rBV	386288	660983	29.27%	3.164%
21	10.175	1217	1222	1232	rBV3	14325	36104	1.60%	0.173%
22	10.363	1246	1254	1263	rBV	424809	679696	30.10%	3.253%
23	10.516	1273	1280	1296	rBV	337579	622481	27.57%	2.979%
24	11.028	1365	1367	1375	rVB8	1980	4016	0.18%	0.019%
25	11.645	1468	1472	1480	rVB2	7256	11383	0.50%	0.054%
26	11.975	1523	1528	1534	rBV4	7391	12978	0.57%	0.062%
27	12.592	1631	1633	1640	rBV8	1573	3061	0.14%	0.015%
28	12.857	1671	1678	1680	rBV8	1944	2995	0.13%	0.014%
29	13.222	1738	1740	1745	rVB6	2223	2970	0.13%	0.014%
30	13.675	1810	1817	1834	rBV	883775	1221426	54.09%	5.846%
31	13.939	1855	1862	1880	rBV	896796	1295716	57.38%	6.202%
32	14.251	1909	1915	1924	rBV	557724	815002	36.09%	3.901%
33	14.498	1951	1957	1971	rBV3	20790	68307	3.02%	0.327%
34	15.257	2078	2086	2100	rBV	1109830	1669324	73.92%	7.990%
35	15.386	2103	2108	2120	rVV	379408	552462	24.46%	2.644%
36	15.498	2123	2127	2137	rVB4	14394	27971	1.24%	0.134%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011421.D
 Acq On : 12 Aug 2022 12:56
 Operator : CG/JU
 Sample : N4129-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.639	2149	2151	2157	rVB6	3402	4449	0.20%	0.021%
38	16.045	2218	2220	2228	rVB9	4363	6200	0.27%	0.030%
39	16.510	2294	2299	2303	rVB6	4472	7017	0.31%	0.034%
40	16.704	2326	2332	2336	rVB8	2962	5815	0.26%	0.028%
41	16.810	2345	2350	2355	rBV9	3011	6149	0.27%	0.029%
42	16.969	2373	2377	2379	rBV5	2728	3590	0.16%	0.017%
43	17.022	2380	2386	2397	rVV	687238	975632	43.20%	4.670%
44	17.122	2397	2403	2420	rVV	1376730	1984152	87.87%	9.497%
45	17.586	2479	2482	2491	rVB5	5748	8707	0.39%	0.042%
46	17.716	2502	2504	2507	rBV4	2484	2358	0.10%	0.011%
47	17.939	2539	2542	2550	rBV7	8658	15677	0.69%	0.075%
48	18.010	2552	2554	2558	rVV3	3875	4798	0.21%	0.023%
49	18.216	2585	2589	2590	rBV4	1710	2390	0.11%	0.011%
50	18.510	2637	2639	2645	rVB5	3624	4905	0.22%	0.023%
51	18.963	2711	2716	2720	rBV2	17055	24121	1.07%	0.115%
52	19.027	2723	2727	2733	rVV	15228	23412	1.04%	0.112%
53	19.386	2782	2788	2796	rBV	1786107	2258173	100.00%	10.809%
54	21.157	3084	3089	3099	rBV	804297	1078697	47.77%	5.163%
55	23.310	3449	3455	3463	rBV2	1215903	2234895	98.97%	10.697%
56	23.462	3474	3481	3493	rVB	548979	1106611	49.00%	5.297%




Sum of corrected areas: 20892536

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011421.D
Acq On : 12 Aug 2022 12:56
Operator : CG/JU
Sample : N4129-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

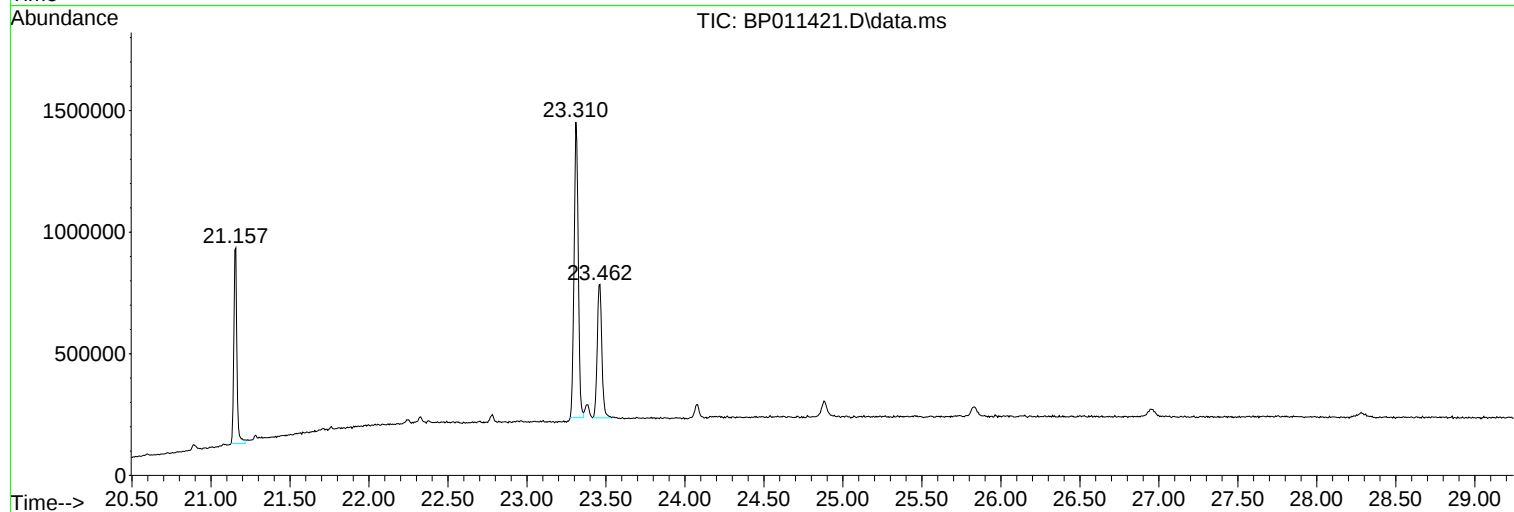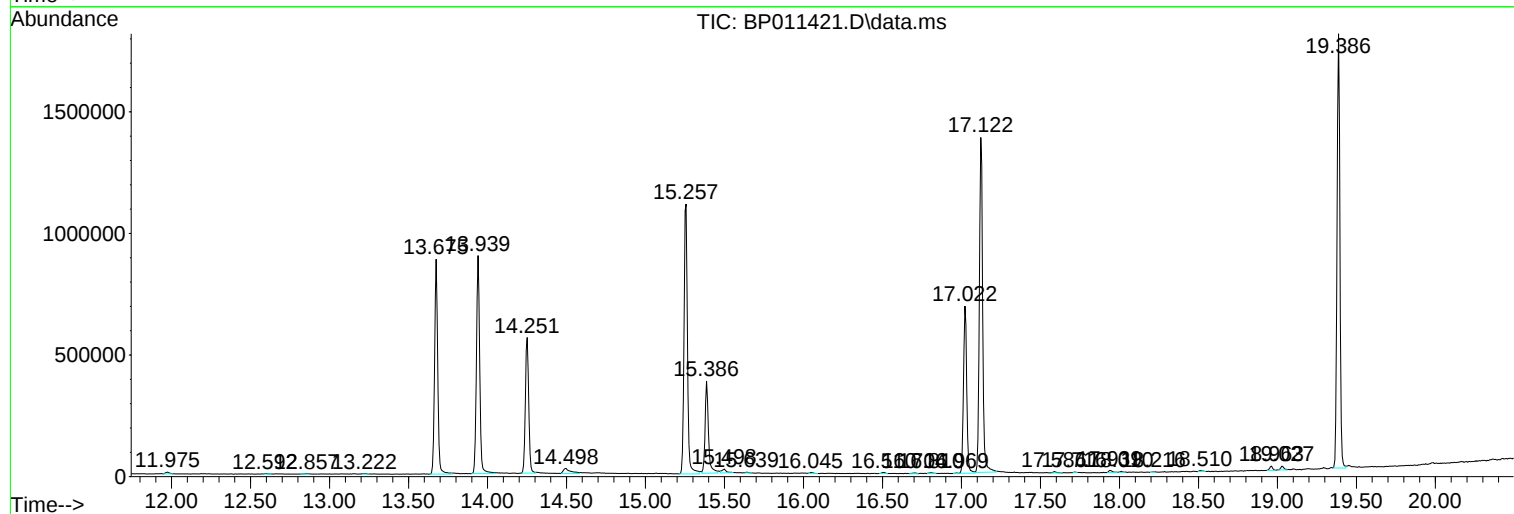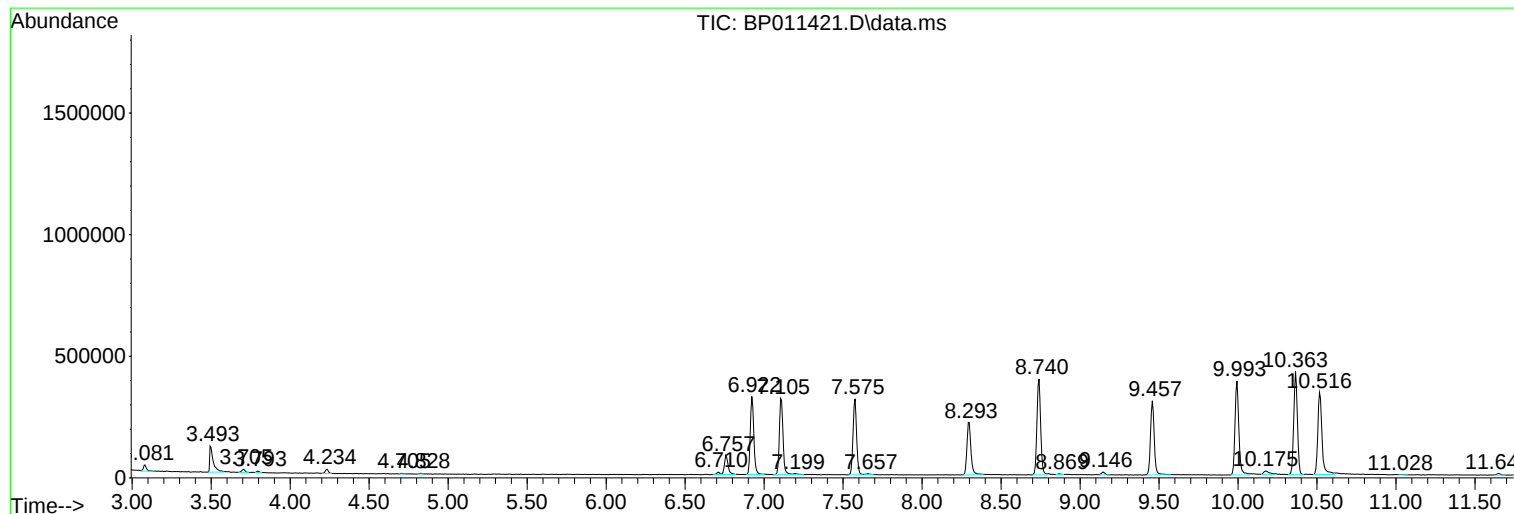

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011421.D
Acq On : 12 Aug 2022 12:56
Operator : CG/JU
Sample : N4129-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011421.D
Acq On : 12 Aug 2022 12:56
Operator : CG/JU
Sample : N4129-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc