

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011422.D
 Acq On : 12 Aug 2022 13:30
 Operator : CG/JU
 Sample : N4129-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	21	rVB	26711	32746	1.17%	0.131%
2	3.493	84	86	100	rBV	145223	220072	7.86%	0.881%
3	3.705	117	122	128	rVB	14359	22695	0.81%	0.091%
4	3.793	134	137	144	rVB2	9248	14189	0.51%	0.057%
5	4.234	208	212	218	rVB	21180	29850	1.07%	0.120%
6	4.711	290	293	296	rVB4	3432	3367	0.12%	0.013%
7	4.828	310	313	317	rVB5	4716	5196	0.19%	0.021%
8	6.711	628	633	636	rBV	11209	15137	0.54%	0.061%
9	6.758	636	641	655	rVB	98804	158540	5.66%	0.635%
10	6.922	662	669	681	rBV	379393	564097	20.15%	2.259%
11	7.105	693	700	711	rBV	369215	587289	20.98%	2.352%
12	7.193	713	715	719	rVB3	2564	3369	0.12%	0.013%
13	7.575	773	780	789	rBV	384023	585542	20.91%	2.345%
14	7.652	791	793	802	rVB8	4563	7435	0.27%	0.030%
15	8.293	896	902	916	rBV	258941	439980	15.71%	1.762%
16	8.740	971	978	987	rBV	465326	751356	26.84%	3.008%
17	9.146	1042	1047	1056	rVB	12830	20697	0.74%	0.083%
18	9.457	1092	1100	1114	rBV	362229	591564	21.13%	2.369%
19	9.993	1183	1191	1206	rBV	448930	772150	27.58%	3.092%
20	10.363	1247	1254	1263	rBV	505999	830350	29.66%	3.325%
21	10.516	1272	1280	1298	rBV	413565	767041	27.40%	3.071%
22	11.646	1467	1472	1478	rBV2	8425	13771	0.49%	0.055%
23	11.975	1523	1528	1533	rBV4	7122	13676	0.49%	0.055%
24	13.210	1735	1738	1741	rBV5	2576	3727	0.13%	0.015%
25	13.675	1810	1817	1833	rBV	983737	1385139	49.47%	5.546%
26	13.940	1855	1862	1876	rBV	1033256	1485913	53.07%	5.950%
27	14.251	1907	1915	1923	rBV	693659	1018182	36.37%	4.077%
28	14.487	1950	1955	1971	rBV4	25302	82670	2.95%	0.331%
29	14.704	1988	1992	1999	rVB10	3294	5710	0.20%	0.023%
30	15.122	2059	2063	2068	rVB8	2658	5072	0.18%	0.020%
31	15.251	2079	2085	2099	rBV	1281957	1906235	68.08%	7.633%
32	15.387	2102	2108	2122	rVV	481836	680412	24.30%	2.724%
33	15.492	2123	2126	2132	rVB2	14319	22865	0.82%	0.092%
34	15.998	2207	2212	2214	rBV5	2649	4281	0.15%	0.017%
35	16.051	2217	2221	2224	rVB5	3841	5278	0.19%	0.021%
36	16.181	2237	2243	2247	rVB8	2761	5503	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011422.D
 Acq On : 12 Aug 2022 13:30
 Operator : CG/JU
 Sample : N4129-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.504	2295	2298	2304	rVB4	8960	11316	0.40%	0.045%
38	16.698	2327	2331	2335	rBV7	2717	5223	0.19%	0.021%
39	16.804	2345	2349	2352	rBV5	3115	6049	0.22%	0.024%
40	17.022	2380	2386	2397	rBV	840189	1214862	43.39%	4.864%
41	17.122	2397	2403	2421	rVV2	1660729	2374437	84.81%	9.507%
42	17.592	2478	2483	2486	rBV3	5304	7504	0.27%	0.030%
43	17.716	2500	2504	2508	rBV6	4574	6385	0.23%	0.026%
44	17.939	2539	2542	2549	rBV8	5212	9150	0.33%	0.037%
45	18.010	2549	2554	2561	rVV4	4236	7771	0.28%	0.031%
46	18.516	2636	2640	2644	rBV3	5346	7611	0.27%	0.030%
47	18.957	2711	2715	2720	rBV2	20248	28965	1.03%	0.116%
48	19.033	2723	2728	2733	rBV	18888	29090	1.04%	0.116%
49	19.386	2782	2788	2797	rBV	2067253	2719891	97.14%	10.891%
50	21.157	3084	3089	3102	rBV	999345	1356812	48.46%	5.433%
51	23.316	3449	3456	3464	rBV2	1509137	2799875	100.00%	11.211%
52	23.463	3475	3481	3489	rVB2	706674	1328719	47.46%	5.320%




Sum of corrected areas: 24974756

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011422.D
Acq On : 12 Aug 2022 13:30
Operator : CG/JU
Sample : N4129-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

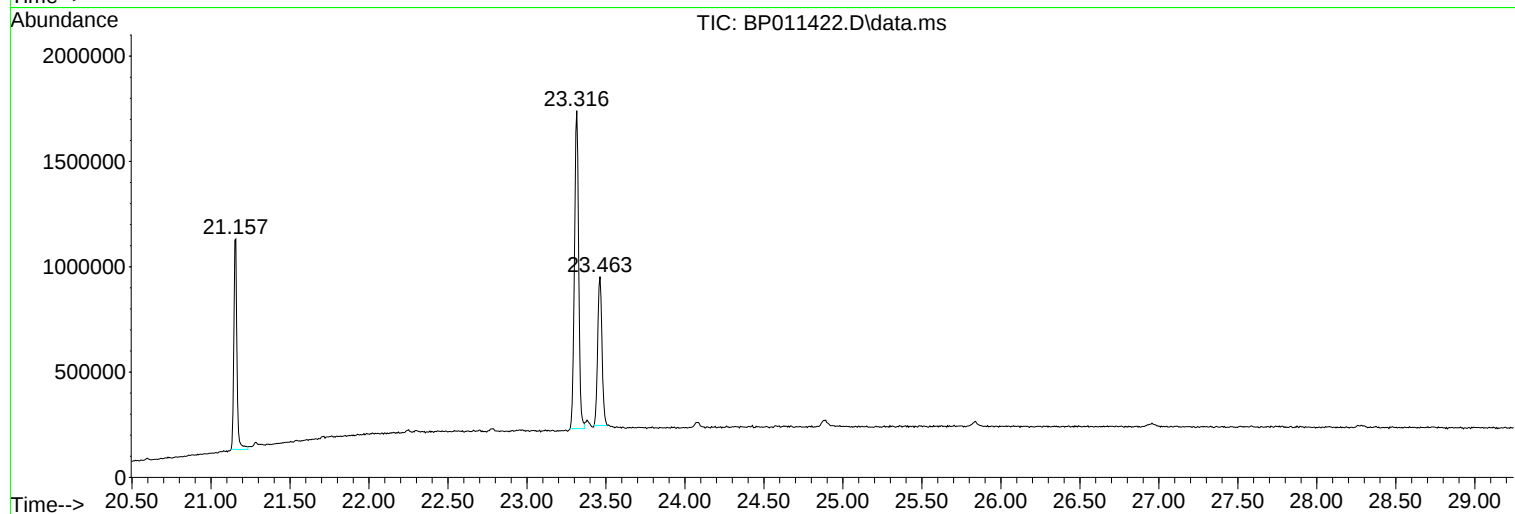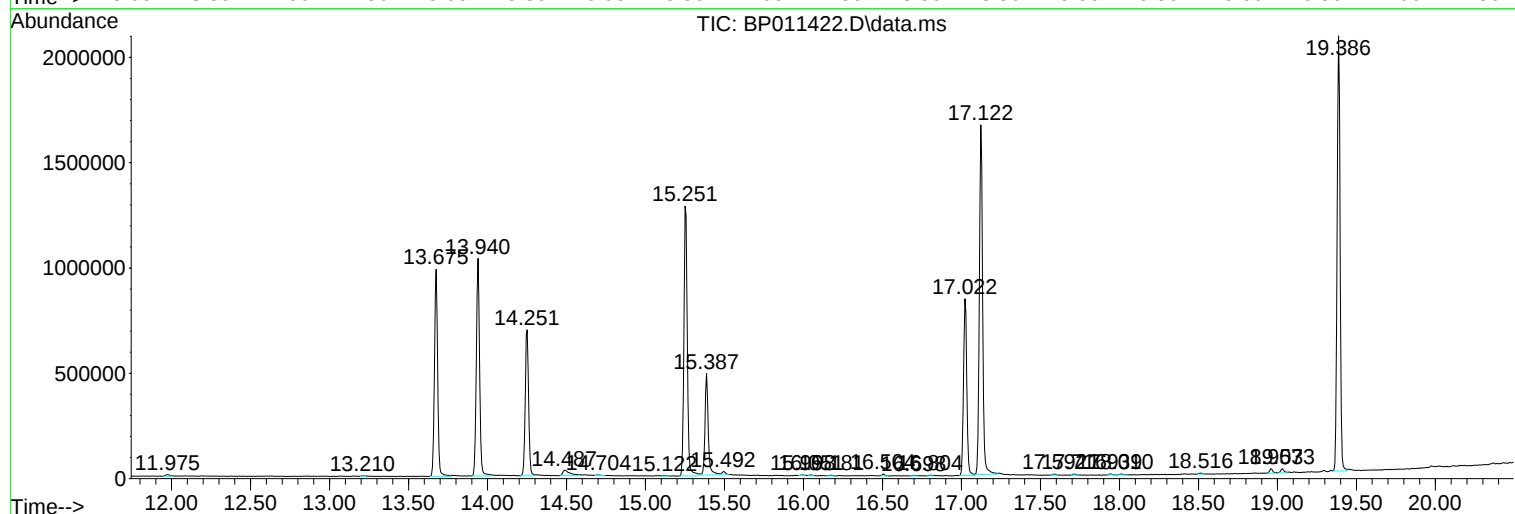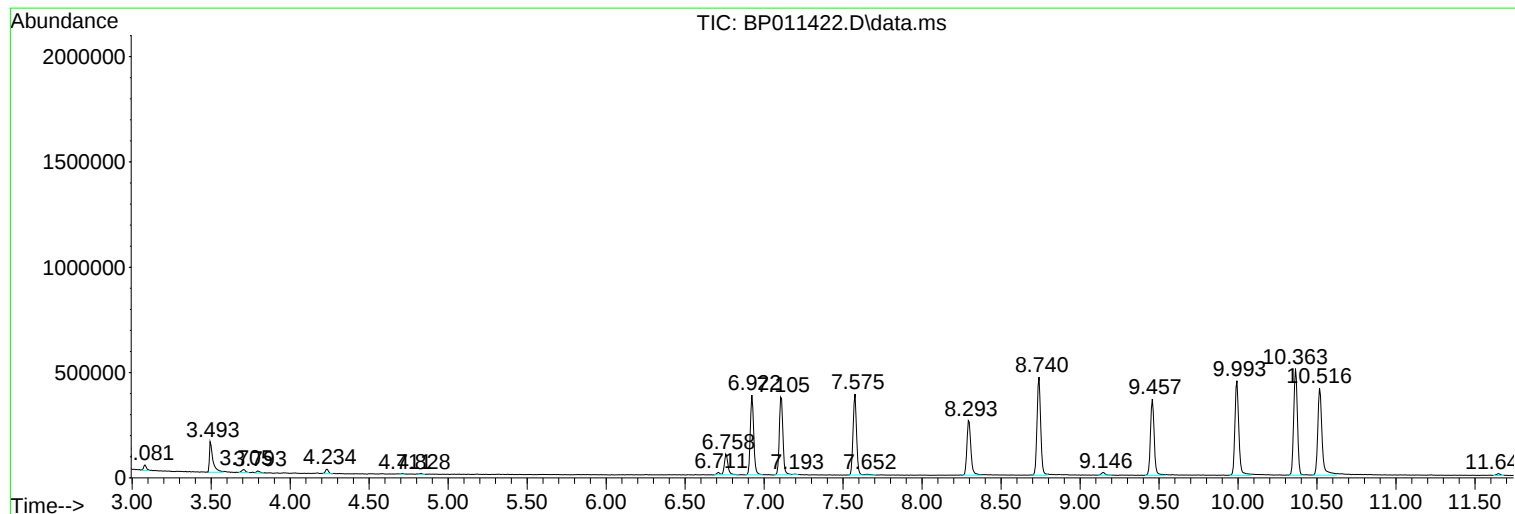

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011422.D
Acq On : 12 Aug 2022 13:30
Operator : CG/JU
Sample : N4129-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011422.D
Acq On : 12 Aug 2022 13:30
Operator : CG/JU
Sample : N4129-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc