

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011423.D
 Acq On : 12 Aug 2022 14:05
 Operator : CG/JU
 Sample : N4129-14
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	24	rVB	27071	36102	1.43%	0.152%
2	3.499	84	87	101	rBV	104881	169405	6.73%	0.713%
3	3.705	117	122	127	rVB3	14727	21793	0.87%	0.092%
4	3.793	133	137	142	rVB	19119	26117	1.04%	0.110%
5	4.234	208	212	219	rVB	19580	28307	1.12%	0.119%
6	4.822	310	312	320	rVB8	3327	4836	0.19%	0.020%
7	6.228	548	551	556	rVB7	1491	2648	0.11%	0.011%
8	6.710	629	633	636	rBV	11281	14378	0.57%	0.060%
9	6.757	636	641	653	rVB	86109	139655	5.55%	0.588%
10	6.922	663	669	683	rBV	367331	559786	22.23%	2.355%
11	7.105	694	700	712	rBV	359905	573779	22.78%	2.414%
12	7.199	712	716	719	rVB5	3276	4781	0.19%	0.020%
13	7.575	773	780	790	rBV	398124	618530	24.56%	2.603%
14	8.293	896	902	917	rBV	238987	405472	16.10%	1.706%
15	8.740	970	978	991	rBV	454698	737079	29.27%	3.101%
16	9.146	1040	1047	1052	rVB	10830	18049	0.72%	0.076%
17	9.457	1093	1100	1110	rBV	349027	564611	22.42%	2.376%
18	9.993	1184	1191	1204	rBV	433974	732512	29.09%	3.082%
19	10.363	1246	1254	1263	rBV	522587	849624	33.74%	3.575%
20	10.516	1273	1280	1294	rBV	358969	664472	26.38%	2.796%
21	11.645	1467	1472	1479	rVB3	8452	13244	0.53%	0.056%
22	11.975	1522	1528	1534	rBV4	7528	14755	0.59%	0.062%
23	12.975	1694	1698	1702	rVB7	1466	2602	0.10%	0.011%
24	13.222	1736	1740	1745	rVB8	1746	2956	0.12%	0.012%
25	13.675	1811	1817	1829	rBV	979801	1343190	53.33%	5.652%
26	13.757	1829	1831	1834	rVB4	2326	3009	0.12%	0.013%
27	13.939	1855	1862	1879	rBV	998840	1428626	56.73%	6.011%
28	14.251	1907	1915	1924	rBV	710835	1027976	40.82%	4.325%
29	14.492	1950	1956	1966	rBV4	20746	62617	2.49%	0.263%
30	15.257	2079	2086	2102	rBV	1239529	1856355	73.71%	7.811%
31	15.386	2102	2108	2122	rVV	427852	625608	24.84%	2.632%
32	15.498	2123	2127	2135	rVB2	15323	27000	1.07%	0.114%
33	15.951	2198	2204	2207	rBV8	1974	4083	0.16%	0.017%
34	15.998	2209	2212	2216	rVV6	2805	4411	0.18%	0.019%
35	16.045	2216	2220	2226	rVB9	4393	7217	0.29%	0.030%
36	16.504	2294	2298	2304	rBV2	5523	8166	0.32%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011423.D
 Acq On : 12 Aug 2022 14:05
 Operator : CG/JU
 Sample : N4129-14
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.698	2329	2331	2337	rVB7	2324	3163	0.13%	0.013%
38	16.810	2345	2350	2353	rBV7	2632	4743	0.19%	0.020%
39	17.022	2380	2386	2397	rBV	865447	1210819	48.08%	5.095%
40	17.122	2397	2403	2419	rVV	1494609	2166597	86.03%	9.116%
41	17.592	2479	2483	2487	rBV4	5632	7207	0.29%	0.030%
42	17.716	2501	2504	2510	rVB8	3455	4941	0.20%	0.021%
43	17.939	2539	2542	2546	rBV6	5888	7909	0.31%	0.033%
44	18.516	2636	2640	2644	rBV7	4585	7494	0.30%	0.032%
45	18.963	2712	2716	2721	rBV3	17100	22673	0.90%	0.095%
46	19.033	2724	2728	2734	rBV	17476	24187	0.96%	0.102%
47	19.339	2777	2780	2782	rBV4	8095	7070	0.28%	0.030%
48	19.386	2782	2788	2797	rBV	1933369	2458749	97.63%	10.346%
49	21.157	3084	3089	3097	rBV	1017858	1333650	52.96%	5.612%
50	23.315	3449	3456	3464	rBV2	1364217	2518427	100.00%	10.597%
51	23.462	3475	3481	3493	rVB2	708876	1384918	54.99%	5.827%




Sum of corrected areas: 23766298

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011423.D
Acq On : 12 Aug 2022 14:05
Operator : CG/JU
Sample : N4129-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

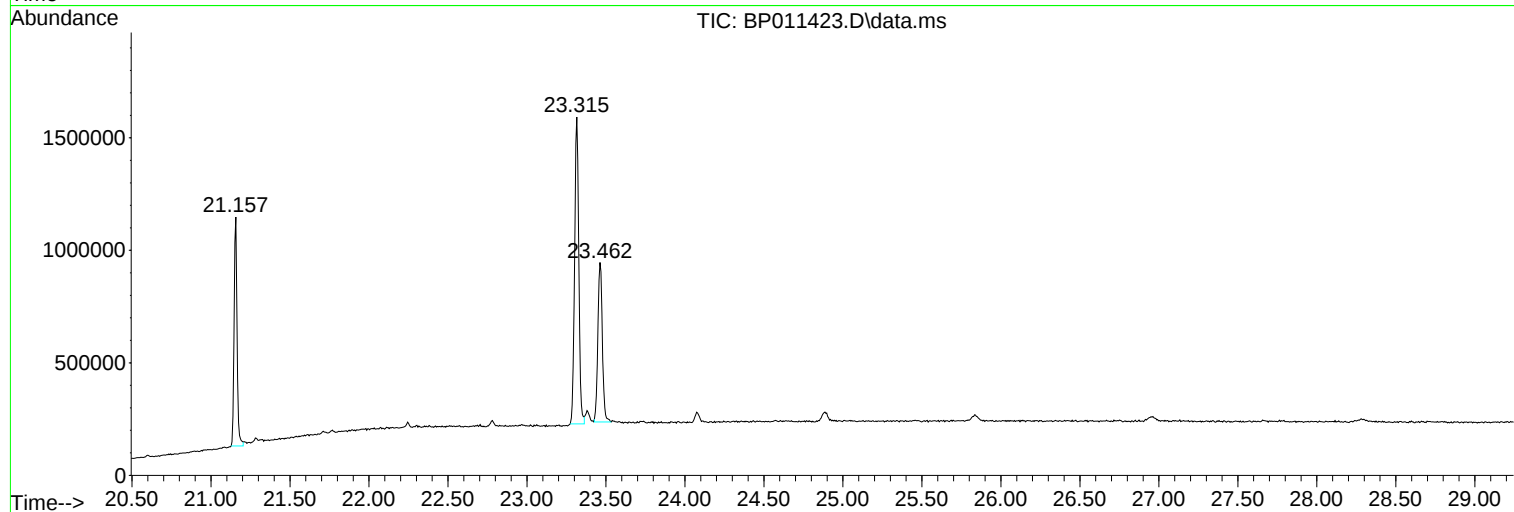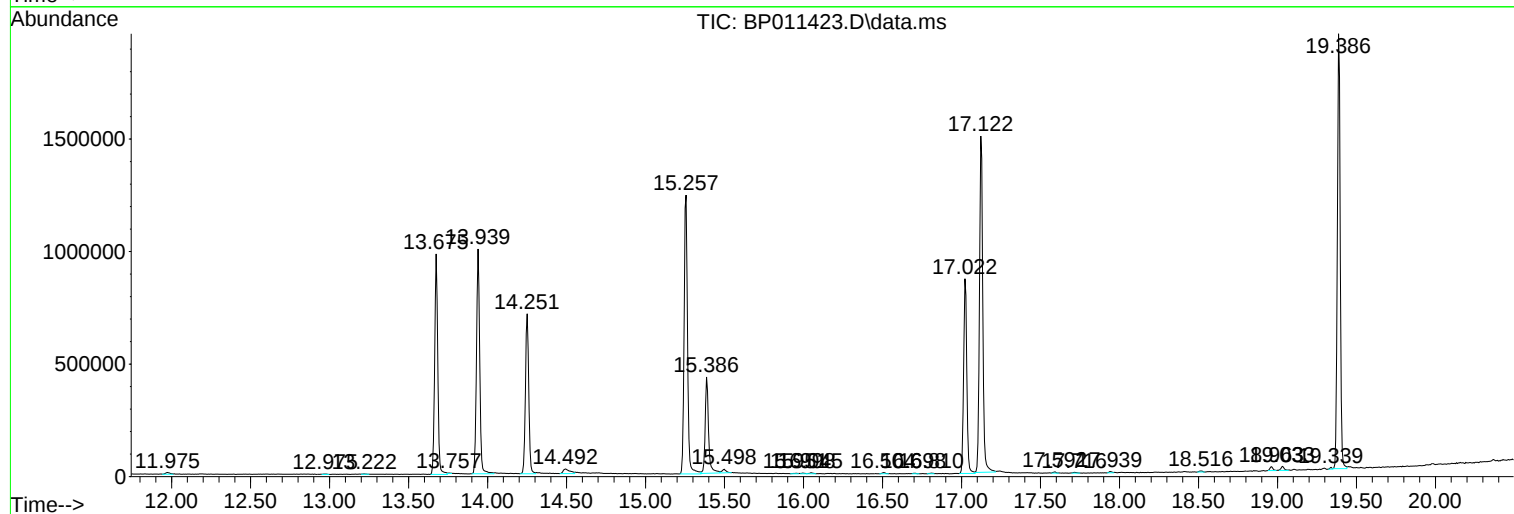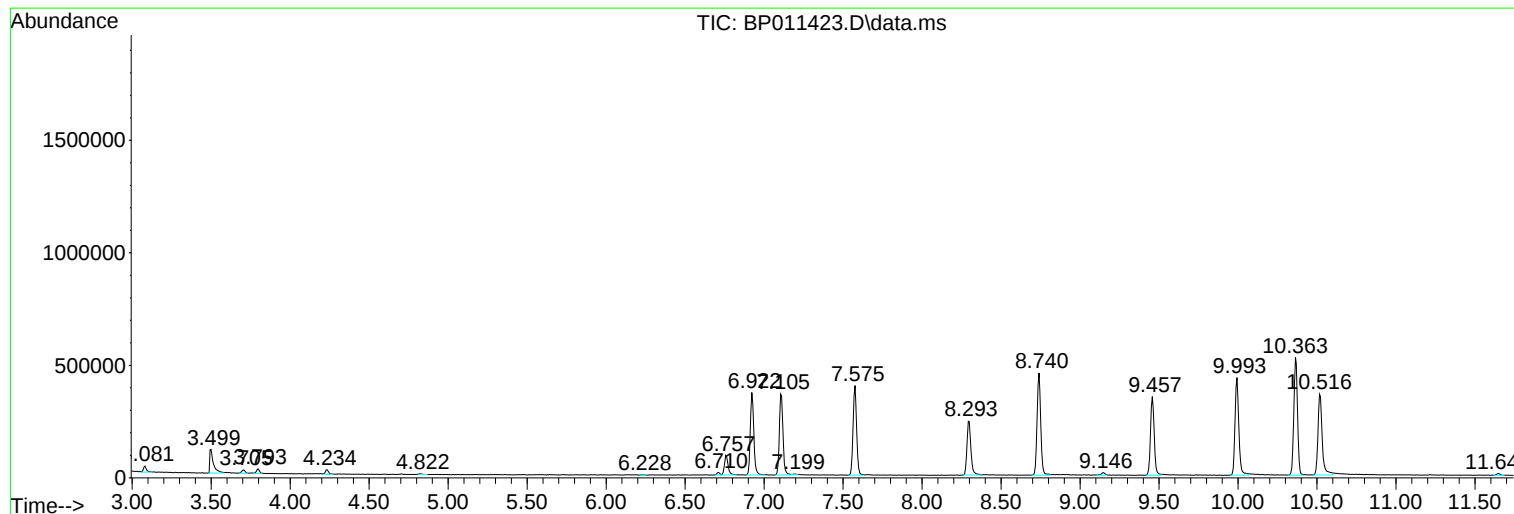

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011423.D
Acq On : 12 Aug 2022 14:05
Operator : CG/JU
Sample : N4129-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011423.D
Acq On : 12 Aug 2022 14:05
Operator : CG/JU
Sample : N4129-14
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc