

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	6	9	13	rBV	28033	36274	1.44%	0.149%
2	3.076	13	15	23	rVB	26936	36343	1.44%	0.149%
3	3.499	85	87	98	rBV	99734	155608	6.16%	0.639%
4	3.705	117	122	129	rVB	13561	21532	0.85%	0.088%
5	3.799	133	138	143	rVB	24558	34056	1.35%	0.140%
6	4.234	207	212	216	rVB	18918	25931	1.03%	0.106%
7	4.581	268	271	274	rBV5	1759	2592	0.10%	0.011%
8	4.828	309	313	316	rBV5	2884	3650	0.14%	0.015%
9	6.122	532	533	541	rVB8	1386	2671	0.11%	0.011%
10	6.711	629	633	636	rBV2	9366	13013	0.51%	0.053%
11	6.758	636	641	649	rVB	81413	128551	5.09%	0.528%
12	6.922	660	669	686	rBV	354318	548031	21.68%	2.249%
13	7.105	694	700	712	rBV	346477	554207	21.93%	2.274%
14	7.575	773	780	788	rBV	406729	636909	25.20%	2.614%
15	7.658	790	794	797	rVB6	2014	3487	0.14%	0.014%
16	8.293	894	902	919	rBV	232740	405823	16.06%	1.665%
17	8.740	971	978	994	rBV	440993	719873	28.48%	2.954%
18	9.146	1041	1047	1053	rVB	11458	19995	0.79%	0.082%
19	9.458	1093	1100	1111	rBV	346873	550109	21.76%	2.258%
20	9.993	1184	1191	1203	rBV	428233	729608	28.87%	2.994%
21	10.363	1247	1254	1268	rVB	548988	880508	34.84%	3.614%
22	10.516	1273	1280	1297	rBV	355481	649118	25.68%	2.664%
23	11.652	1464	1473	1477	rBV3	7570	12616	0.50%	0.052%
24	11.975	1522	1528	1535	rBV7	8347	16300	0.64%	0.067%
25	12.057	1538	1542	1546	rBV4	3024	5229	0.21%	0.021%
26	12.857	1673	1678	1681	rVB7	1779	2541	0.10%	0.010%
27	13.157	1723	1729	1732	rBV7	2582	4503	0.18%	0.018%
28	13.675	1809	1817	1831	rBV	953095	1330841	52.65%	5.462%
29	13.940	1855	1862	1875	rBV	976938	1409069	55.75%	5.783%
30	14.251	1908	1915	1925	rBV	741242	1076102	42.58%	4.416%
31	14.493	1950	1956	1974	rBV4	22072	78483	3.11%	0.322%
32	15.257	2078	2086	2100	rBV	1192819	1812768	71.72%	7.440%
33	15.387	2102	2108	2121	rVV	445322	637218	25.21%	2.615%
34	15.493	2124	2126	2131	rVB3	12982	18183	0.72%	0.075%
35	16.051	2217	2221	2226	rVB7	4568	6539	0.26%	0.027%
36	16.169	2237	2241	2244	rBV6	1828	2866	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.510	2295	2299	2304	rVB4	4589	6094	0.24%	0.025%
38	16.704	2328	2332	2335	rVB5	2821	3762	0.15%	0.015%
39	16.804	2345	2349	2356	rBV10	4160	7796	0.31%	0.032%
40	16.969	2374	2377	2380	rBV4	2112	3129	0.12%	0.013%
41	17.022	2380	2386	2397	rVV	900756	1274517	50.43%	5.231%
42	17.122	2397	2403	2426	rVB	1524702	2218974	87.79%	9.107%
43	17.587	2478	2482	2488	rVB3	4982	8578	0.34%	0.035%
44	17.710	2500	2503	2509	rVB7	3224	5622	0.22%	0.023%
45	17.939	2539	2542	2548	rBV7	4930	6770	0.27%	0.028%
46	18.010	2552	2554	2558	rVB3	2894	4067	0.16%	0.017%
47	18.516	2636	2640	2644	rBV7	6288	8400	0.33%	0.034%
48	18.963	2711	2716	2721	rBV5	18783	27817	1.10%	0.114%
49	19.034	2723	2728	2732	rVV2	18023	25798	1.02%	0.106%
50	19.104	2738	2740	2745	rVB5	4408	4816	0.19%	0.020%
51	19.339	2776	2780	2782	rBV5	9230	12858	0.51%	0.053%
52	19.386	2782	2788	2798	rVV	1933357	2521775	99.77%	10.349%
53	19.645	2827	2832	2836	rBV	112778	130394	5.16%	0.535%
54	21.157	3084	3089	3098	rBV	1063551	1386257	54.85%	5.689%
55	22.033	3234	3238	3244	rBV	203050	250925	9.93%	1.030%
56	23.316	3449	3456	3464	rBV2	1310874	2527496	100.00%	10.373%
57	23.463	3475	3481	3491	rVB2	690795	1359514	53.79%	5.579%




Sum of corrected areas: 24366506

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011424.D
Acq On : 12 Aug 2022 14:39
Operator : CG/JU
Sample : N4129-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

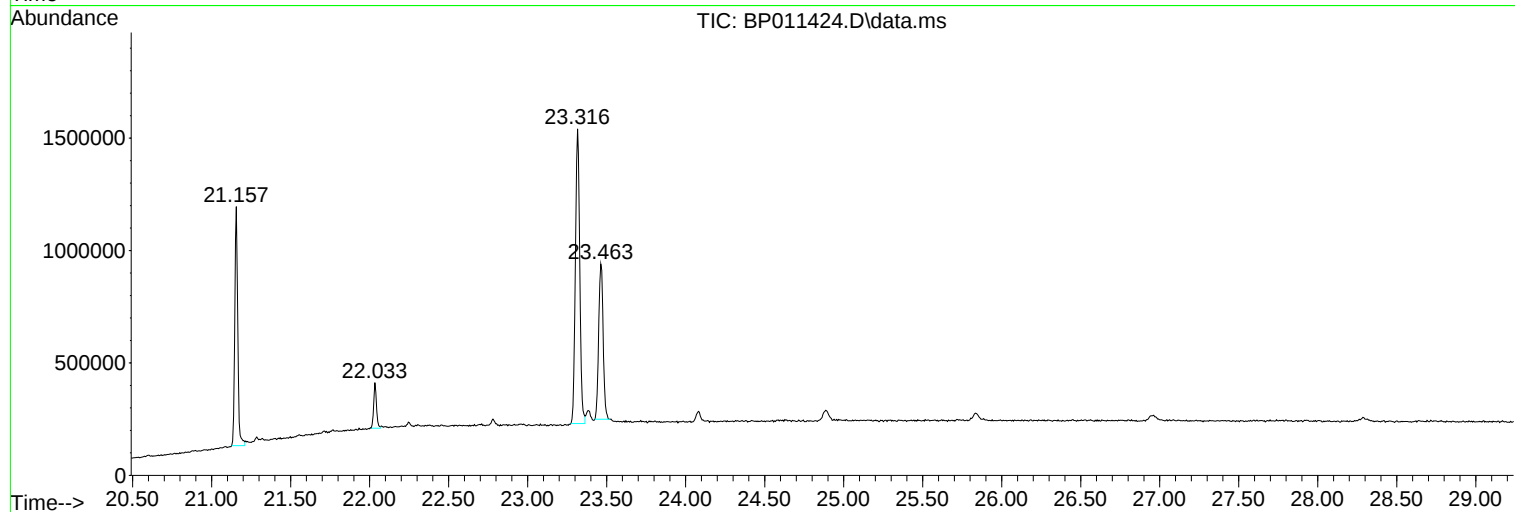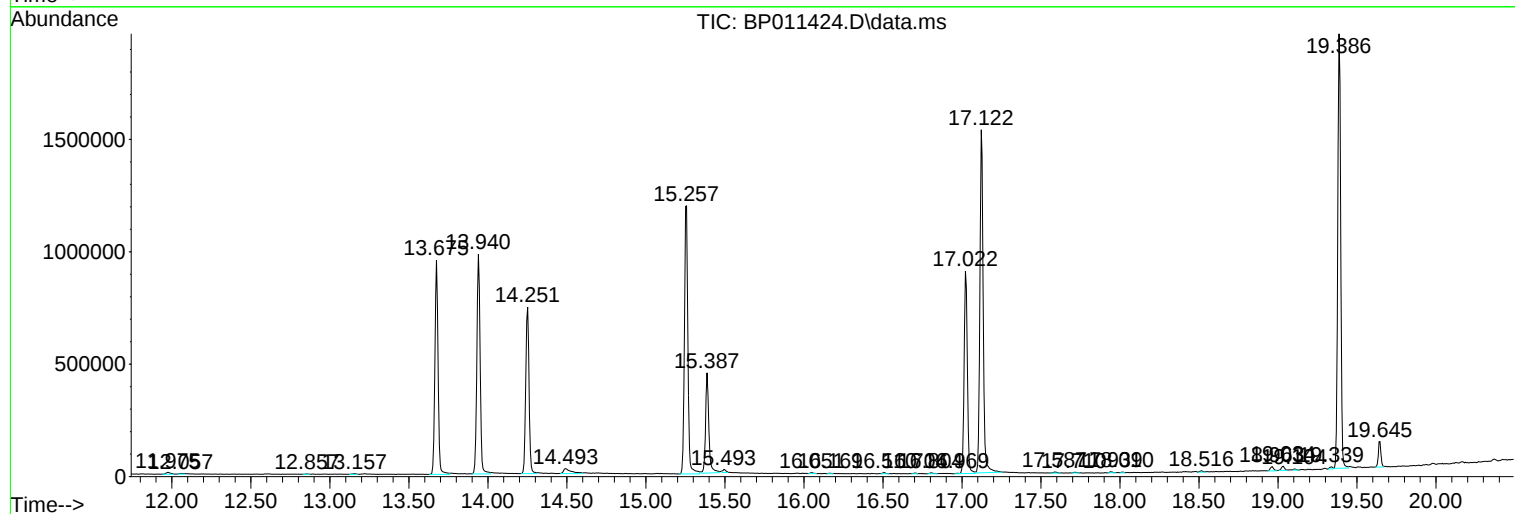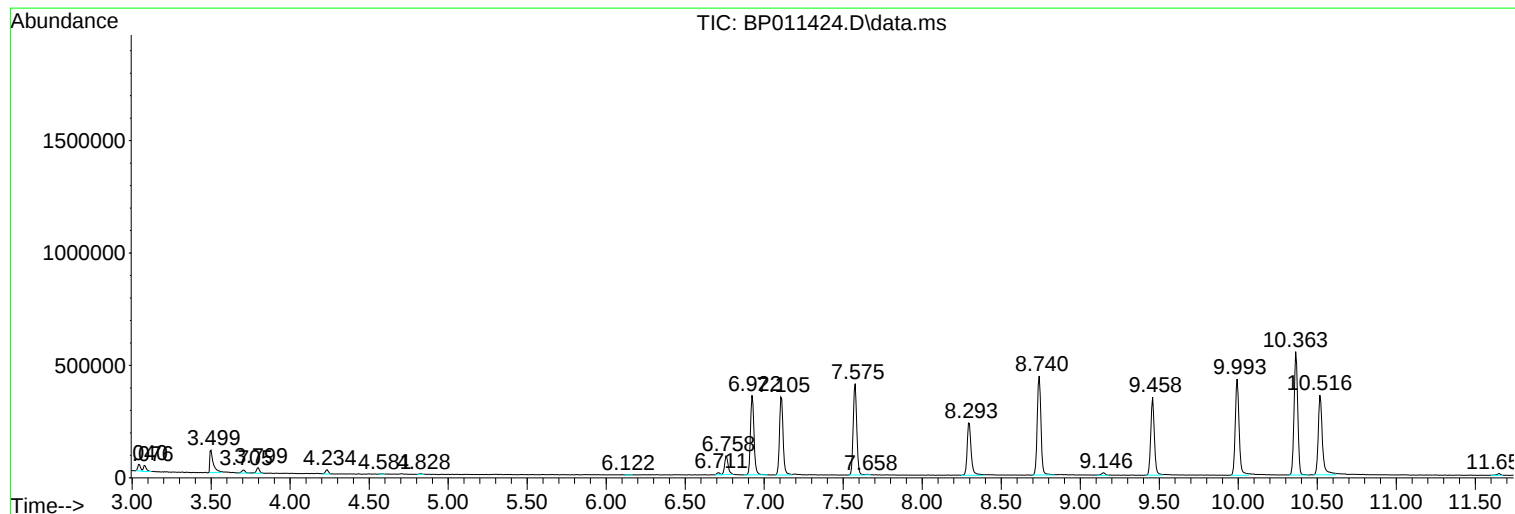

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011424.D
Acq On : 12 Aug 2022 14:39
Operator : CG/JU
Sample : N4129-15
Misc :
ALS Vial : 48 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
BGBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,3-Benzenedicarboxylic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
22.033	3.62 ng/ul	250925	Chrysene-d12	21.157	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,3-Benzenedicarboxylic acid, bi...	390	C24H38O4	000137-89-3	64
2	1,4-Benzenedicarboxylic acid, bi...	390	C24H38O4	006422-86-2	52
3	1,4-Benzenedicarboxylic acid, bi...	390	C24H38O4	006422-86-2	50
4	1,3-Benzenedicarboxylic acid, bi...	390	C24H38O4	000137-89-3	47
5	1,4-Benzenedicarboxylic acid, bi...	390	C24H38O4	006422-86-2	25

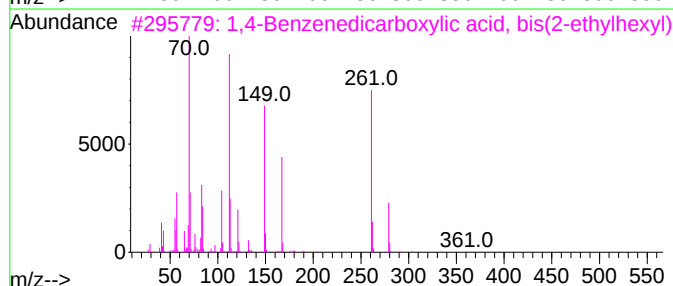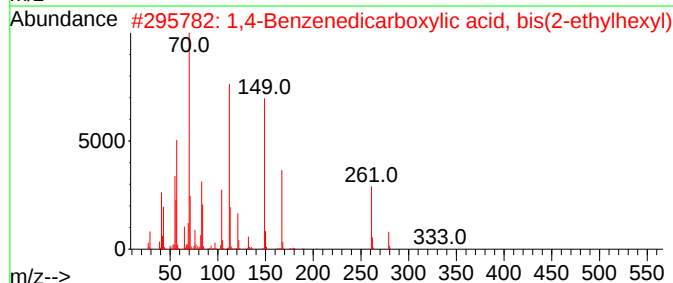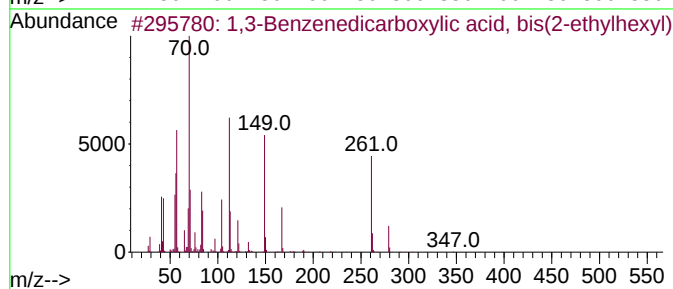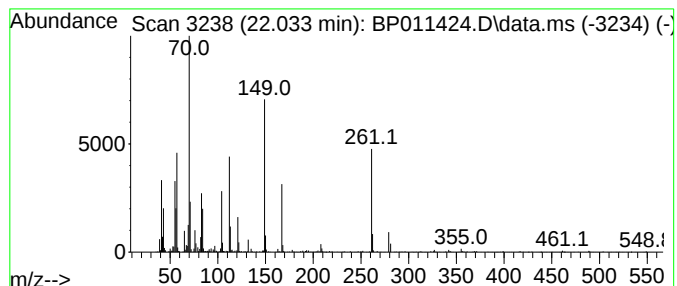

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011424.D
Acq On : 12 Aug 2022 14:39
Operator : CG/JU
Sample : N4129-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Benzenedica...	22.033	3.6	ng/u1	250925	5	21.157	1386260	20.0