

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011431.D
 Acq On : 12 Aug 2022 19:15
 Operator : CG/JU
 Sample : N4165-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	21	rBV	26013	32272	1.67%	0.166%
2	3.499	84	87	102	rBV	91260	145793	7.53%	0.751%
3	3.705	118	122	127	rVB2	13152	20364	1.05%	0.105%
4	3.799	134	138	142	rVB2	8830	10871	0.56%	0.056%
5	4.228	207	211	219	rVB	18839	28866	1.49%	0.149%
6	4.711	289	293	297	rVB5	1727	2304	0.12%	0.012%
7	4.822	310	312	317	rVB4	2805	3817	0.20%	0.020%
8	6.710	628	633	636	rBV2	9299	14650	0.76%	0.075%
9	6.758	636	641	652	rVB	74954	123273	6.37%	0.635%
10	6.922	663	669	681	rBV	285895	433916	22.40%	2.235%
11	7.105	694	700	712	rBV	288594	449313	23.20%	2.314%
12	7.193	712	715	719	rVB6	4216	5897	0.30%	0.030%
13	7.575	773	780	790	rBV	346448	540670	27.92%	2.785%
14	8.293	896	902	915	rBV	205211	346706	17.90%	1.786%
15	8.740	969	978	991	rBV	352187	586524	30.28%	3.021%
16	8.910	1004	1007	1011	rVB6	2074	3022	0.16%	0.016%
17	9.146	1038	1047	1054	rVB2	11353	18630	0.96%	0.096%
18	9.457	1093	1100	1113	rBV	271508	444136	22.93%	2.288%
19	9.993	1184	1191	1206	rBV	331151	570651	29.47%	2.939%
20	10.363	1246	1254	1262	rBV	471696	753336	38.90%	3.880%
21	10.516	1271	1280	1293	rBV	288927	531199	27.43%	2.736%
22	11.651	1467	1473	1478	rVB3	7870	12717	0.66%	0.066%
23	11.975	1523	1528	1537	rVB6	5863	11810	0.61%	0.061%
24	13.222	1735	1740	1746	rBV10	1443	3044	0.16%	0.016%
25	13.675	1809	1817	1834	rBV	718550	1027406	53.05%	5.292%
26	13.940	1850	1862	1871	rBV	750044	1105996	57.11%	5.697%
27	14.251	1908	1915	1931	rBV	612702	933840	48.22%	4.810%
28	14.487	1949	1955	1964	rBV5	18805	54941	2.84%	0.283%
29	14.616	1976	1977	1982	rVB5	2542	2512	0.13%	0.013%
30	14.716	1992	1994	2000	rVB7	1841	2581	0.13%	0.013%
31	15.075	2048	2055	2057	rBV7	2248	4033	0.21%	0.021%
32	15.192	2071	2075	2078	rVB5	1341	2019	0.10%	0.010%
33	15.251	2078	2085	2102	rBV	947499	1424036	73.53%	7.335%
34	15.386	2102	2108	2122	rVV	316378	456201	23.56%	2.350%
35	15.992	2202	2211	2214	rBV7	5643	10498	0.54%	0.054%
36	16.169	2234	2241	2246	rBV9	3685	8685	0.45%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011431.D
 Acq On : 12 Aug 2022 19:15
 Operator : CG/JU
 Sample : N4165-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.504	2294	2298	2301	rVB5	5059	6119	0.32%	0.032%
38	16.704	2328	2332	2335	rVB6	1851	2387	0.12%	0.012%
39	16.810	2345	2350	2355	rBV8	2454	4282	0.22%	0.022%
40	17.022	2380	2386	2397	rBV	791976	1119907	57.83%	5.768%
41	17.122	2397	2403	2422	rVV	1191589	1727254	89.19%	8.897%
42	17.328	2435	2438	2449	rVB2	10266	17931	0.93%	0.092%
43	17.586	2479	2482	2487	rVB4	4929	7718	0.40%	0.040%
44	17.716	2500	2504	2505	rBV4	3003	4020	0.21%	0.021%
45	17.939	2539	2542	2547	rBV7	5827	7569	0.39%	0.039%
46	18.016	2552	2555	2558	rVB4	3724	4220	0.22%	0.022%
47	18.222	2588	2590	2593	rBV4	1893	2639	0.14%	0.014%
48	18.275	2597	2599	2602	rVB4	2466	2182	0.11%	0.011%
49	18.404	2618	2621	2622	rBV3	3890	4024	0.21%	0.021%
50	18.516	2636	2640	2644	rVV6	5208	6832	0.35%	0.035%
51	18.957	2711	2715	2720	rBV5	14129	21587	1.11%	0.111%
52	19.027	2723	2727	2733	rVV2	14381	23701	1.22%	0.122%
53	19.098	2737	2739	2742	rVB4	4267	4578	0.24%	0.024%
54	19.386	2782	2788	2796	rBV	1540307	1936701	100.00%	9.976%
55	21.151	3084	3088	3100	rBV	933984	1227198	63.37%	6.321%
56	23.310	3449	3455	3464	rBV2	1046677	1900927	98.15%	9.791%
57	23.463	3474	3481	3491	rBV	651693	1256048	64.86%	6.470%




Sum of corrected areas: 19414353

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011431.D
Acq On : 12 Aug 2022 19:15
Operator : CG/JU
Sample : N4165-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

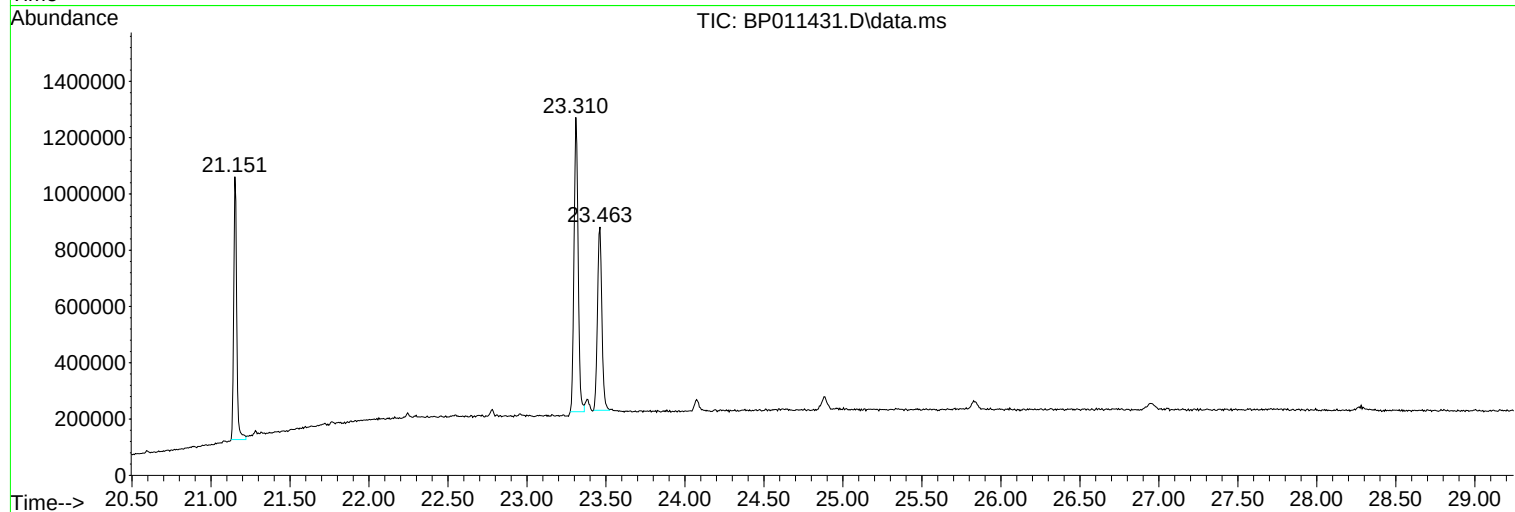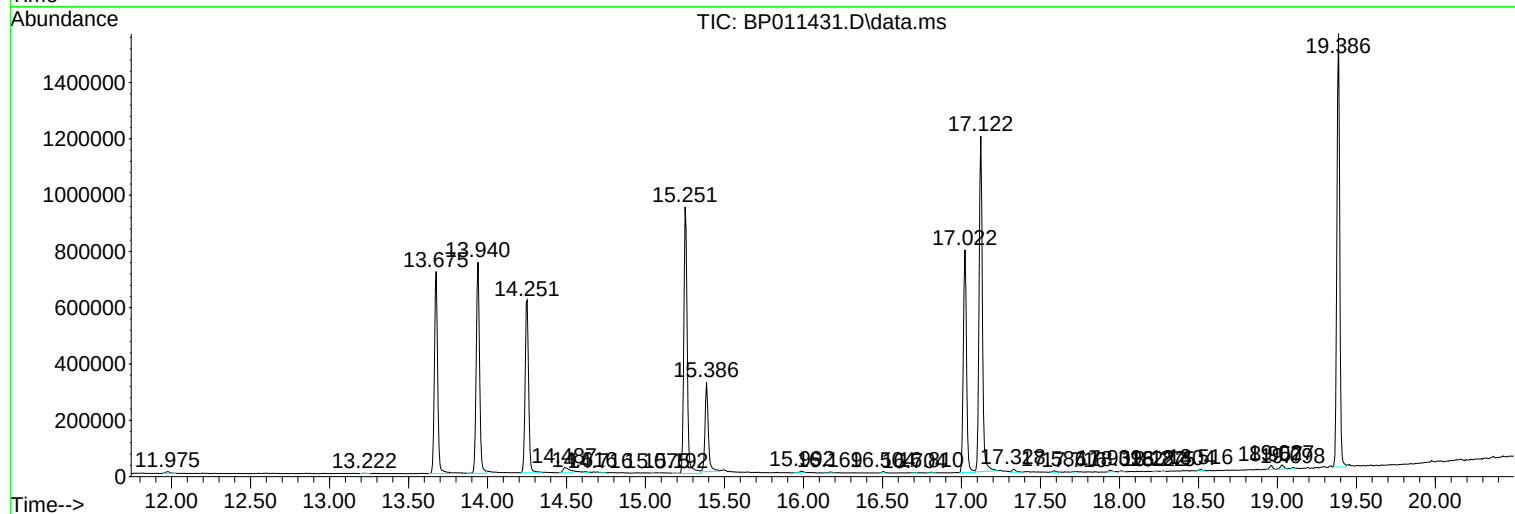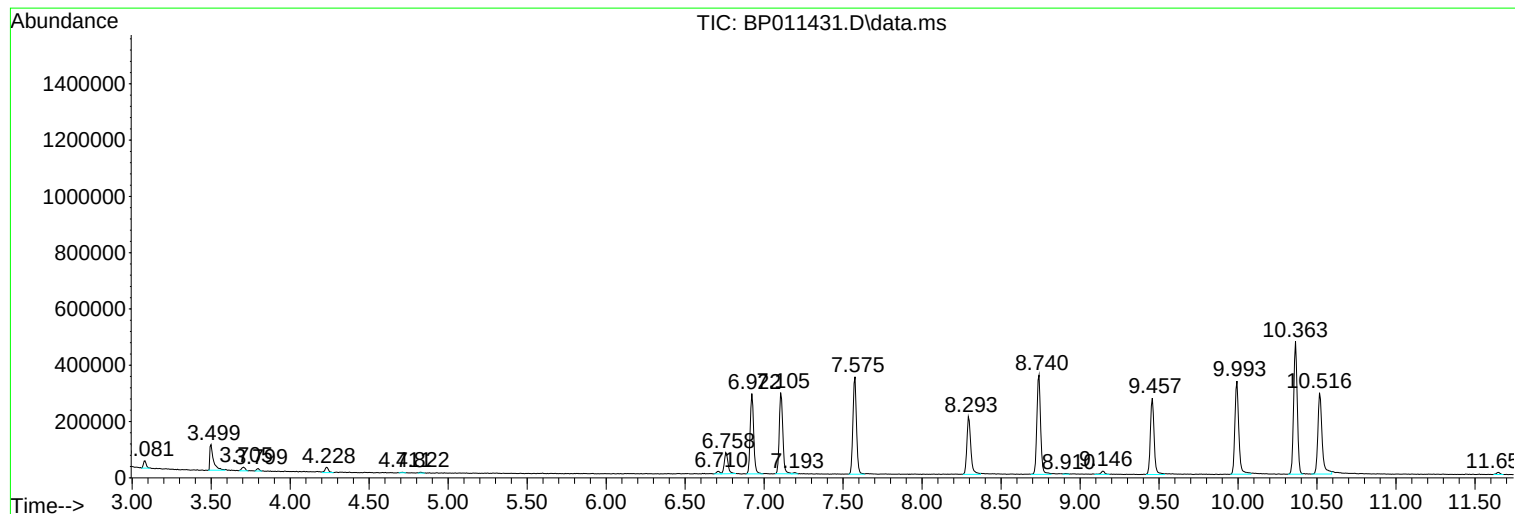

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011431.D
Acq On : 12 Aug 2022 19:15
Operator : CG/JU
Sample : N4165-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011431.D
Acq On : 12 Aug 2022 19:15
Operator : CG/JU
Sample : N4165-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc