

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011432.D
 Acq On : 12 Aug 2022 19:50
 Operator : CG/JU
 Sample : N4165-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.076	12	15	21	rVB	23833	29905	1.51%	0.151%
2	3.493	84	86	101	rBV	108542	173518	8.77%	0.876%
3	3.705	116	122	127	rVB2	14698	25331	1.28%	0.128%
4	3.793	134	137	144	rVB2	15159	21885	1.11%	0.111%
5	4.228	207	211	218	rVB	22381	31958	1.61%	0.161%
6	4.711	289	293	296	rVB6	3253	4871	0.25%	0.025%
7	4.828	311	313	316	rVB4	3929	3550	0.18%	0.018%
8	6.711	628	633	636	rBV3	11636	16254	0.82%	0.082%
9	6.758	636	641	654	rVB	91940	153551	7.76%	0.776%
10	6.922	663	669	679	rBV	310457	471628	23.83%	2.382%
11	7.105	694	700	712	rBV	332262	510723	25.81%	2.580%
12	7.193	712	715	721	rVB7	4889	8416	0.43%	0.043%
13	7.575	772	780	789	rBV	334477	535704	27.07%	2.706%
14	7.781	813	815	820	rVB6	1589	2110	0.11%	0.011%
15	8.293	896	902	916	rBV	231523	392121	19.81%	1.981%
16	8.740	971	978	987	rBV	368608	611781	30.91%	3.090%
17	8.869	996	1000	1005	rBV3	10442	15543	0.79%	0.079%
18	9.146	1041	1047	1053	rVB2	13934	22497	1.14%	0.114%
19	9.458	1091	1100	1111	rBV	284782	477765	24.14%	2.413%
20	9.993	1183	1191	1206	rBV	357380	627567	31.71%	3.170%
21	10.116	1210	1212	1214	rVB3	2403	2052	0.10%	0.010%
22	10.363	1247	1254	1262	rVB	456578	733955	37.09%	3.707%
23	10.516	1273	1280	1298	rBV	295154	549360	27.76%	2.775%
24	11.646	1467	1472	1477	rBV2	8069	13015	0.66%	0.066%
25	11.975	1523	1528	1534	rBV4	6770	13954	0.71%	0.070%
26	13.087	1712	1717	1720	rVB7	1601	3068	0.16%	0.015%
27	13.222	1734	1740	1743	rBV8	1930	3861	0.20%	0.020%
28	13.675	1810	1817	1831	rBV	727319	1063487	53.74%	5.372%
29	13.781	1833	1835	1838	rVB4	2119	2525	0.13%	0.013%
30	13.940	1853	1862	1872	rBV	770172	1144296	57.82%	5.780%
31	14.246	1908	1914	1929	rBV	585300	897397	45.34%	4.533%
32	14.487	1948	1955	1966	rBV3	23085	68161	3.44%	0.344%
33	15.069	2050	2054	2056	rBV5	1704	2423	0.12%	0.012%
34	15.251	2079	2085	2102	rBV	988273	1456030	73.57%	7.354%
35	15.387	2102	2108	2122	rVV	324291	472916	23.90%	2.389%
36	15.828	2178	2183	2184	rBV5	2362	2649	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011432.D
 Acq On : 12 Aug 2022 19:50
 Operator : CG/JU
 Sample : N4165-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.987	2207	2210	2217	rBV9	2625	4980	0.25%	0.025%
38	16.157	2235	2239	2245	rBV8	2723	5087	0.26%	0.026%
39	16.504	2292	2298	2303	rBV3	6245	8491	0.43%	0.043%
40	16.692	2327	2330	2335	rBV6	1836	2427	0.12%	0.012%
41	16.804	2345	2349	2354	rBV8	3391	4834	0.24%	0.024%
42	16.969	2373	2377	2380	rBV5	2194	4106	0.21%	0.021%
43	17.022	2380	2386	2397	rVV	766797	1067445	53.94%	5.392%
44	17.122	2397	2403	2430	rVB	1224977	1783695	90.13%	9.009%
45	17.334	2435	2439	2442	rVB5	4152	5725	0.29%	0.029%
46	17.587	2479	2482	2486	rVB3	5478	7667	0.39%	0.039%
47	17.622	2486	2488	2491	rBV4	1721	2232	0.11%	0.011%
48	17.716	2499	2504	2508	rBV7	3288	6675	0.34%	0.034%
49	17.939	2538	2542	2546	rBV3	10815	15826	0.80%	0.080%
50	18.004	2551	2553	2561	rVB2	4164	7415	0.37%	0.037%
51	18.410	2620	2622	2627	rVB6	2672	3016	0.15%	0.015%
52	18.516	2637	2640	2644	rBV3	4766	6486	0.33%	0.033%
53	18.957	2711	2715	2722	rBV3	14917	22159	1.12%	0.112%
54	19.028	2723	2727	2734	rVV2	14961	22747	1.15%	0.115%
55	19.292	2770	2772	2776	rVB5	6430	5311	0.27%	0.027%
56	19.386	2782	2788	2797	rBV	1477250	1966305	99.35%	9.932%
57	21.151	3083	3088	3100	rBV	923208	1185613	59.91%	5.988%
58	23.310	3448	3455	3463	rBV2	1041630	1979098	100.00%	9.996%
59	23.457	3474	3480	3487	rBV2	596022	1115024	56.34%	5.632%




Sum of corrected areas: 19798191

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011432.D
Acq On : 12 Aug 2022 19:50
Operator : CG/JU
Sample : N4165-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

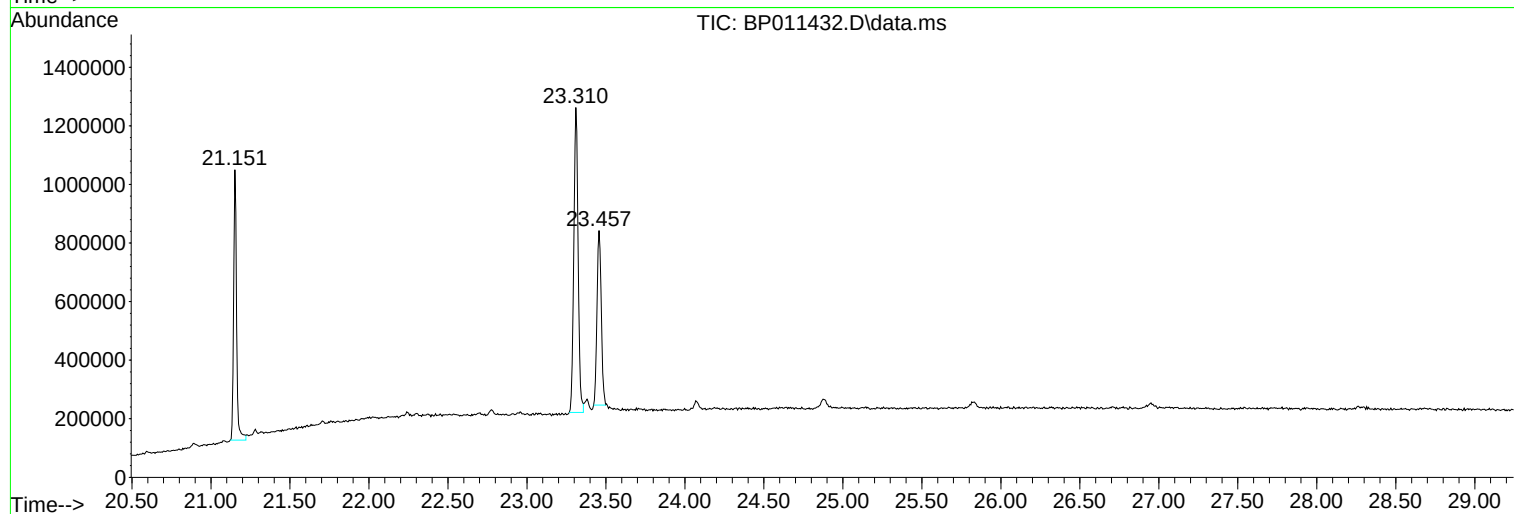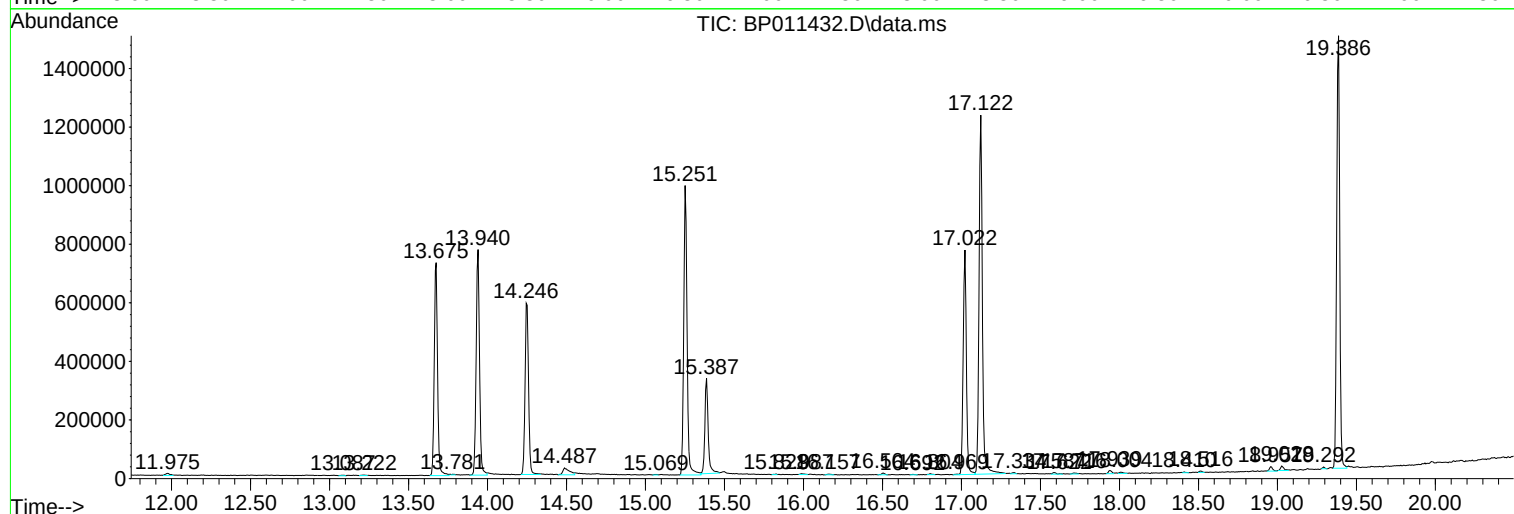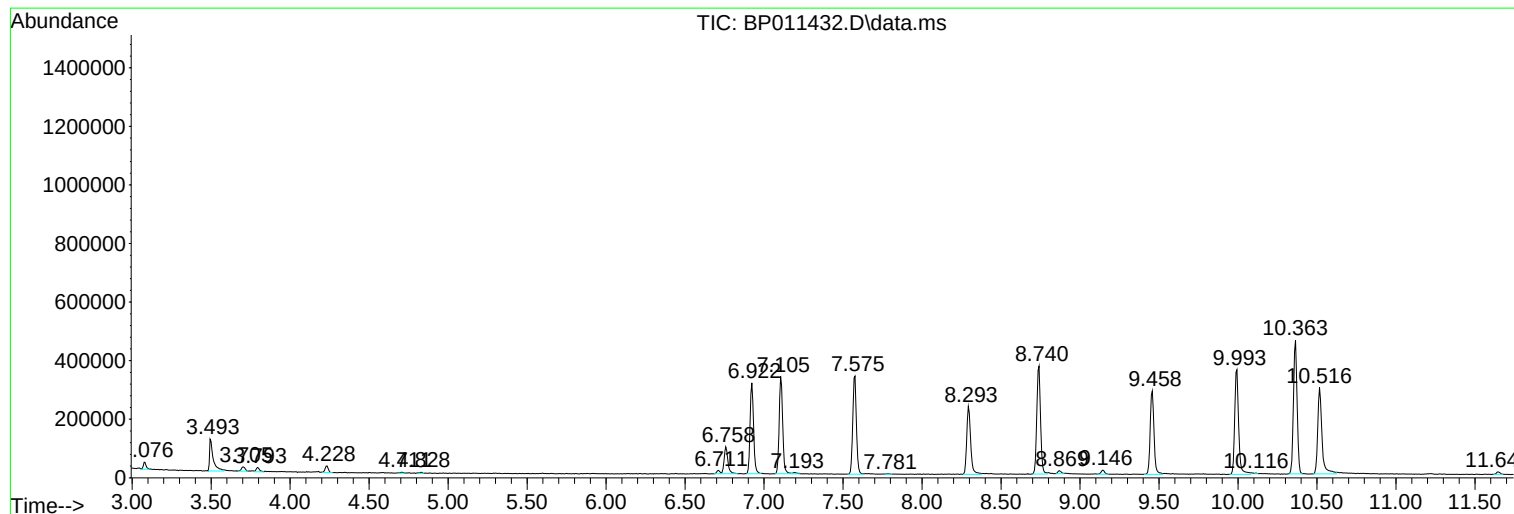

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011432.D
Acq On : 12 Aug 2022 19:50
Operator : CG/JU
Sample : N4165-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011432.D
Acq On : 12 Aug 2022 19:50
Operator : CG/JU
Sample : N4165-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc