

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011433.D
 Acq On : 12 Aug 2022 20:24
 Operator : CG/JU
 Sample : N4165-16
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	24	rVB2	26857	36288	1.63%	0.164%
2	3.493	83	86	99	rBV	112999	173996	7.80%	0.788%
3	3.705	117	122	127	rVB	15334	22340	1.00%	0.101%
4	3.799	134	138	142	rVB2	7074	9758	0.44%	0.044%
5	4.228	207	211	218	rVB	20971	29142	1.31%	0.132%
6	4.575	267	270	274	rBV6	1863	2859	0.13%	0.013%
7	6.611	611	616	619	rBV6	1738	2837	0.13%	0.013%
8	6.710	629	633	636	rBV3	9509	14039	0.63%	0.064%
9	6.758	636	641	656	rVB	85376	135630	6.08%	0.614%
10	6.922	663	669	684	rVB	322984	490168	21.98%	2.219%
11	7.105	693	700	712	rBV	318655	501742	22.50%	2.272%
12	7.193	712	715	718	rVB4	3601	4899	0.22%	0.022%
13	7.575	772	780	790	rBV	356709	575119	25.79%	2.604%
14	8.293	895	902	916	rBV	223205	378282	16.96%	1.713%
15	8.399	918	920	927	rVB7	1801	3683	0.17%	0.017%
16	8.740	970	978	987	rBV	391293	641489	28.77%	2.904%
17	8.869	995	1000	1005	rBV6	8872	16627	0.75%	0.075%
18	9.146	1042	1047	1053	rVB	12412	19218	0.86%	0.087%
19	9.457	1092	1100	1112	rBV	313153	510684	22.90%	2.312%
20	9.993	1183	1191	1204	rBV	369554	655120	29.38%	2.966%
21	10.363	1247	1254	1264	rBV	499380	803671	36.04%	3.639%
22	10.428	1264	1265	1271	rVB6	2215	2387	0.11%	0.011%
23	10.516	1271	1280	1296	rBV	330853	616400	27.64%	2.791%
24	11.646	1466	1472	1479	rVB2	7739	13538	0.61%	0.061%
25	11.810	1496	1500	1505	rBV8	2879	4076	0.18%	0.018%
26	11.969	1521	1527	1536	rBV6	6834	13073	0.59%	0.059%
27	12.316	1581	1586	1589	rBV6	1255	2488	0.11%	0.011%
28	12.857	1670	1678	1680	rVB9	1921	2621	0.12%	0.012%
29	13.069	1711	1714	1720	rVB3	7650	10924	0.49%	0.049%
30	13.157	1722	1729	1733	rVV10	3127	6128	0.27%	0.028%
31	13.216	1735	1739	1746	rVB9	2487	5215	0.23%	0.024%
32	13.487	1780	1785	1787	rBV6	1690	2498	0.11%	0.011%
33	13.675	1810	1817	1833	rBV	832400	1209303	54.23%	5.475%
34	13.781	1833	1835	1839	rVB5	3159	3530	0.16%	0.016%
35	13.940	1855	1862	1884	rBV	890354	1300582	58.32%	5.888%
36	14.163	1896	1900	1906	rVB	15611	20632	0.93%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011433.D
 Acq On : 12 Aug 2022 20:24
 Operator : CG/JU
 Sample : N4165-16
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	14.251	1907	1915	1924	rBV	654451	996807	44.70%	4.513%
38	14.487	1949	1955	1968	rBV3	21416	69857	3.13%	0.316%
39	14.781	2002	2005	2015	rVB3	3462	5655	0.25%	0.026%
40	14.851	2015	2017	2022	rVB5	1630	2293	0.10%	0.010%
41	15.122	2058	2063	2068	rVB	22252	28718	1.29%	0.130%
42	15.251	2078	2085	2102	rBV	1149921	1661102	74.49%	7.520%
43	15.387	2102	2108	2120	rVV	356584	516426	23.16%	2.338%
44	15.492	2123	2126	2130	rVB6	3788	7010	0.31%	0.032%
45	15.686	2156	2159	2164	rVV7	2666	4114	0.18%	0.019%
46	15.739	2166	2168	2172	rVB5	2206	3110	0.14%	0.014%
47	15.828	2179	2183	2186	rBV6	2708	4392	0.20%	0.020%
48	15.992	2206	2211	2219	rVV2	29640	45620	2.05%	0.207%
49	16.151	2235	2238	2241	rBV4	2206	2774	0.12%	0.013%
50	16.504	2292	2298	2303	rVB3	8473	12512	0.56%	0.057%
51	16.575	2307	2310	2312	rBV4	2397	2497	0.11%	0.011%
52	16.745	2338	2339	2344	rBV5	1847	3231	0.14%	0.015%
53	16.792	2344	2347	2352	rVV2	18977	27491	1.23%	0.124%
54	16.845	2352	2356	2360	rVB7	3819	6695	0.30%	0.030%
55	17.022	2380	2386	2396	rBV	863972	1196285	53.65%	5.416%
56	17.122	2396	2403	2419	rVV	1402842	1991562	89.31%	9.017%
57	17.239	2421	2423	2435	rVB	12811	21105	0.95%	0.096%
58	17.539	2470	2474	2478	rBV2	13929	16647	0.75%	0.075%
59	17.581	2478	2481	2485	rVB2	6050	8062	0.36%	0.036%
60	17.722	2500	2505	2508	rBV3	14656	16798	0.75%	0.076%
61	17.939	2538	2542	2547	rBV5	13178	21545	0.97%	0.098%
62	18.010	2551	2554	2558	rVV3	3782	5658	0.25%	0.026%
63	18.228	2587	2591	2595	rVB	8265	9266	0.42%	0.042%
64	18.510	2637	2639	2642	rVB4	3308	3188	0.14%	0.014%
65	18.845	2692	2696	2698	rBV4	9965	12793	0.57%	0.058%
66	18.869	2698	2700	2704	rVB4	8134	7641	0.34%	0.035%
67	18.957	2711	2715	2719	rBV3	16236	22458	1.01%	0.102%
68	19.027	2724	2727	2732	rVB	18028	22923	1.03%	0.104%
69	19.386	2782	2788	2796	rBV	1642137	2229994	100.00%	10.096%
70	21.151	3083	3088	3098	rBV	1021047	1332078	59.73%	6.031%
71	23.310	3448	3455	3463	rBV2	1199686	2229535	99.98%	10.094%
72	23.457	3474	3480	3488	rVB2	710899	1299102	58.26%	5.882%




Sum of corrected areas: 22087930

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011433.D
Acq On : 12 Aug 2022 20:24
Operator : CG/JU
Sample : N4165-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

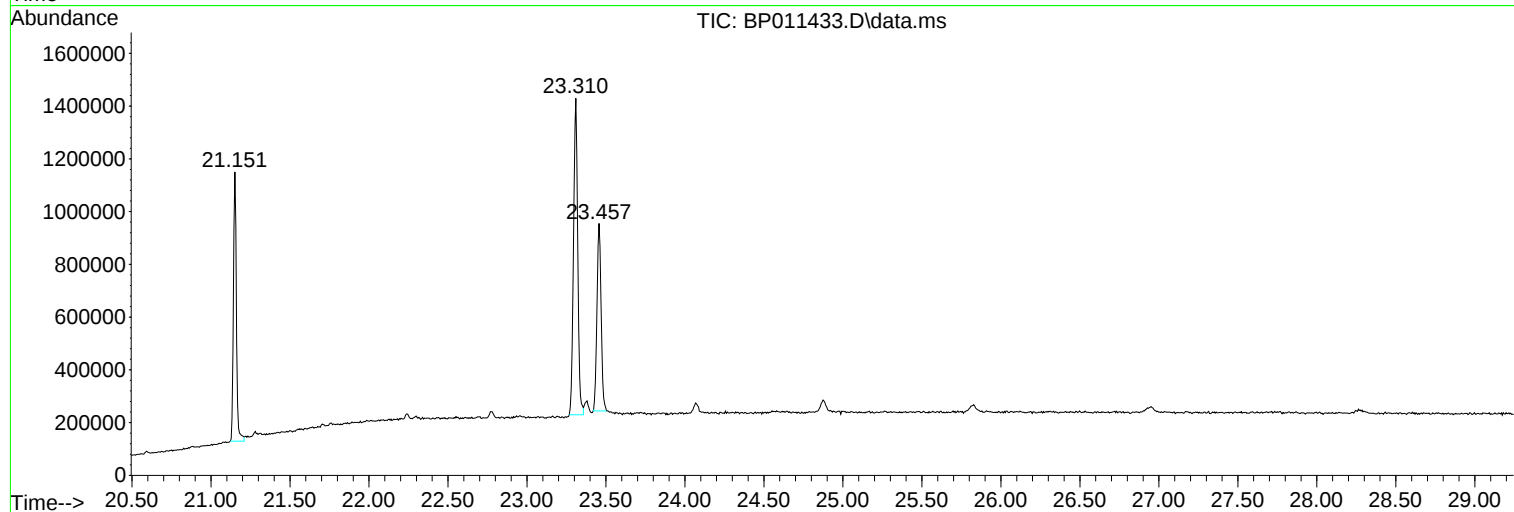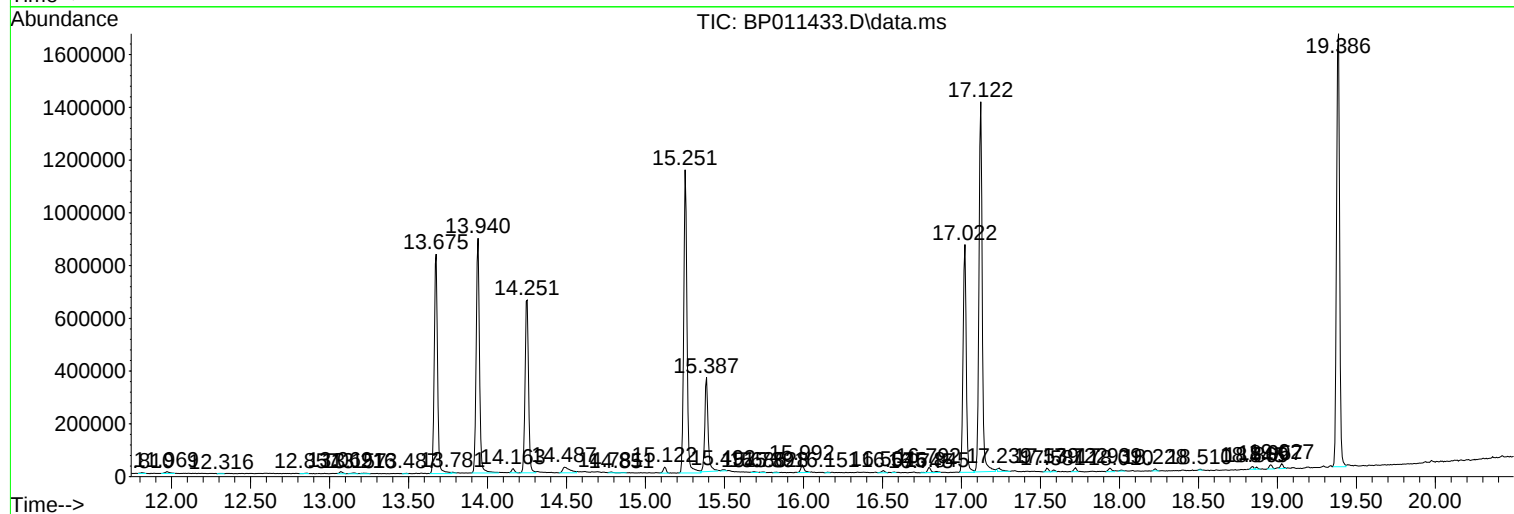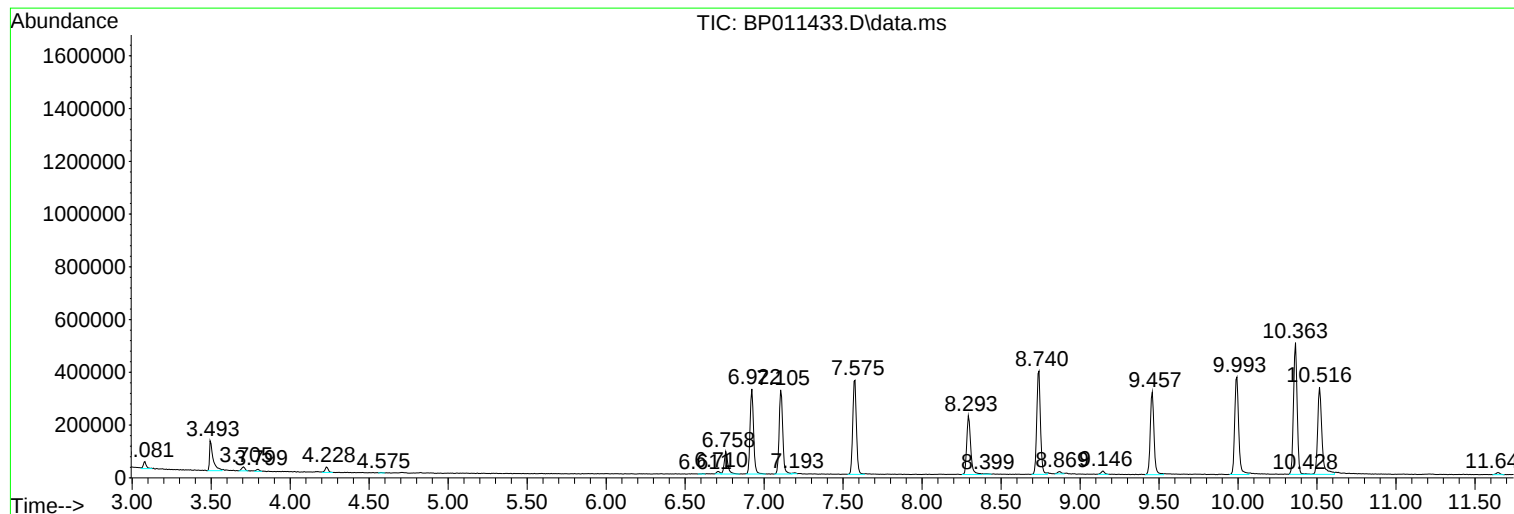

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011433.D
Acq On : 12 Aug 2022 20:24
Operator : CG/JU
Sample : N4165-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011433.D
Acq On : 12 Aug 2022 20:24
Operator : CG/JU
Sample : N4165-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc