

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011435.D
 Acq On : 12 Aug 2022 21:33
 Operator : CG/JU
 Sample : N4165-18
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	12	15	22	rVB	22124	28098	1.44%	0.149%
2	3.499	86	87	96	rBV	53212	79864	4.10%	0.423%
3	3.705	119	122	127	rVB2	10631	14891	0.76%	0.079%
4	3.793	135	137	142	rVB2	9003	10761	0.55%	0.057%
5	4.228	207	211	215	rVB	15843	20753	1.07%	0.110%
6	6.711	628	633	636	rBV	8274	12596	0.65%	0.067%
7	6.758	636	641	651	rVB	49680	83570	4.29%	0.443%
8	6.922	663	669	681	rBV	262366	404837	20.79%	2.144%
9	7.105	694	700	711	rBV	251032	385589	19.80%	2.042%
10	7.352	741	742	747	rBV4	2000	2670	0.14%	0.014%
11	7.569	773	779	788	rBV	355805	562725	28.90%	2.980%
12	8.293	896	902	915	rBV	152200	263022	13.51%	1.393%
13	8.734	970	977	986	rBV	320576	543584	27.92%	2.879%
14	9.140	1042	1046	1051	rVB2	9307	14938	0.77%	0.079%
15	9.457	1091	1100	1108	rBV	237052	403426	20.72%	2.136%
16	9.993	1183	1191	1205	rBV	288392	512595	26.32%	2.715%
17	10.363	1247	1254	1263	rBV	485654	785370	40.33%	4.159%
18	10.516	1271	1280	1298	rBV	261521	496496	25.50%	2.629%
19	11.651	1466	1473	1479	rVB2	6476	12045	0.62%	0.064%
20	11.981	1522	1529	1535	rBV7	5334	12635	0.65%	0.067%
21	12.857	1671	1678	1681	rBV9	1682	2828	0.15%	0.015%
22	13.151	1723	1728	1733	rBV8	1291	2298	0.12%	0.012%
23	13.210	1735	1738	1744	rBV8	2087	3440	0.18%	0.018%
24	13.669	1810	1816	1831	rBV	674308	987660	50.72%	5.230%
25	13.940	1854	1862	1873	rBV	707965	1060504	54.46%	5.616%
26	14.245	1907	1914	1924	rBV	639465	944256	48.49%	5.001%
27	14.498	1951	1957	1968	rBV	10481	36077	1.85%	0.191%
28	14.704	1990	1992	1998	rVB7	1864	2580	0.13%	0.014%
29	15.063	2049	2053	2056	rBV5	2022	3057	0.16%	0.016%
30	15.251	2079	2085	2101	rBV	929377	1358968	69.79%	7.197%
31	15.387	2102	2108	2121	rVV	306889	439034	22.55%	2.325%
32	16.169	2237	2241	2245	rVB6	1581	2143	0.11%	0.011%
33	16.504	2293	2298	2303	rVB4	4699	7092	0.36%	0.038%
34	16.698	2327	2331	2333	rBV4	1716	2030	0.10%	0.011%
35	16.810	2346	2350	2353	rBV6	2482	4206	0.22%	0.022%
36	17.022	2379	2386	2396	rVV	775081	1127598	57.91%	5.972%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011435.D
 Acq On : 12 Aug 2022 21:33
 Operator : CG/JU
 Sample : N4165-18
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	17.122	2397	2403	2429	rVB	1205217	1779196	91.37%	9.422%
38	17.586	2479	2482	2487	rVB4	4485	5320	0.27%	0.028%
39	17.710	2500	2503	2509	rVV8	3296	6025	0.31%	0.032%
40	17.945	2539	2543	2544	rBV4	3717	4426	0.23%	0.023%
41	18.392	2616	2619	2620	rBV3	2697	2586	0.13%	0.014%
42	18.510	2636	2639	2644	rBV6	4323	4870	0.25%	0.026%
43	18.957	2711	2715	2721	rVB5	13990	19137	0.98%	0.101%
44	19.028	2723	2727	2732	rVV2	13545	19756	1.01%	0.105%
45	19.104	2738	2740	2742	rBV2	3464	2611	0.13%	0.014%
46	19.386	2782	2788	2797	rBV	1447733	1947264	100.00%	10.312%
47	21.151	3083	3088	3102	rBV	970578	1289592	66.23%	6.829%
48	23.310	3449	3455	3463	rBV	1056768	1913884	98.29%	10.136%
49	23.457	3474	3480	3491	rVB2	657976	1253906	64.39%	6.640%




Sum of corrected areas: 18882809

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011435.D
Acq On : 12 Aug 2022 21:33
Operator : CG/JU
Sample : N4165-18
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

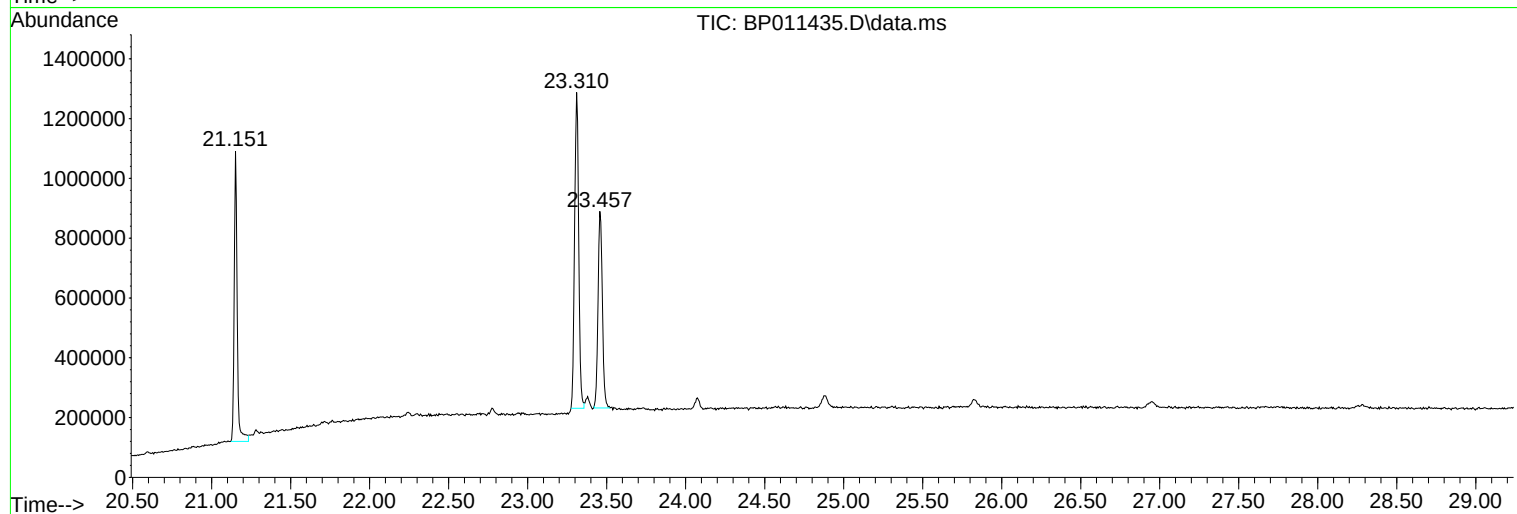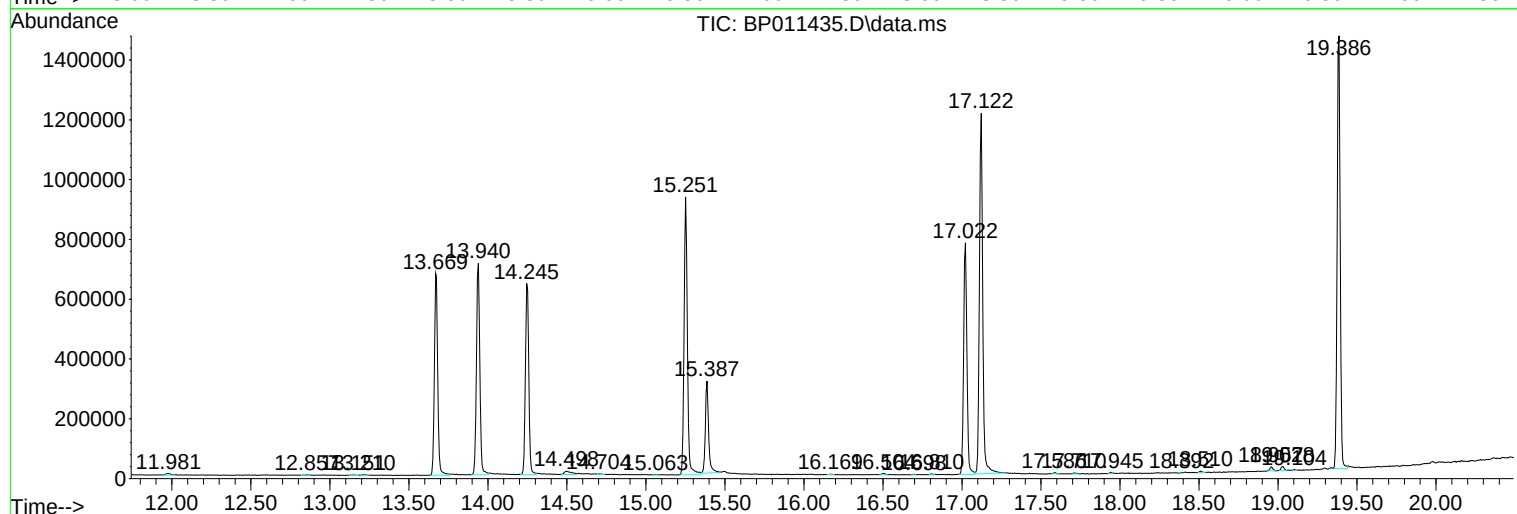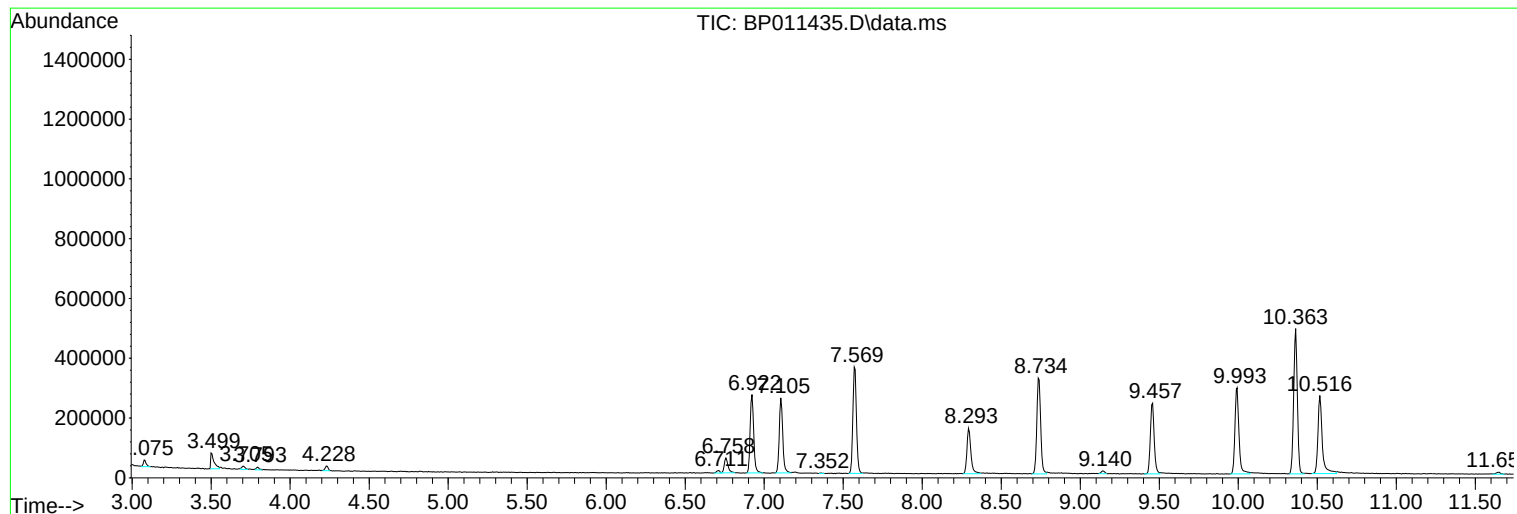

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011435.D
Acq On : 12 Aug 2022 21:33
Operator : CG/JU
Sample : N4165-18
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011435.D
Acq On : 12 Aug 2022 21:33
Operator : CG/JU
Sample : N4165-18
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
