

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011436.D
 Acq On : 12 Aug 2022 22:08
 Operator : CG/JU
 Sample : N4165-19
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	27350	35285	1.60%	0.165%
2	3.499	84	87	99	rBV	80242	124138	5.63%	0.582%
3	3.705	118	122	128	rVB	13705	19418	0.88%	0.091%
4	3.793	134	137	143	rVB3	9712	14195	0.64%	0.067%
5	4.234	207	212	217	rVB	18117	26053	1.18%	0.122%
6	4.699	289	291	294	rBV4	2491	3768	0.17%	0.018%
7	4.823	310	312	318	rVB7	2564	3517	0.16%	0.016%
8	6.711	627	633	636	rBV2	10266	15750	0.71%	0.074%
9	6.758	636	641	650	rVB	65188	109304	4.95%	0.513%
10	6.922	663	669	681	rVB	310881	471754	21.38%	2.212%
11	7.105	693	700	712	rBV	300954	469696	21.29%	2.203%
12	7.187	712	714	719	rVB6	3423	5353	0.24%	0.025%
13	7.575	772	780	790	rBV	366288	586145	26.57%	2.749%
14	8.293	895	902	914	rBV	198862	333441	15.11%	1.564%
15	8.375	914	916	922	rVB7	2561	3653	0.17%	0.017%
16	8.740	967	978	994	rBV	383337	645943	29.28%	3.029%
17	9.146	1039	1047	1053	rVB2	11756	21185	0.96%	0.099%
18	9.458	1093	1100	1109	rBV	287846	478406	21.68%	2.243%
19	9.775	1149	1154	1158	rVB7	1378	2297	0.10%	0.011%
20	9.987	1184	1190	1206	rBV	352698	630520	28.58%	2.957%
21	10.363	1247	1254	1261	rBV	510583	826856	37.47%	3.877%
22	10.516	1273	1280	1297	rBV	303073	568428	25.76%	2.666%
23	11.646	1462	1472	1477	rVB3	7997	13411	0.61%	0.063%
24	11.975	1524	1528	1536	rVB4	7119	12911	0.59%	0.061%
25	13.228	1735	1741	1744	rVB7	1838	3393	0.15%	0.016%
26	13.669	1810	1816	1829	rBV	781920	1127776	51.11%	5.288%
27	13.940	1854	1862	1881	rBV	829134	1250640	56.68%	5.865%
28	14.246	1908	1914	1924	rBV	695482	1025371	46.47%	4.808%
29	14.493	1951	1956	1960	rBV3	13220	27875	1.26%	0.131%
30	15.063	2051	2053	2057	rBV5	2000	2276	0.10%	0.011%
31	15.251	2077	2085	2102	rBV	1062955	1555980	70.52%	7.296%
32	15.387	2102	2108	2123	rVV	351010	501775	22.74%	2.353%
33	16.051	2217	2221	2223	rVB5	2021	2576	0.12%	0.012%
34	16.504	2294	2298	2302	rBV3	4744	6650	0.30%	0.031%
35	16.692	2328	2330	2337	rVB8	3028	2655	0.12%	0.012%
36	16.804	2345	2349	2354	rBV8	2775	4306	0.20%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011436.D
 Acq On : 12 Aug 2022 22:08
 Operator : CG/JU
 Sample : N4165-19
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	17.022	2379	2386	2397	rBV	847747	1227937	55.65%	5.758%
38	17.122	2397	2403	2425	rVV	1371389	2000999	90.69%	9.383%
39	17.275	2427	2429	2432	rVB4	3128	3329	0.15%	0.016%
40	17.416	2448	2453	2456	rBV6	2573	4629	0.21%	0.022%
41	17.587	2478	2482	2489	rBV6	6157	10640	0.48%	0.050%
42	17.934	2538	2541	2546	rBV6	4391	8859	0.40%	0.042%
43	18.010	2551	2554	2559	rBV5	3497	5411	0.25%	0.025%
44	18.269	2594	2598	2599	rBV4	1769	2239	0.10%	0.010%
45	18.404	2617	2621	2622	rBV3	2784	4364	0.20%	0.020%
46	18.510	2636	2639	2643	rBV5	4207	4598	0.21%	0.022%
47	18.957	2711	2715	2720	rVB2	15479	19520	0.88%	0.092%
48	19.028	2723	2727	2731	rBV3	15742	21668	0.98%	0.102%
49	19.339	2777	2780	2781	rBV3	4860	4913	0.22%	0.023%
50	19.386	2782	2788	2796	rVV	1649468	2177148	98.67%	10.209%
51	19.639	2828	2831	2835	rVB5	12495	15237	0.69%	0.071%
52	21.151	3083	3088	3096	rBV	1061163	1345744	60.99%	6.311%
53	23.310	3448	3455	3464	rBV2	1187051	2206439	100.00%	10.347%
54	23.457	3474	3480	3488	rVB2	722445	1328701	60.22%	6.231%




Sum of corrected areas: 21325075

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011436.D
Acq On : 12 Aug 2022 22:08
Operator : CG/JU
Sample : N4165-19
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

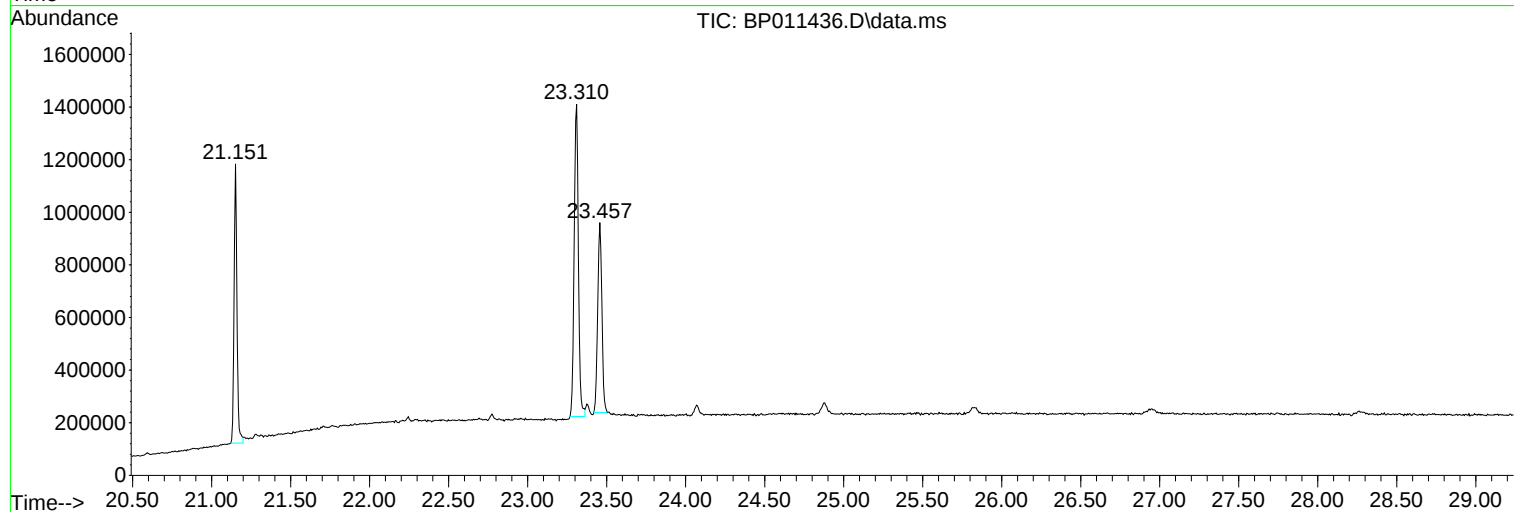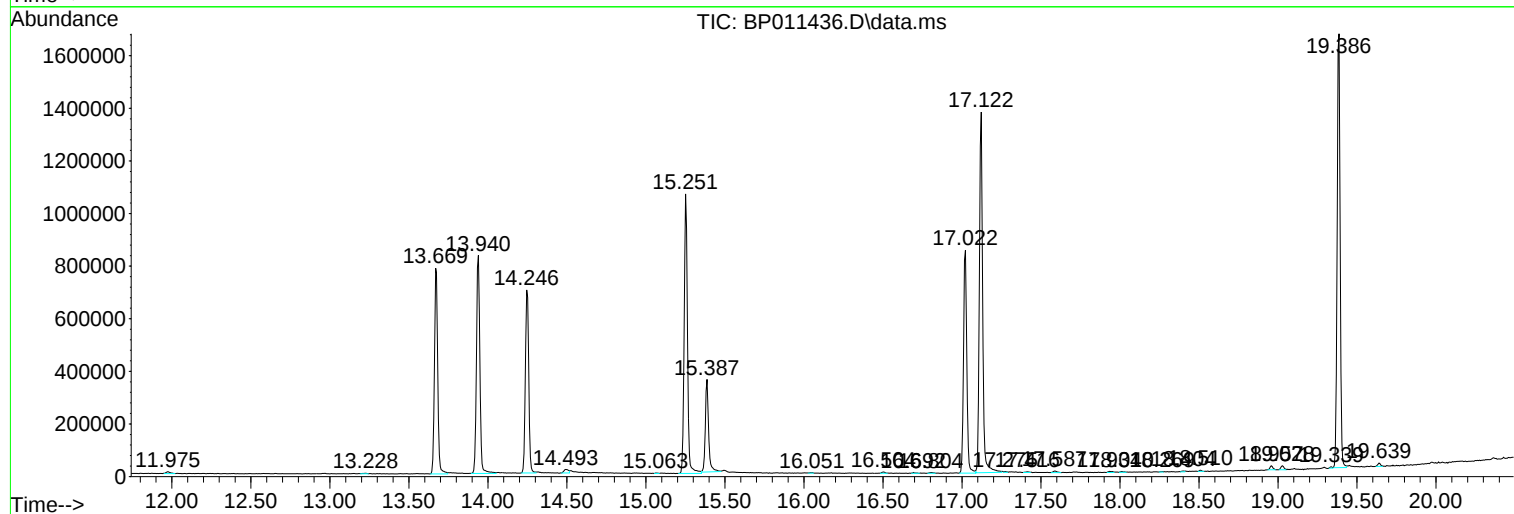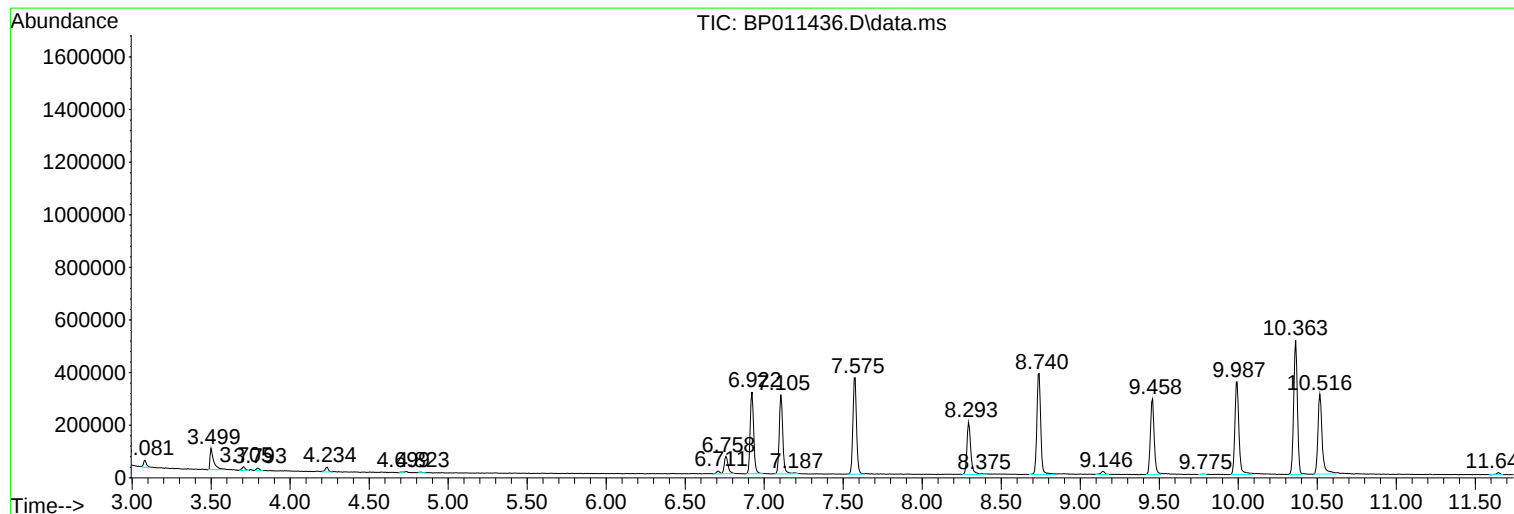

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011436.D
Acq On : 12 Aug 2022 22:08
Operator : CG/JU
Sample : N4165-19
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011436.D
Acq On : 12 Aug 2022 22:08
Operator : CG/JU
Sample : N4165-19
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc