

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011437.D
 Acq On : 12 Aug 2022 22:42
 Operator : CG/JU
 Sample : N4166-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	6	9	13	rVV4	10798	13364	0.55%	0.058%
2	3.081	13	16	22	rVB	26899	33812	1.39%	0.146%
3	3.493	83	86	102	rBV	128511	208129	8.58%	0.901%
4	3.705	118	122	127	rVB	13768	21836	0.90%	0.095%
5	3.793	134	137	144	rVB2	9361	12964	0.53%	0.056%
6	4.228	208	211	216	rVB	20378	25060	1.03%	0.109%
7	4.711	290	293	297	rBV6	2131	2980	0.12%	0.013%
8	4.822	309	312	317	rVB7	3111	5728	0.24%	0.025%
9	6.711	628	633	636	rBV2	10115	13934	0.57%	0.060%
10	6.758	636	641	654	rVB	66630	109400	4.51%	0.474%
11	6.922	662	669	681	rBV	320097	495963	20.45%	2.148%
12	7.105	694	700	713	rBV	299921	463652	19.11%	2.008%
13	7.187	713	714	719	rVB5	2850	3308	0.14%	0.014%
14	7.569	771	779	791	rBV	397335	636151	26.22%	2.755%
15	7.787	813	816	820	rVB5	2444	2872	0.12%	0.012%
16	8.293	895	902	916	rBV	199835	332728	13.72%	1.441%
17	8.734	970	977	992	rBV	396366	664359	27.39%	2.877%
18	9.146	1039	1047	1053	rVB3	10544	18915	0.78%	0.082%
19	9.457	1090	1100	1112	rBV	281531	476500	19.64%	2.064%
20	9.987	1184	1190	1206	rBV	359954	629000	25.93%	2.724%
21	10.363	1246	1254	1263	rBV	540100	895985	36.94%	3.880%
22	10.516	1273	1280	1299	rBV	345970	656384	27.06%	2.843%
23	11.246	1403	1404	1409	rVB5	2012	2551	0.11%	0.011%
24	11.646	1468	1472	1478	rVB2	8497	15155	0.62%	0.066%
25	11.975	1520	1528	1536	rBV3	7779	17525	0.72%	0.076%
26	12.969	1692	1697	1699	rBV5	1340	2459	0.10%	0.011%
27	13.145	1723	1727	1734	rVB8	2382	4340	0.18%	0.019%
28	13.669	1809	1816	1840	rBV	848977	1230502	50.73%	5.329%
29	13.940	1855	1862	1876	rBV	856800	1304327	53.77%	5.649%
30	14.245	1907	1914	1932	rBV	763567	1118226	46.10%	4.843%
31	14.492	1951	1956	1972	rBV4	16898	56693	2.34%	0.246%
32	15.116	2060	2062	2069	rVB8	2376	3802	0.16%	0.016%
33	15.251	2077	2085	2101	rBV	1164582	1677871	69.17%	7.266%
34	15.387	2102	2108	2122	rVV	340985	517029	21.31%	2.239%
35	15.492	2124	2126	2130	rVB4	6697	8149	0.34%	0.035%
36	15.987	2205	2210	2218	rBV4	7397	15111	0.62%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011437.D
 Acq On : 12 Aug 2022 22:42
 Operator : CG/JU
 Sample : N4166-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.039	2218	2219	2227	rVB8	3216	3310	0.14%	0.014%
38	16.504	2294	2298	2302	rBV	5571	7659	0.32%	0.033%
39	16.798	2343	2348	2354	rBV8	5757	10734	0.44%	0.046%
40	16.904	2364	2366	2373	rVB8	2169	3424	0.14%	0.015%
41	16.969	2373	2377	2379	rBV5	2859	3860	0.16%	0.017%
42	17.022	2379	2386	2396	rBV	932233	1321423	54.47%	5.723%
43	17.122	2396	2403	2425	rVB	1441590	2084038	85.91%	9.025%
44	17.586	2479	2482	2488	rVB5	5987	7682	0.32%	0.033%
45	17.710	2498	2503	2507	rBV8	4389	8588	0.35%	0.037%
46	17.933	2539	2541	2546	rBV6	2922	4239	0.17%	0.018%
47	18.010	2551	2554	2557	rBV3	5589	6175	0.25%	0.027%
48	18.228	2589	2591	2595	rBV5	1978	2617	0.11%	0.011%
49	18.510	2636	2639	2644	rBV6	5559	8587	0.35%	0.037%
50	18.957	2711	2715	2721	rBV4	17357	26649	1.10%	0.115%
51	19.028	2723	2727	2732	rVV2	16899	23909	0.99%	0.104%
52	19.286	2769	2771	2775	rBV2	4757	5701	0.24%	0.025%
53	19.333	2777	2779	2782	rBV4	6283	6264	0.26%	0.027%
54	19.380	2782	2787	2797	rBV	1786250	2356925	97.16%	10.207%
55	21.080	3073	3076	3081	rBV2	35337	40647	1.68%	0.176%
56	21.151	3083	3088	3099	rBV	1169899	1506028	62.08%	6.522%
57	23.310	3448	3455	3463	rBV2	1297630	2425764	100.00%	10.505%
58	23.457	3473	3480	3492	rVB2	779052	1529715	63.06%	6.625%




Sum of corrected areas: 23090702

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

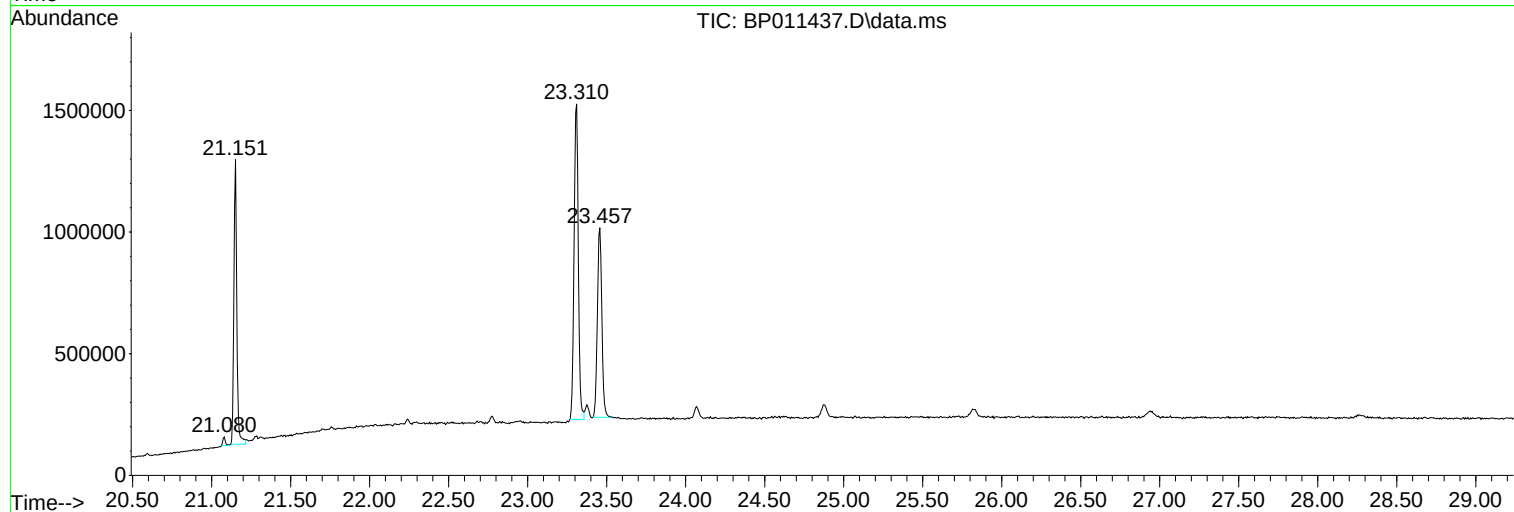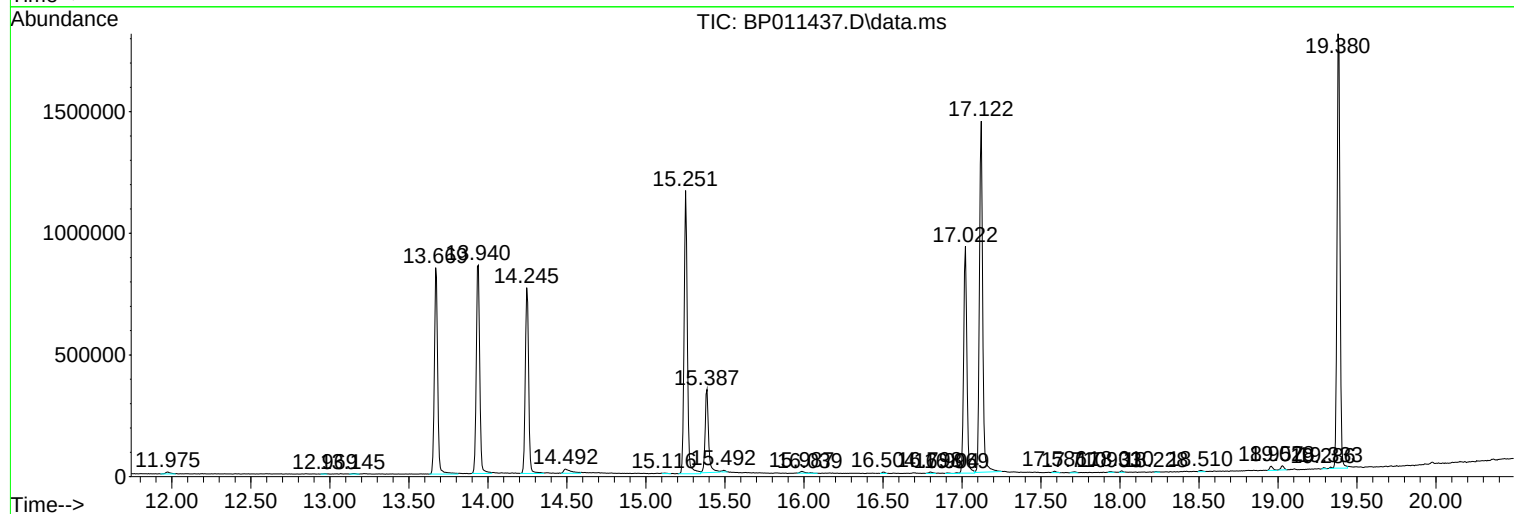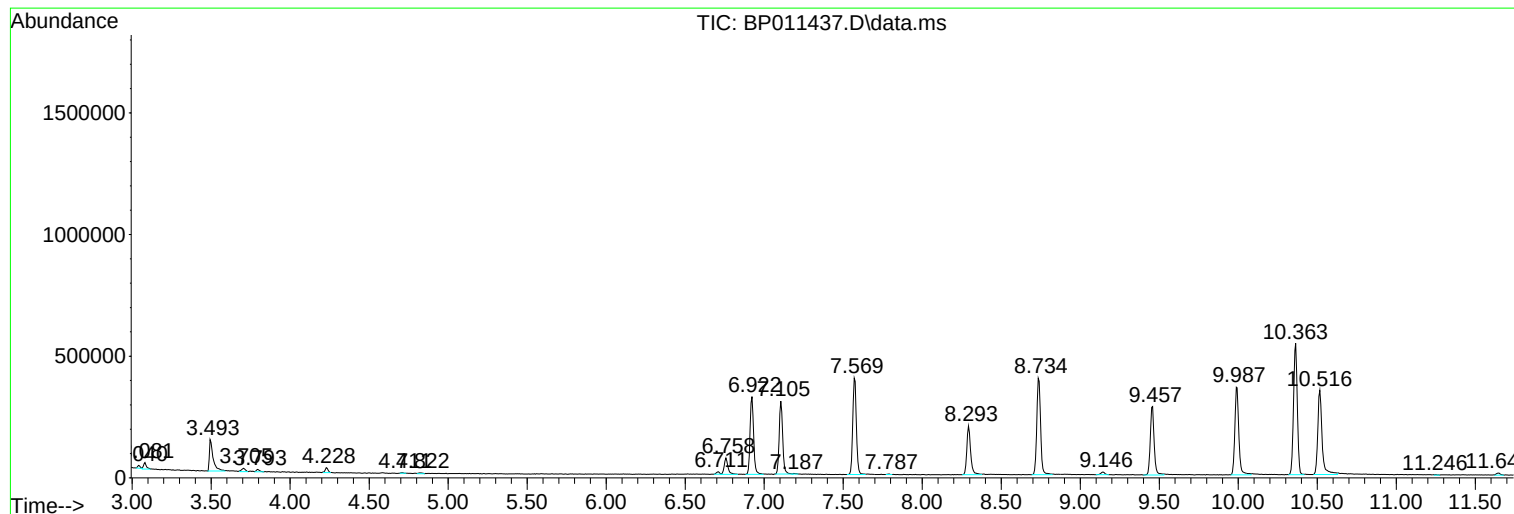

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc