

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011439.D
 Acq On : 12 Aug 2022 23:51
 Operator : CG/JU
 Sample : N4166-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	24	rVB	27631	36113	1.57%	0.160%
2	3.493	84	86	100	rBV	106106	167605	7.27%	0.742%
3	3.705	117	122	128	rVB	13647	20937	0.91%	0.093%
4	3.799	135	138	143	rVB3	10199	12829	0.56%	0.057%
5	4.228	207	211	216	rVB	16924	23567	1.02%	0.104%
6	4.822	308	312	315	rBV6	3355	4563	0.20%	0.020%
7	6.246	549	554	557	rBV5	5352	9200	0.40%	0.041%
8	6.705	626	632	636	rBV3	9413	13641	0.59%	0.060%
9	6.758	636	641	649	rVV	69709	108524	4.71%	0.480%
10	6.922	662	669	678	rBV	320311	491124	21.30%	2.173%
11	7.105	693	700	710	rBV	311912	475870	20.64%	2.106%
12	7.187	713	714	719	rVB5	4204	4433	0.19%	0.020%
13	7.569	772	779	788	rBV	388045	600696	26.05%	2.658%
14	7.652	788	793	799	rVB9	4878	10543	0.46%	0.047%
15	7.787	811	816	821	rVV8	3494	5015	0.22%	0.022%
16	7.875	825	831	837	rVB8	7322	12344	0.54%	0.055%
17	8.293	895	902	912	rBV	214433	354527	15.38%	1.569%
18	8.734	970	977	985	rBV	401450	658394	28.55%	2.914%
19	8.922	1009	1013	1013	rVB5	2542	2511	0.11%	0.011%
20	9.140	1041	1046	1052	rVB2	13786	21787	0.94%	0.096%
21	9.452	1091	1099	1108	rBV	303331	501449	21.75%	2.219%
22	9.846	1160	1166	1172	rBV7	5296	9457	0.41%	0.042%
23	9.987	1183	1190	1208	rBV	390390	674964	29.27%	2.987%
24	10.157	1215	1219	1226	rVV9	3938	7925	0.34%	0.035%
25	10.234	1226	1232	1237	rVB10	2876	7152	0.31%	0.032%
26	10.363	1246	1254	1261	rBV	517018	845123	36.65%	3.740%
27	10.516	1271	1280	1302	rBV	315988	614181	26.64%	2.718%
28	11.210	1396	1398	1403	rVB6	2236	2659	0.12%	0.012%
29	11.651	1466	1473	1480	rVB2	8482	16127	0.70%	0.071%
30	11.798	1493	1498	1502	rVB8	2643	4132	0.18%	0.018%
31	11.969	1518	1527	1534	rBV4	7915	16575	0.72%	0.073%
32	12.598	1629	1634	1637	rBV6	2761	3664	0.16%	0.016%
33	12.857	1674	1678	1685	rVB7	2927	5270	0.23%	0.023%
34	12.963	1690	1696	1699	rBV8	1804	3142	0.14%	0.014%
35	13.151	1724	1728	1733	rVB8	2332	4608	0.20%	0.020%
36	13.210	1733	1738	1739	rBV5	2295	3503	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011439.D
 Acq On : 12 Aug 2022 23:51
 Operator : CG/JU
 Sample : N4166-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	13.492	1783	1786	1790	rVB5	1776	2583	0.11%	0.011%
38	13.669	1809	1816	1830	rBV	905770	1263278	54.79%	5.591%
39	13.934	1854	1861	1877	rBV	906529	1351158	58.60%	5.979%
40	14.245	1908	1914	1927	rBV	737303	1047828	45.44%	4.637%
41	14.487	1948	1955	1972	rBV5	19455	68971	2.99%	0.305%
42	14.692	1988	1990	1996	rVB7	3570	5881	0.26%	0.026%
43	15.069	2050	2054	2061	rBV3	5198	8317	0.36%	0.037%
44	15.251	2077	2085	2098	rBV	1175299	1708038	74.08%	7.559%
45	15.381	2102	2107	2122	rVV	366392	552517	23.96%	2.445%
46	15.486	2122	2125	2132	rVB7	7689	15857	0.69%	0.070%
47	15.981	2204	2209	2217	rVV2	24009	44255	1.92%	0.196%
48	16.039	2217	2219	2224	rVB6	2676	4532	0.20%	0.020%
49	16.163	2235	2240	2249	rBV6	2514	6013	0.26%	0.027%
50	16.504	2293	2298	2305	rBV2	6172	8700	0.38%	0.039%
51	16.798	2344	2348	2355	rBV10	3576	7193	0.31%	0.032%
52	16.963	2371	2376	2379	rBV7	2292	3696	0.16%	0.016%
53	17.022	2379	2386	2396	rBV	856756	1234885	53.56%	5.465%
54	17.122	2396	2403	2420	rVV	1365864	2024927	87.82%	8.961%
55	17.333	2435	2439	2445	rVB2	5599	8422	0.37%	0.037%
56	17.586	2478	2482	2488	rBV6	5705	9234	0.40%	0.041%
57	17.716	2501	2504	2508	rBV6	2240	3374	0.15%	0.015%
58	17.851	2525	2527	2531	rBV5	1965	2358	0.10%	0.010%
59	17.939	2538	2542	2547	rBV4	15272	22615	0.98%	0.100%
60	18.010	2552	2554	2559	rVB5	2150	2983	0.13%	0.013%
61	18.345	2609	2611	2615	rVB4	2645	3187	0.14%	0.014%
62	18.510	2636	2639	2644	rBV5	4692	6460	0.28%	0.029%
63	18.957	2711	2715	2719	rBV3	17647	23185	1.01%	0.103%
64	19.027	2723	2727	2733	rVV	18046	26199	1.14%	0.116%
65	19.104	2737	2740	2741	rBV3	4508	3940	0.17%	0.017%
66	19.186	2752	2754	2757	rBV4	5105	4551	0.20%	0.020%
67	19.333	2777	2779	2781	rBV3	5330	5165	0.22%	0.023%
68	19.386	2782	2788	2797	rVV	1714387	2271343	98.51%	10.052%
69	21.151	3083	3088	3100	rBV	1092934	1376707	59.71%	6.092%
70	23.310	3448	3455	3462	rBV	1248372	2305766	100.00%	10.204%
71	23.457	3474	3480	3495	rVB2	725631	1408503	61.09%	6.233%




Sum of corrected areas: 22596775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011439.D
Acq On : 12 Aug 2022 23:51
Operator : CG/JU
Sample : N4166-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

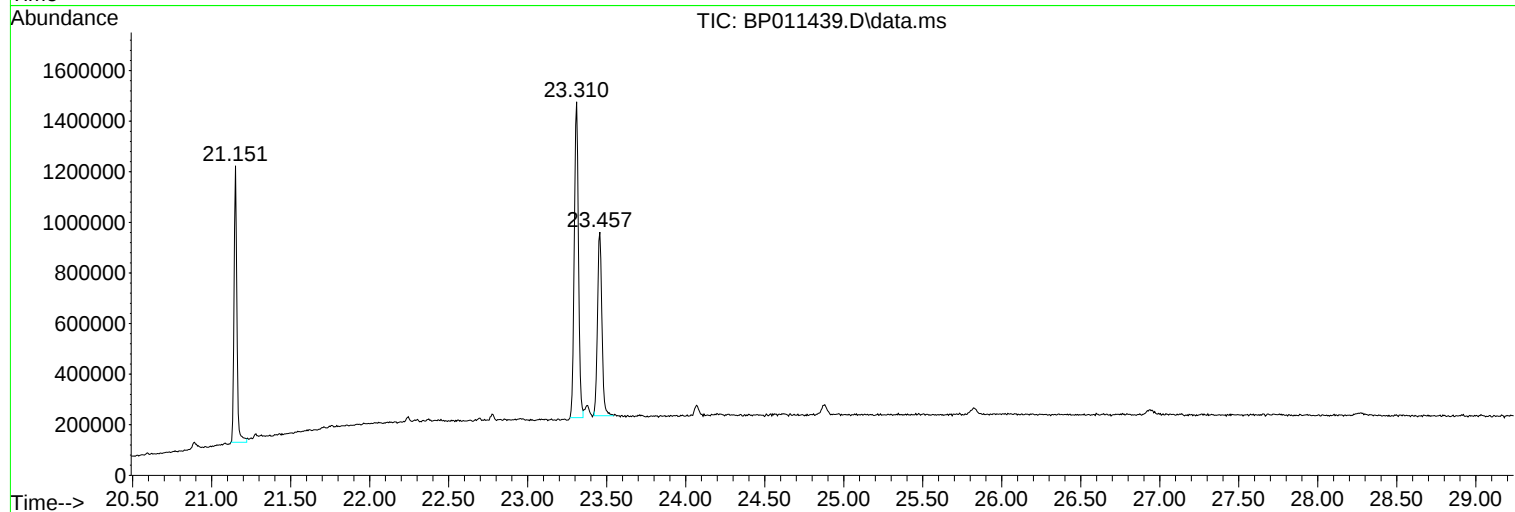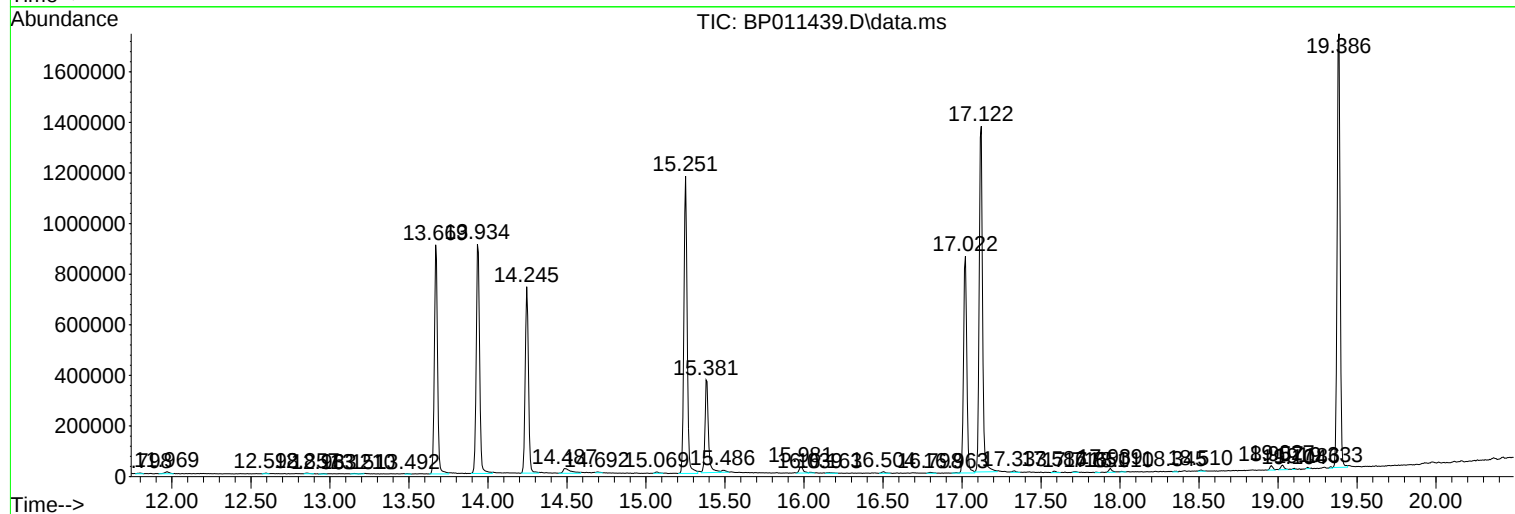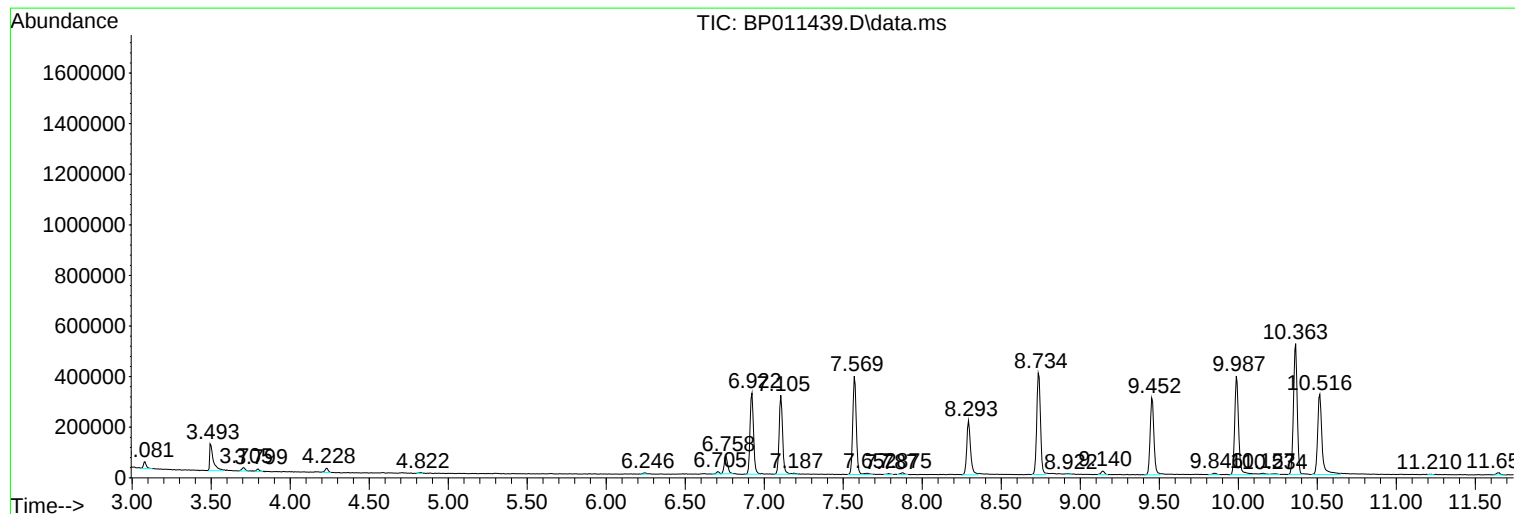

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011439.D
Acq On : 12 Aug 2022 23:51
Operator : CG/JU
Sample : N4166-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011439.D
Acq On : 12 Aug 2022 23:51
Operator : CG/JU
Sample : N4166-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc