
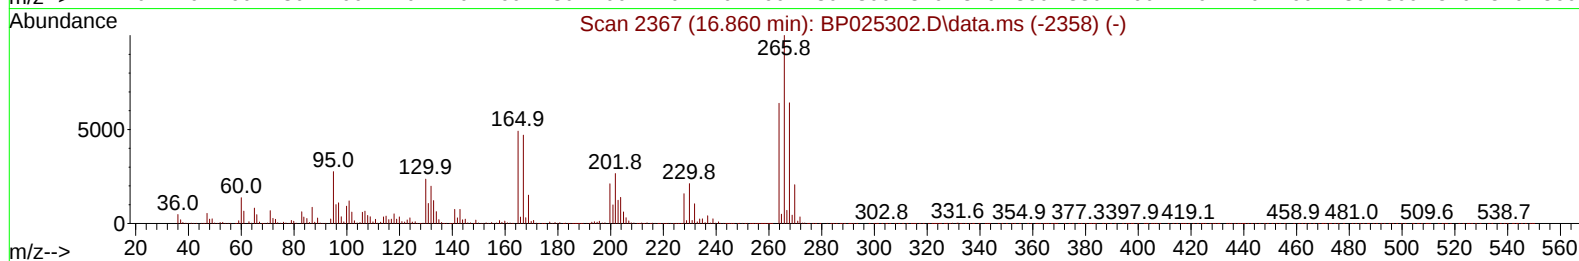
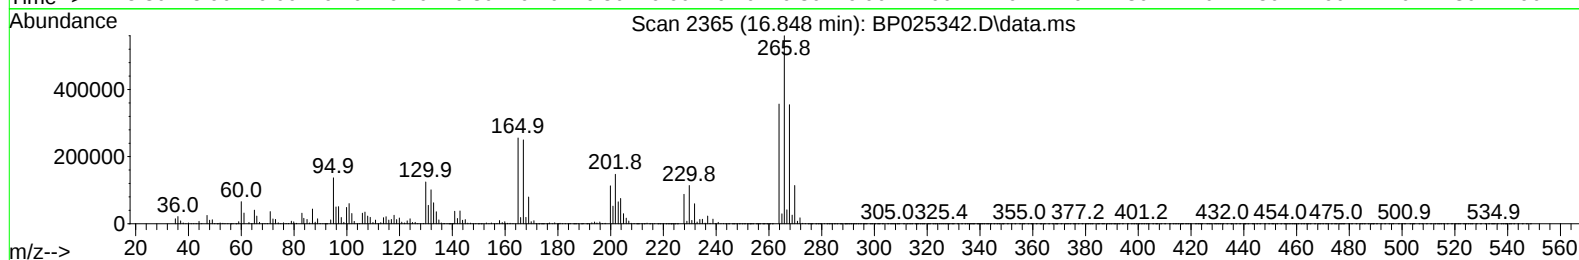


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025342.D
Acq On : 11 Aug 2025 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 12:20:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

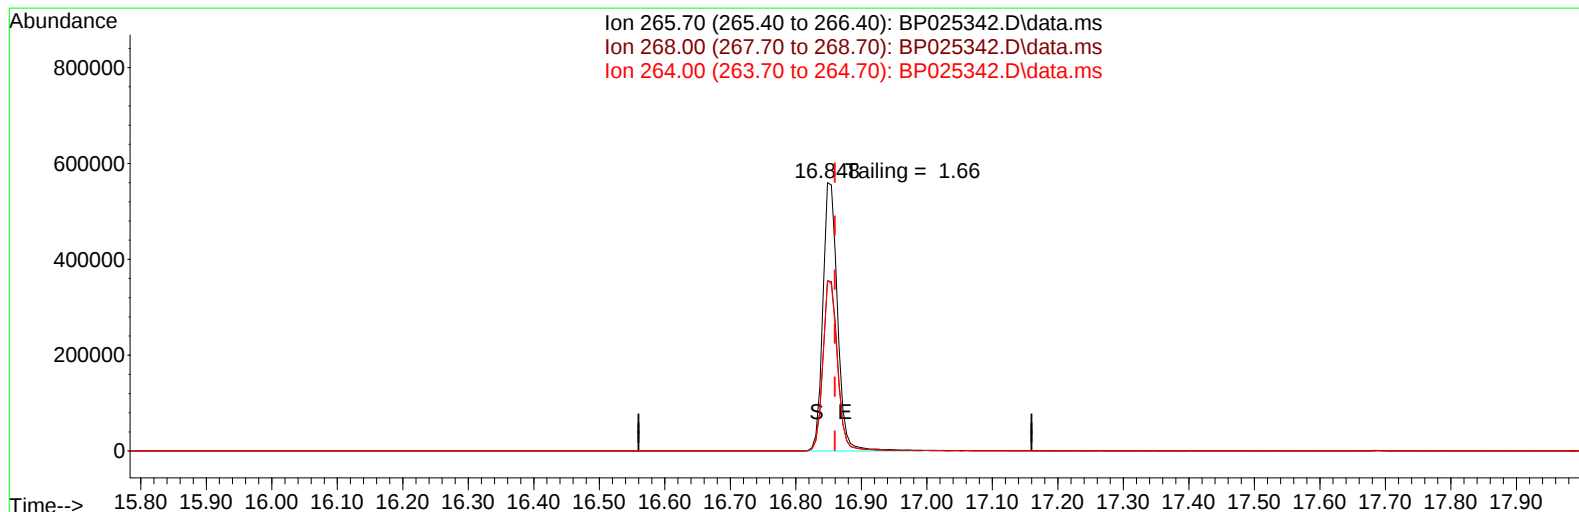

TIC: BP025342.D\data.ms

(70) Pentachlorophenol (C)




16.848min (-0.012) 2299749.99 ng

response 876713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.31
264.00	63.90	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025342.D
Acq On : 11 Aug 2025 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 12:20:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

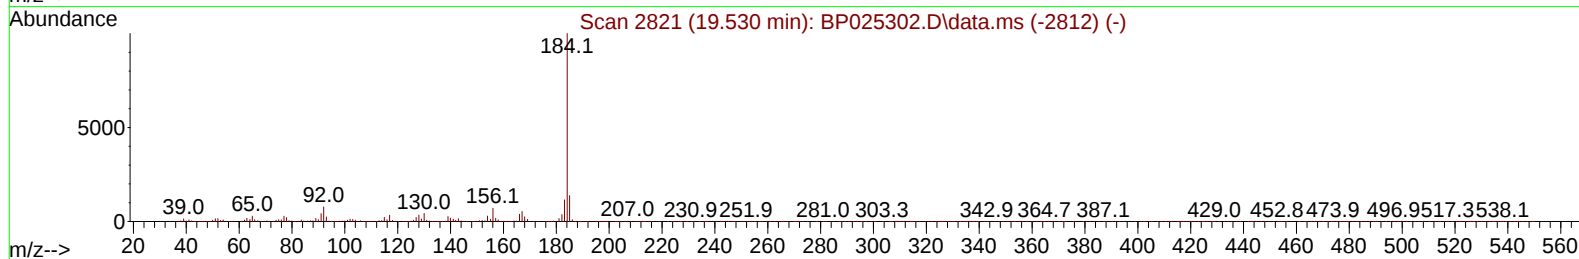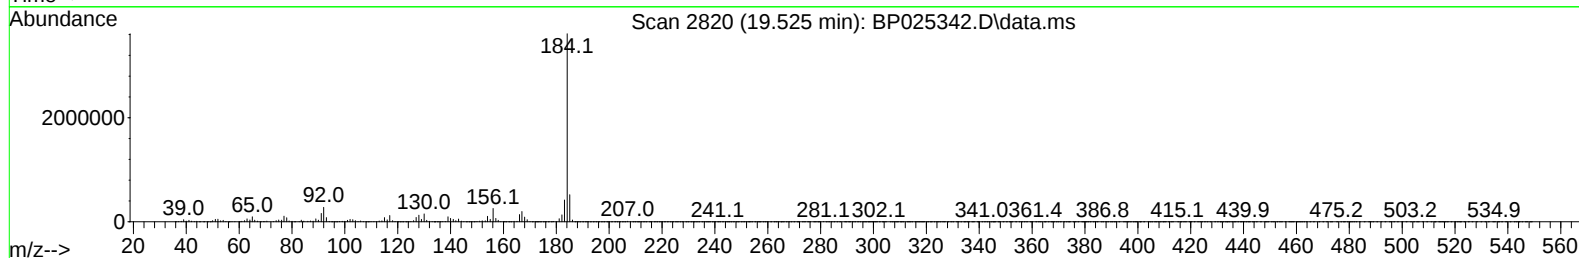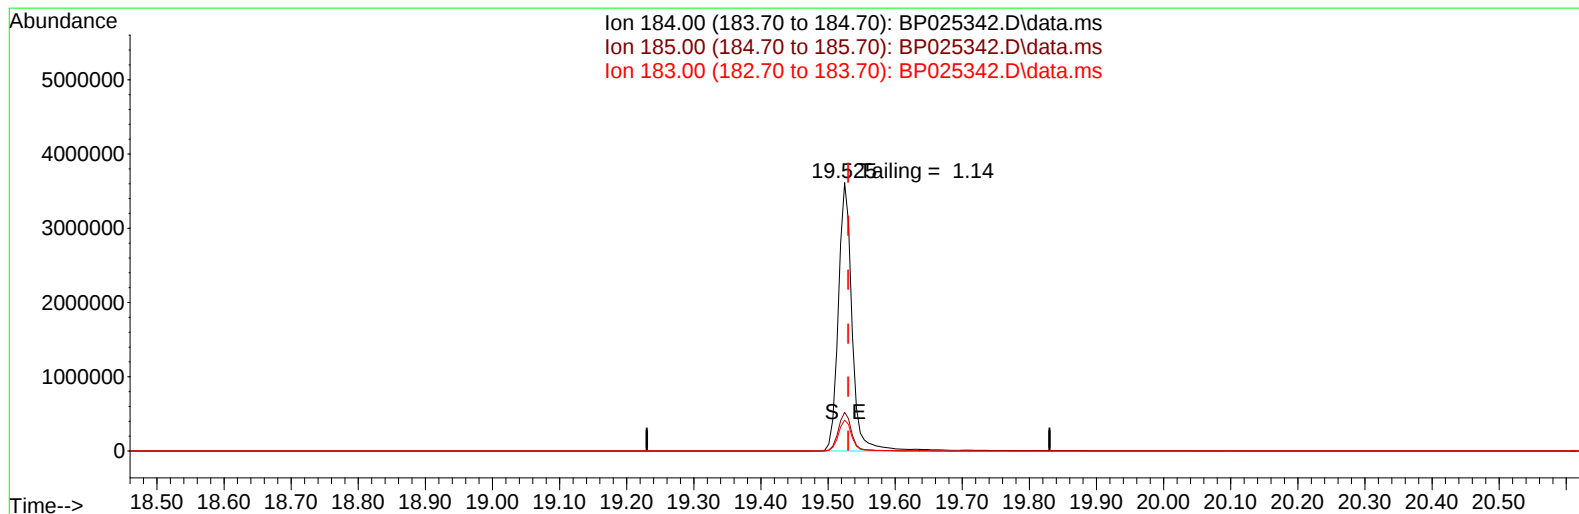

TIC: BP025342.D\data.ms

(77) Benzidine**19.525min (-0.005) 1639801.98 ng****response 5104250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.42
183.00	11.50	11.55
0.00	0.00	0.00