

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
 Data File : BP025351.D
 Acq On : 11 Aug 2025 16:47
 Operator : CG/JU
 Sample : Q2798-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-6


Quant Time: Aug 11 17:14:06 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 06 06:41:44 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	2			

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025351.D
Acq On : 11 Aug 2025 16:47
Operator : CG/JU
Sample : Q2798-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-6

Quant Time: Aug 11 17:14:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

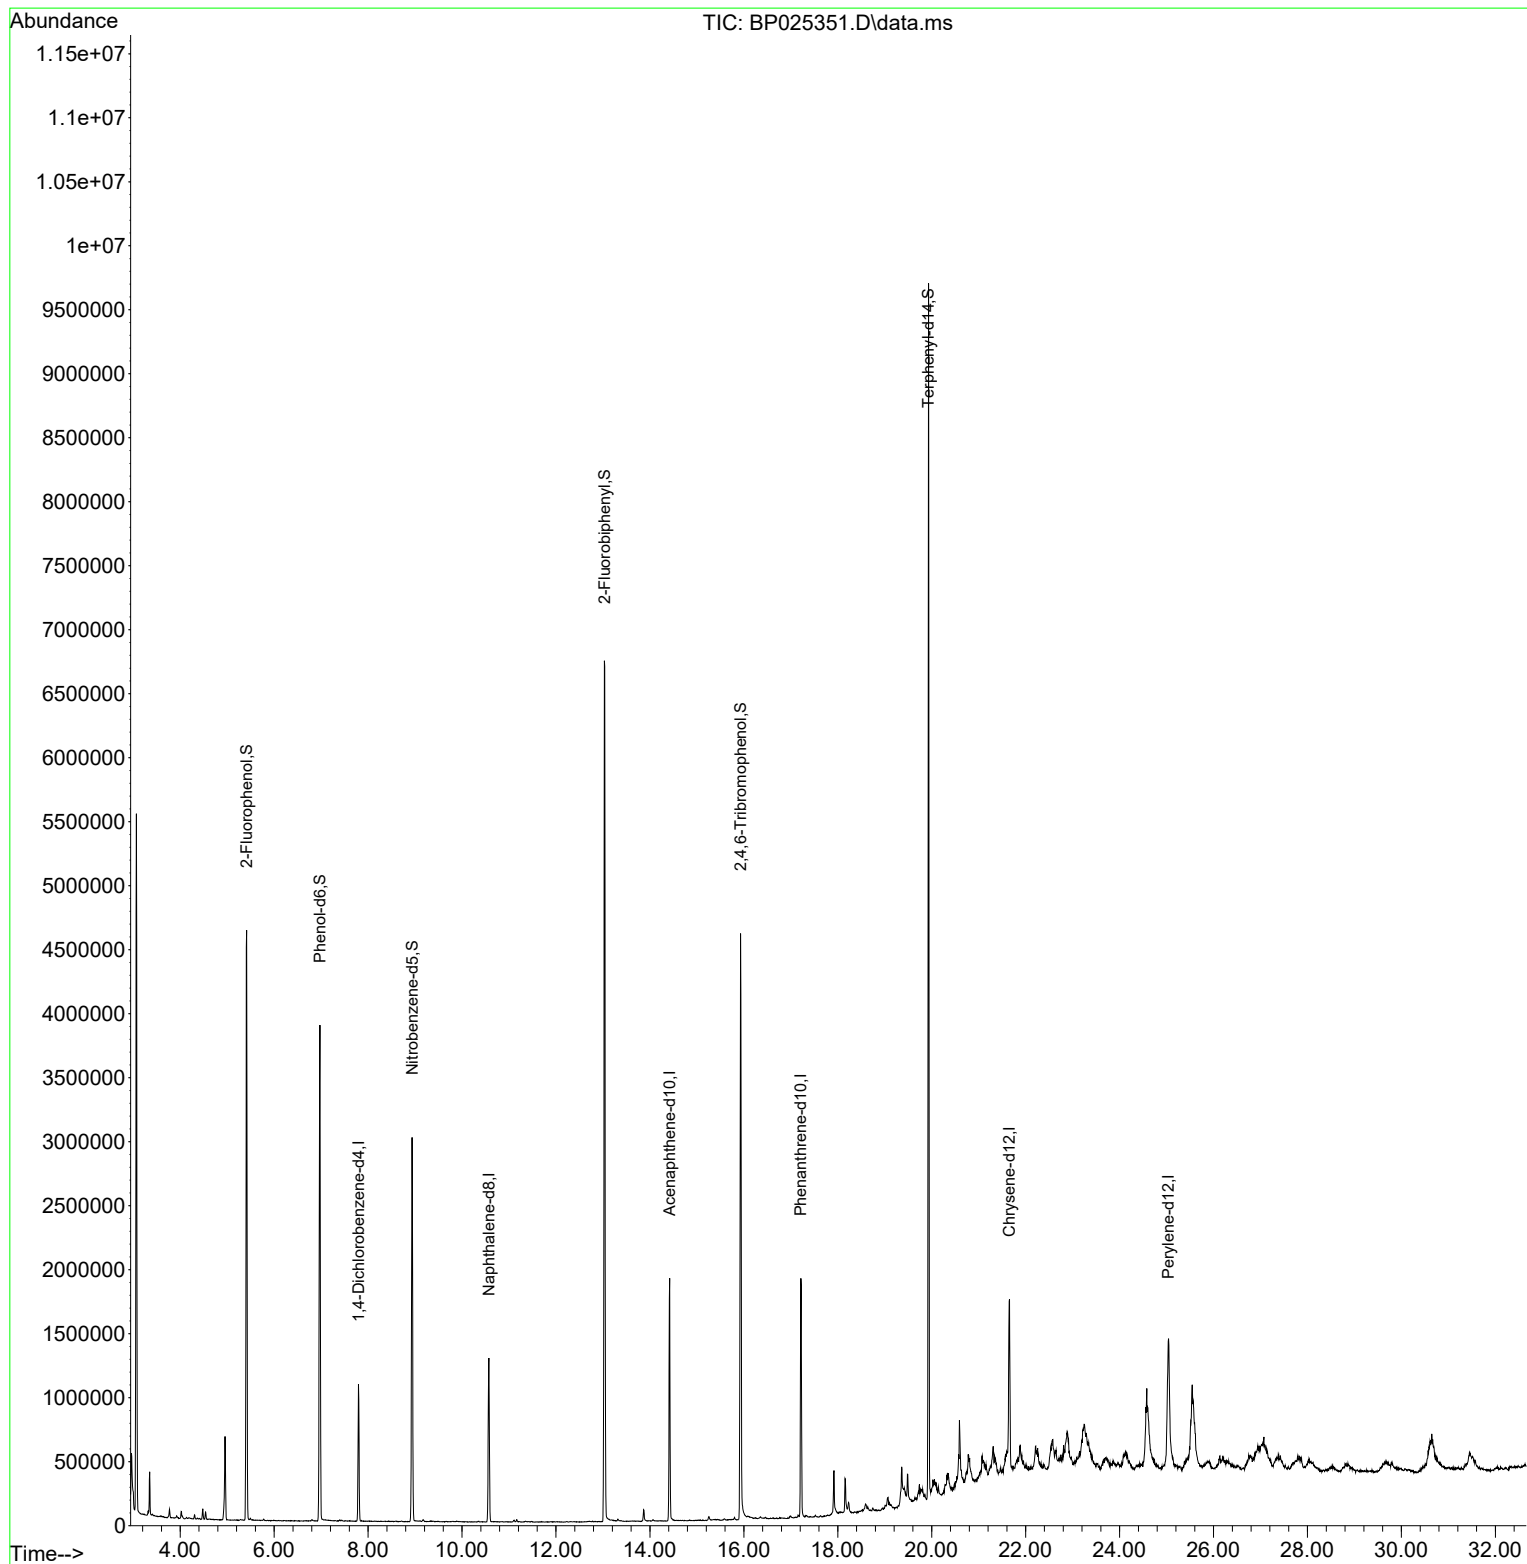


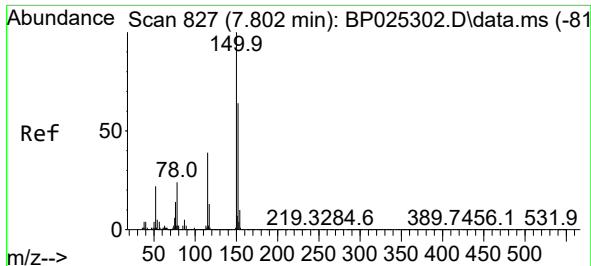


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.796 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP025351.D
Acq: 11 Aug 2025 16:47

Instrument :
BNA_P
ClientSampleId :
TP-6

Tgt Ion:152 Resp: 296550
Ion Ratio Lower Upper
152 100
150 155.0 125.1 187.7
115 59.9 48.4 72.6

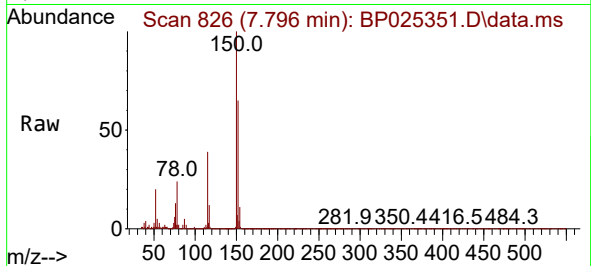


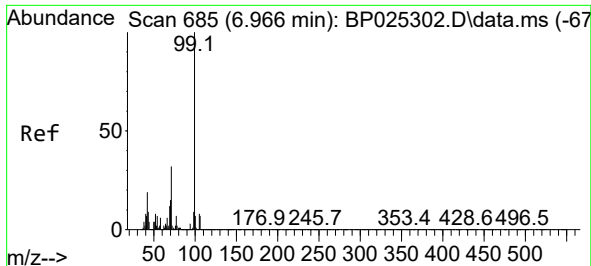


#7
Phenol-d6
Concen: 95.446 ng
RT: 6.972 min Scan# 686
Delta R.T. 0.006 min
Lab File: BP025351.D
Acq: 11 Aug 2025 16:47

Instrument :
BNA_P
ClientSampleId :
TP-6

Tgt Ion: 99 Resp: 2316072
Ion Ratio Lower Upper
99 100
42 16.3 15.0 22.6
71 31.1 25.5 38.3

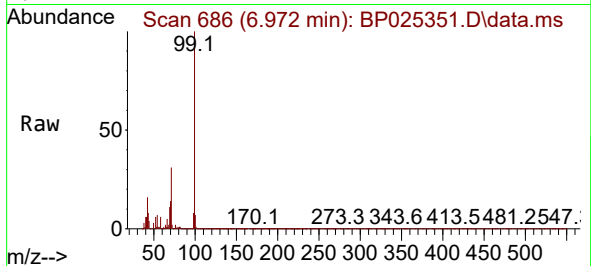


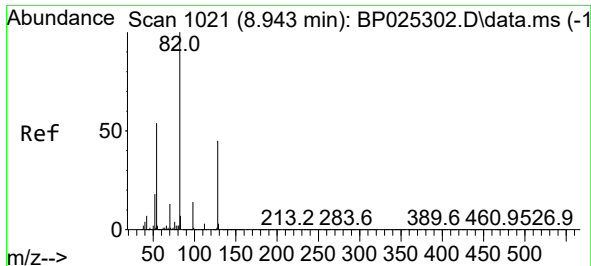


#23
Nitrobenzene-d5
Concen: 84.749 ng
RT: 8.937 min Scan# 1020
Delta R.T. -0.006 min
Lab File: BP025351.D
Acq: 11 Aug 2025 16:47

Instrument :
BNA_P
ClientSampleId :
TP-6

Tgt Ion: 82 Resp: 1746307
Ion Ratio Lower Upper
82 100
128 47.6 35.4 53.2
54 50.2 42.9 64.3

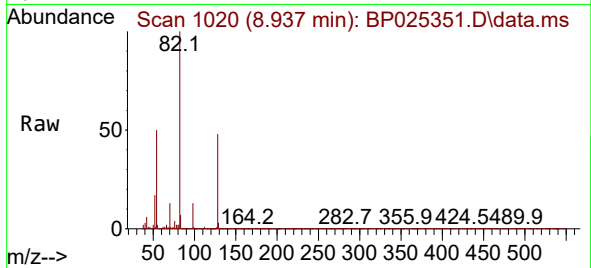

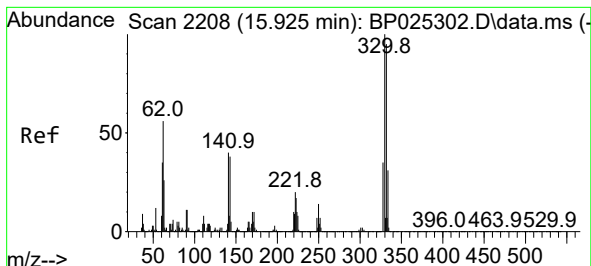

#42

2,4,6-Tribromophenol

Concen: 146.329 ng


RT: 15.931 min Scan# 2209

Delta R.T. 0.006 min

Lab File: BP025351.D

Acq: 11 Aug 2025 16:47


Instrument :

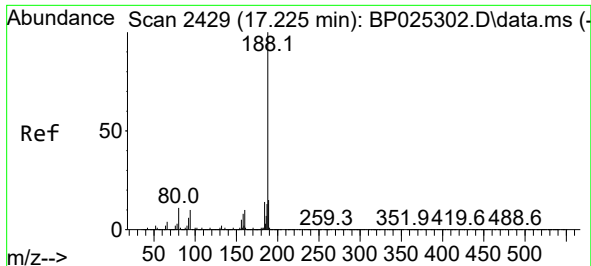


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.213 min Scan# 2429
Delta R.T. -0.012 min
Lab File: BP025351.D
Acq: 11 Aug 2025 16:47

Instrument :
BNA_P
ClientSampleId :
TP-6

Tgt Ion:188 Resp: 1214515
Ion Ratio Lower Upper
188 100
94 9.5 8.0 12.0
80 10.0 8.5 12.7

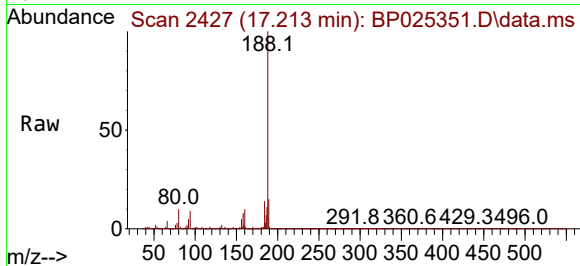

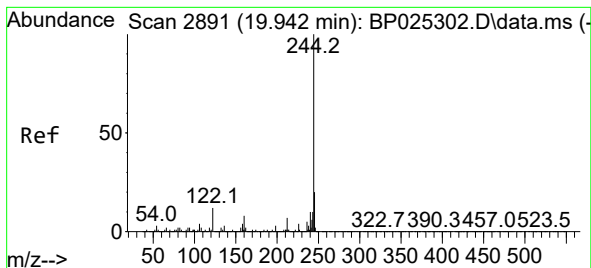

#79

Terphenyl-d14

Concen: 87.187 ng

RT: 19.930 min Scan# 2889

Delta R.T. -0.012 min

Lab File: BP025351.D

Acq: 11 Aug 2025 16:47

Instrument :

BNA_P