


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025342.D
Acq On : 11 Aug 2025 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

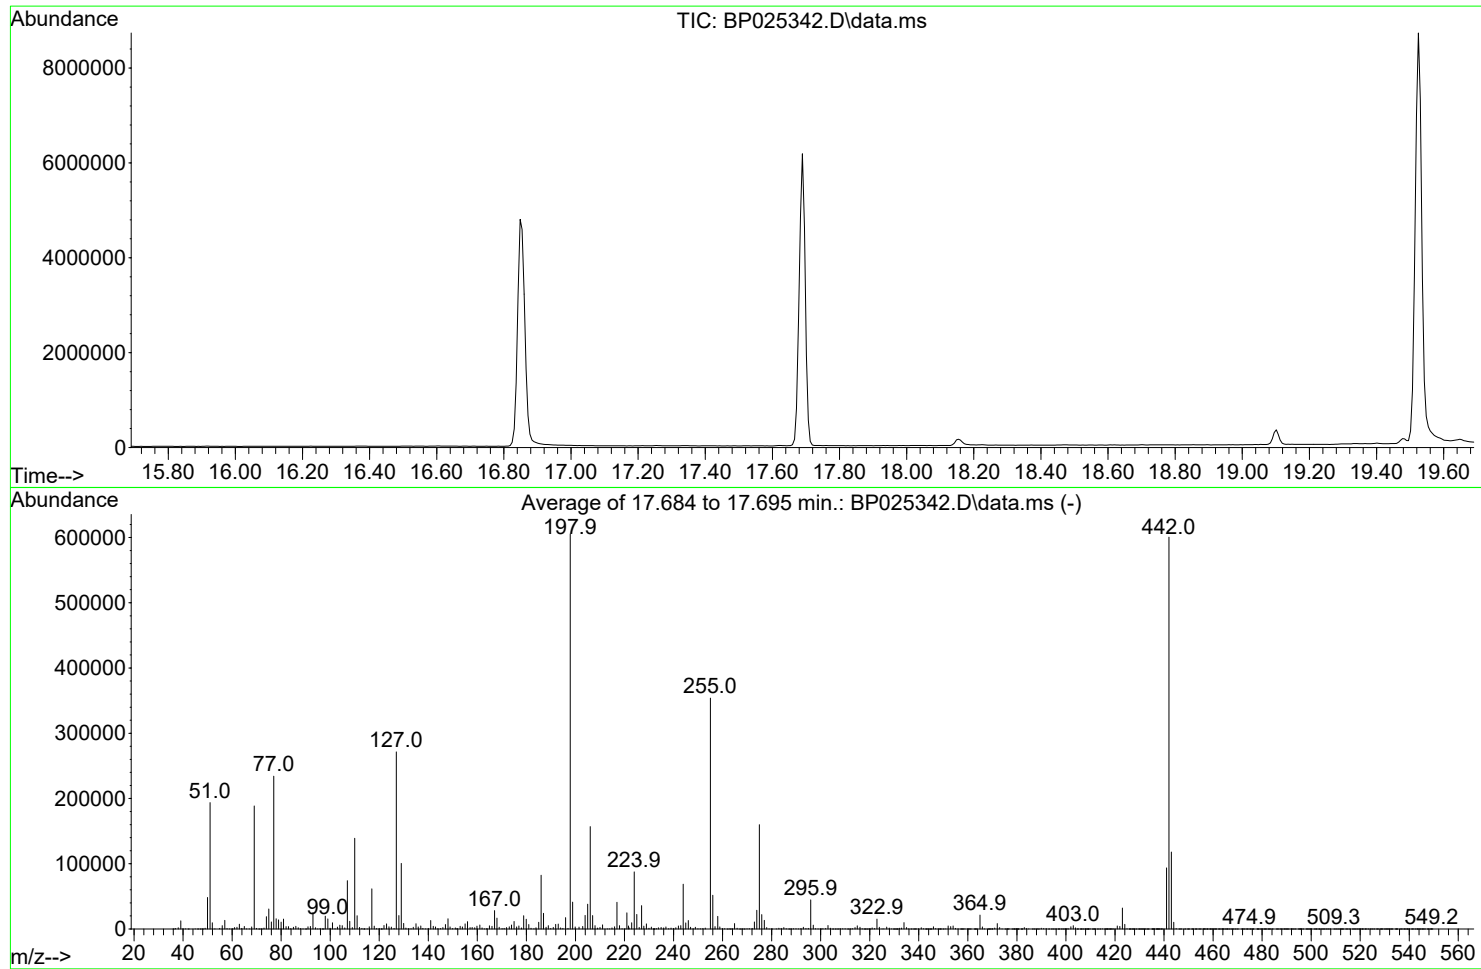

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2498

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3158	PASS
69	69	100	100	100.0	188556	PASS
70	69	0.00	2	0.5	968	PASS
197	198	0.00	2	0.2	1108	PASS
198	198	100	100	100.0	605119	PASS
199	198	5	9	6.8	41280	PASS
365	198	1	100	3.5	21336	PASS
441	443	0.01	150	79.4	93718	PASS
442	442	100	100	100.0	600651	PASS
443	442	15	24	19.6	118003	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/11/2025	BNA_P	<u>BP025342.D</u>
Compound Name	Response	Retention Time
DDT	2163555	20.836
DDD	35787	20.425
DDE	1369	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37156	2200711	1.69

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025342.D
Acq On : 11 Aug 2025 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 11 12:20:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

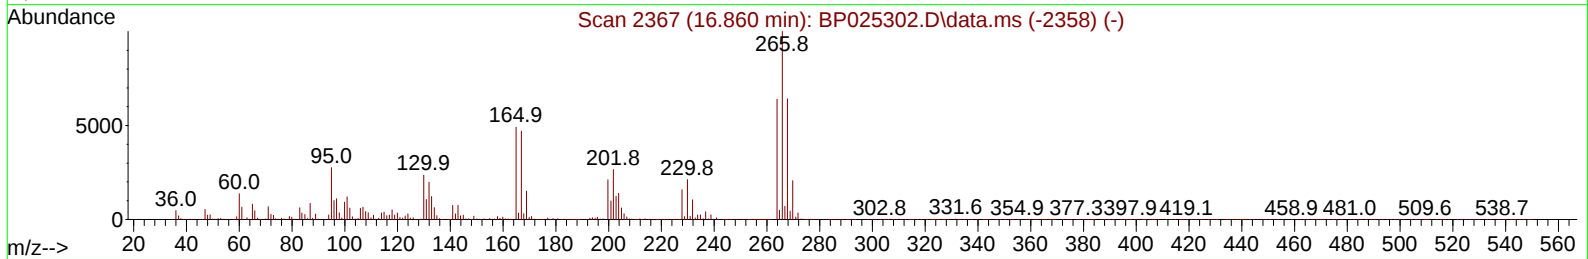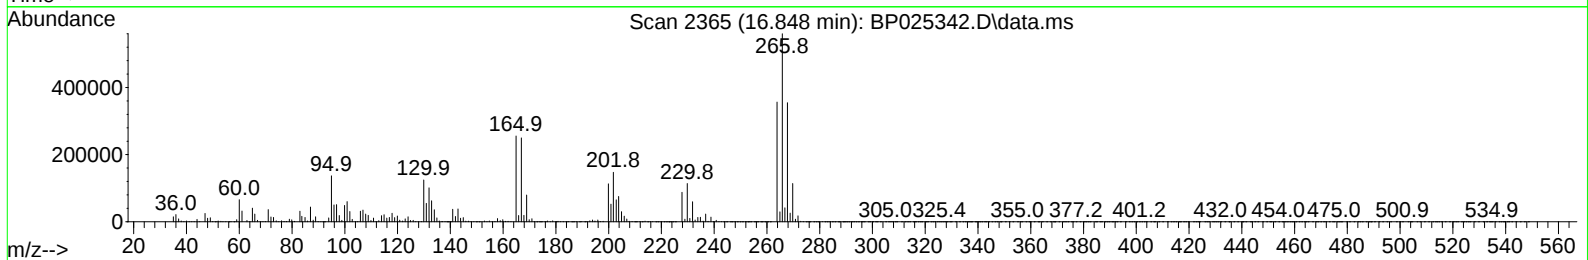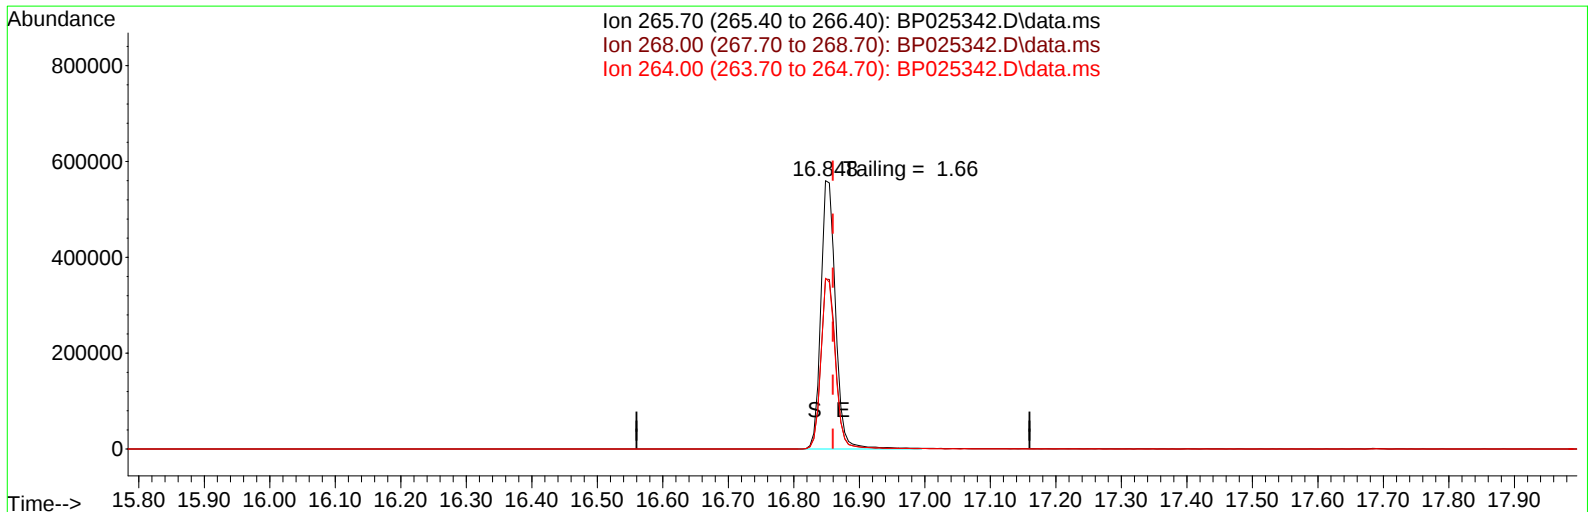

TIC: BP025342.D\data.ms

(70) Pentachlorophenol (C)

16.848min (-0.012) 2299749.99 ng




response 876713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.31
264.00	63.90	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081125\
Data File : BP025342.D
Acq On : 11 Aug 2025 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 11 12:20:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

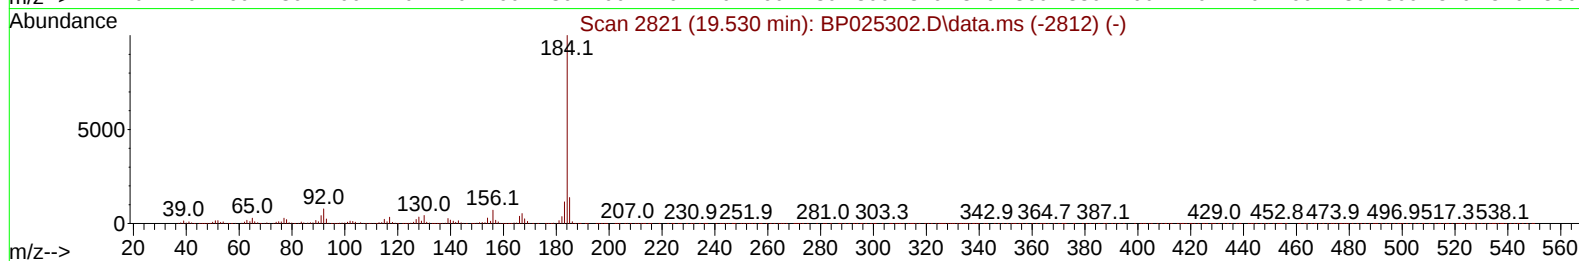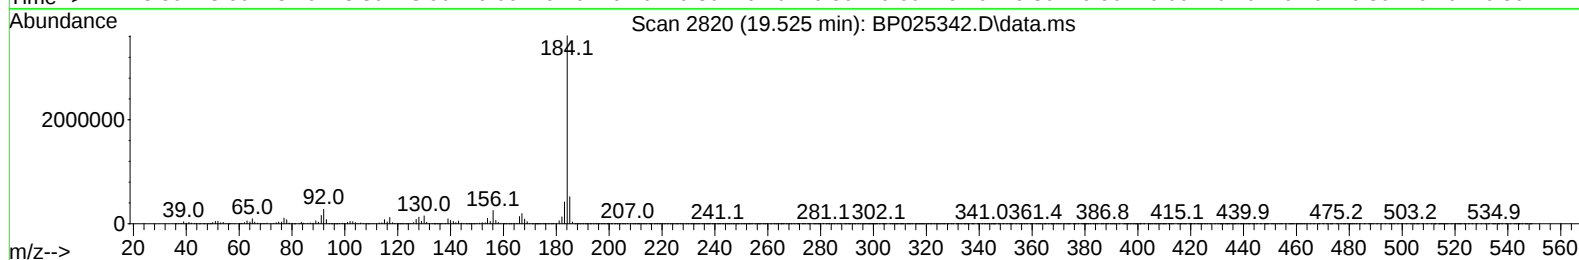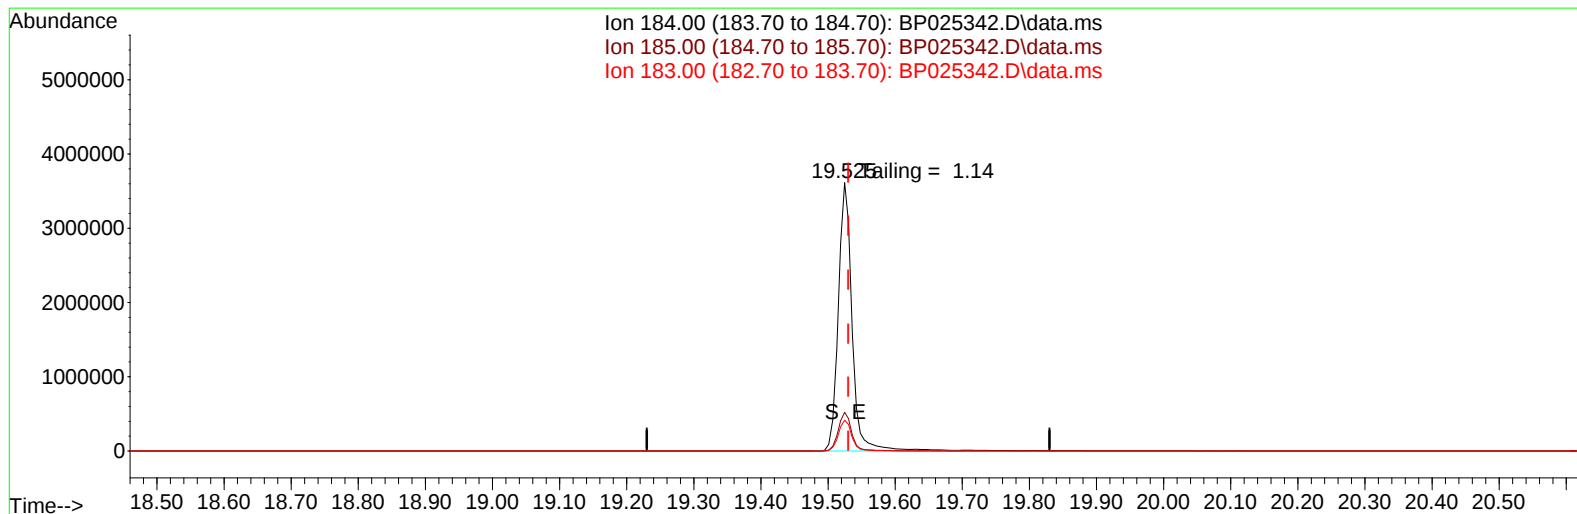

TIC: BP025342.D\data.ms

(77) Benzidine

19.525min (-0.005) 1639801.98 ng

response 5104250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.42
183.00	11.50	11.55
0.00	0.00	0.00