
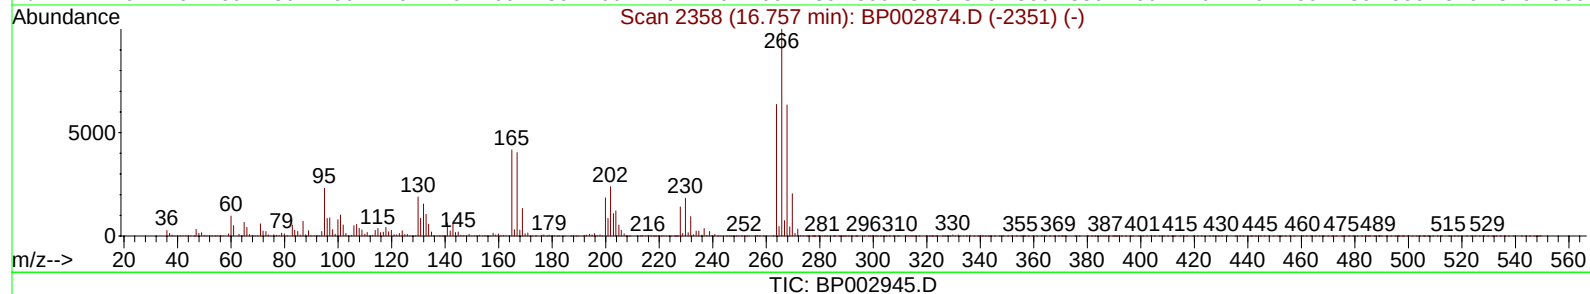
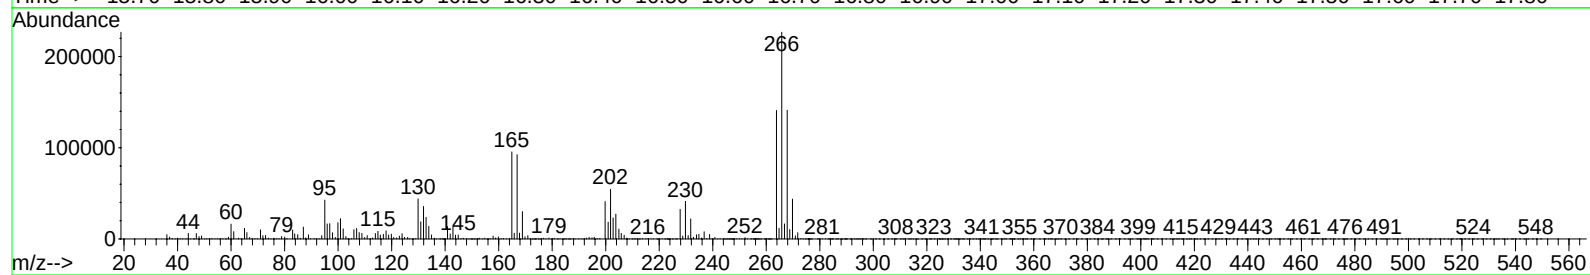


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081220\
Data File : BP002945.D
Acq On : 12 Aug 2020 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 17:52:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 11 17:14:14 2020
Response via : Initial Calibration

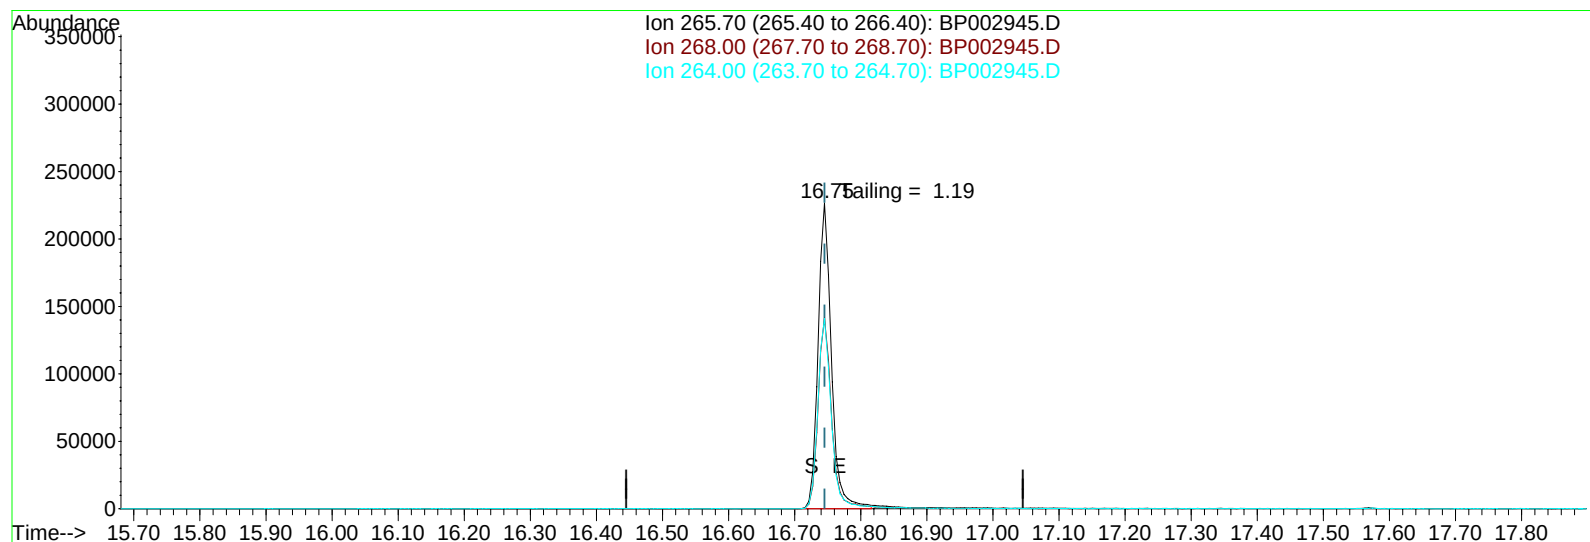

(70) Pentachlorophenol (C)




16.745min (-0.000) 52846.24ng

response 324695

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	62.31
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081220\
 Data File : BP002945.D
 Acq On : 12 Aug 2020 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 17:52:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 11 17:14:14 2020
 Response via : Initial Calibration

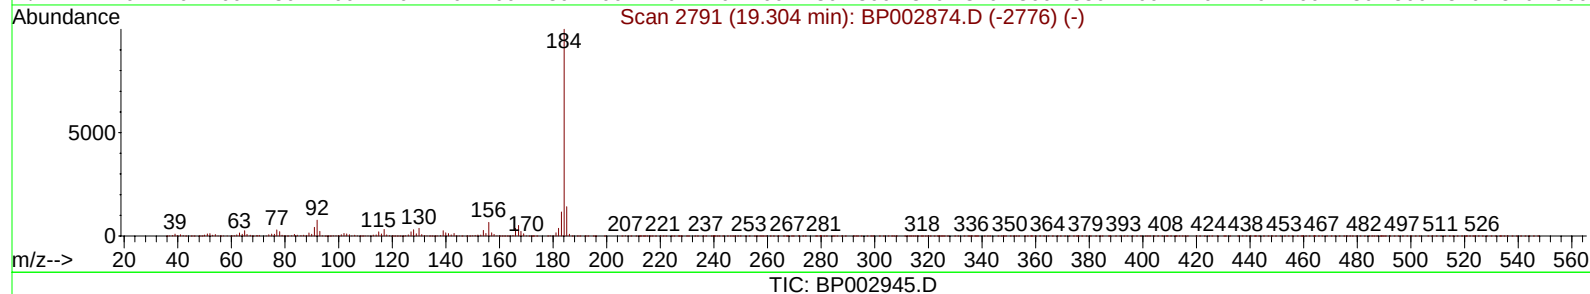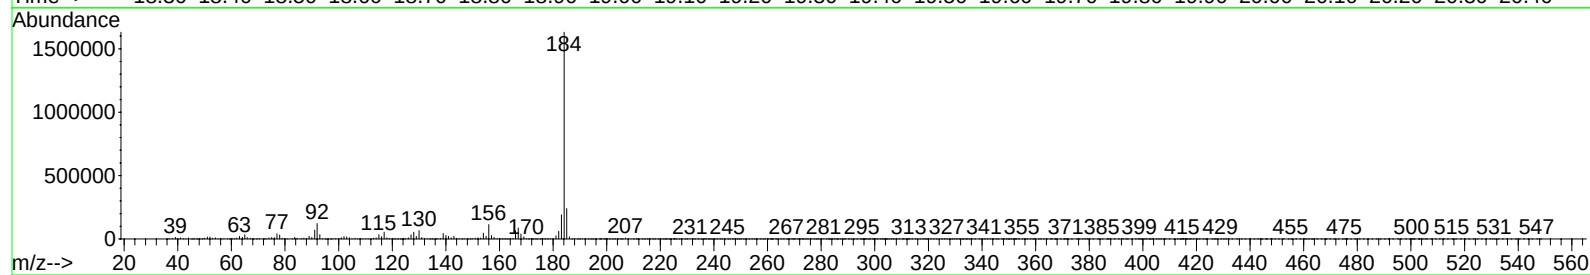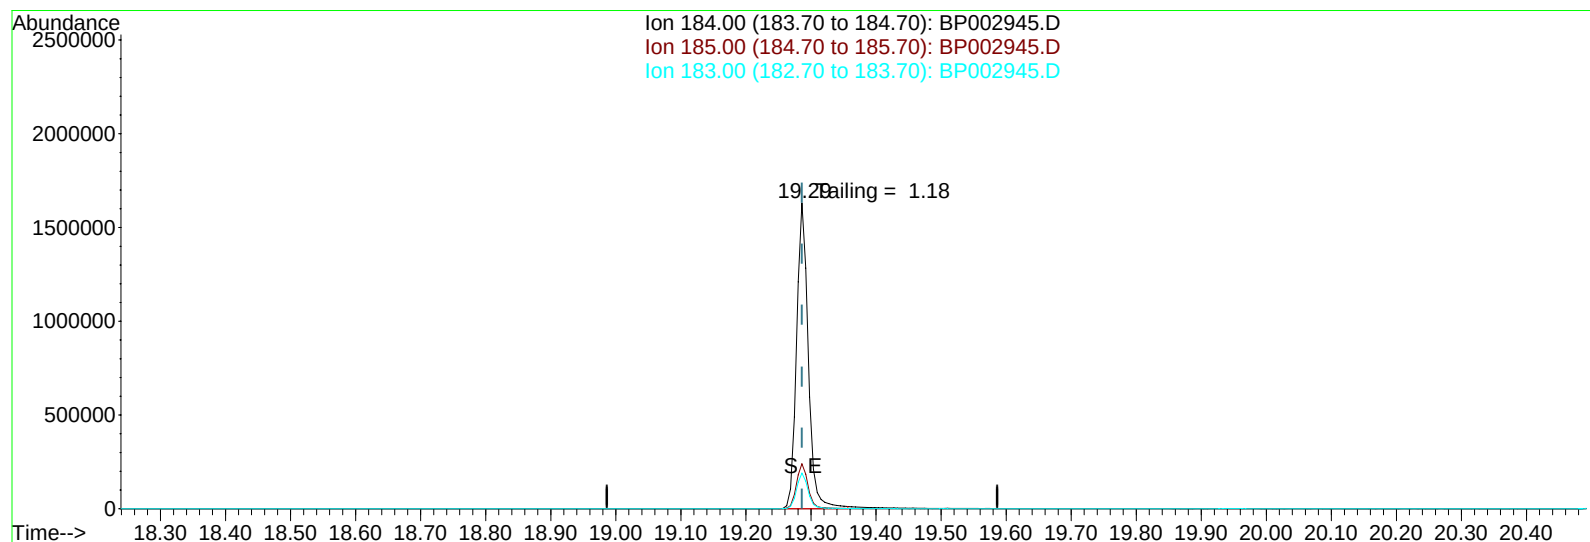

(77) Benzidine

19.286min (-0.000) 73468.41ng

response 2094691

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.69
183.00	11.90	11.69
0.00	0.00	0.00