


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081220\
 Data File : BP002945.D
 Acq On : 12 Aug 2020 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 11 17:14:14 2020

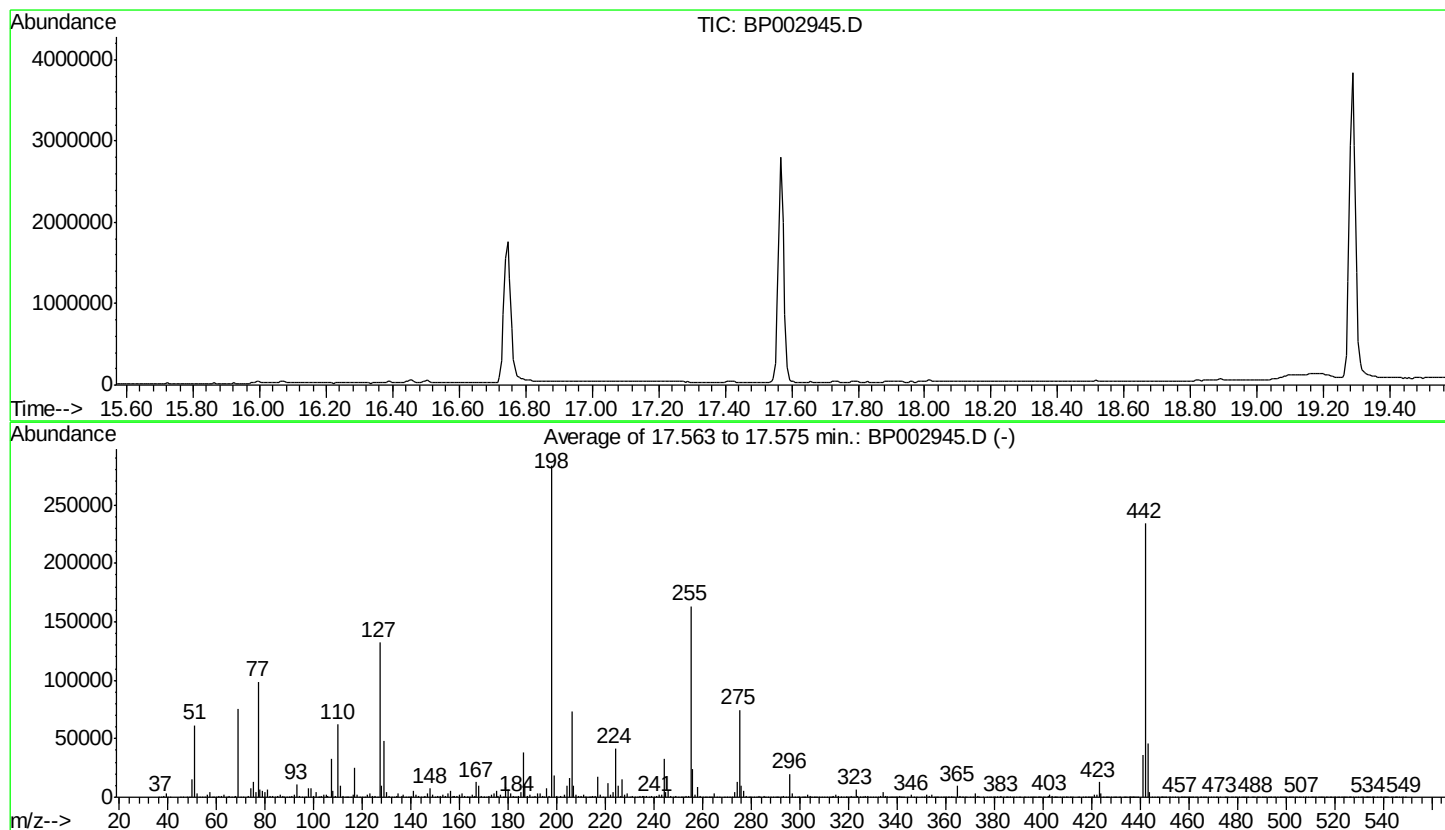

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	61653	PASS
68	69	0.00	2	1.7	1288	PASS
69	198	0.00	100	26.7	75821	PASS
70	69	0.00	2	0.6	482	PASS
127	198	10	80	46.6	132275	PASS
197	198	0.00	2	0.5	1427	PASS
198	198	100	100	100.0	283598	PASS
199	198	5	9	6.6	18692	PASS
275	198	10	60	26.4	74880	PASS
365	198	1	100	3.3	9371	PASS
441	198	0.01	100	12.9	36469	PASS
442	198	50	100	82.5	233997	PASS
443	442	15	24	19.6	45906	PASS