
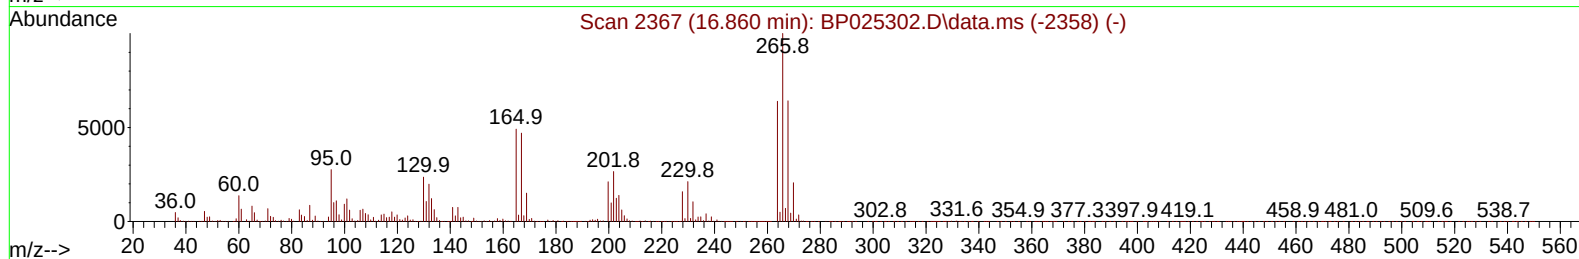
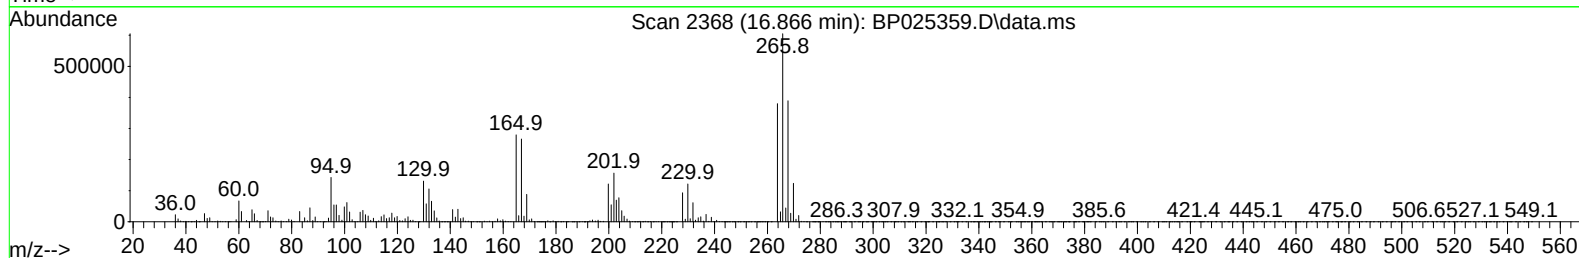


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081225\
Data File : BP025359.D
Acq On : 12 Aug 2025 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 11:27:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

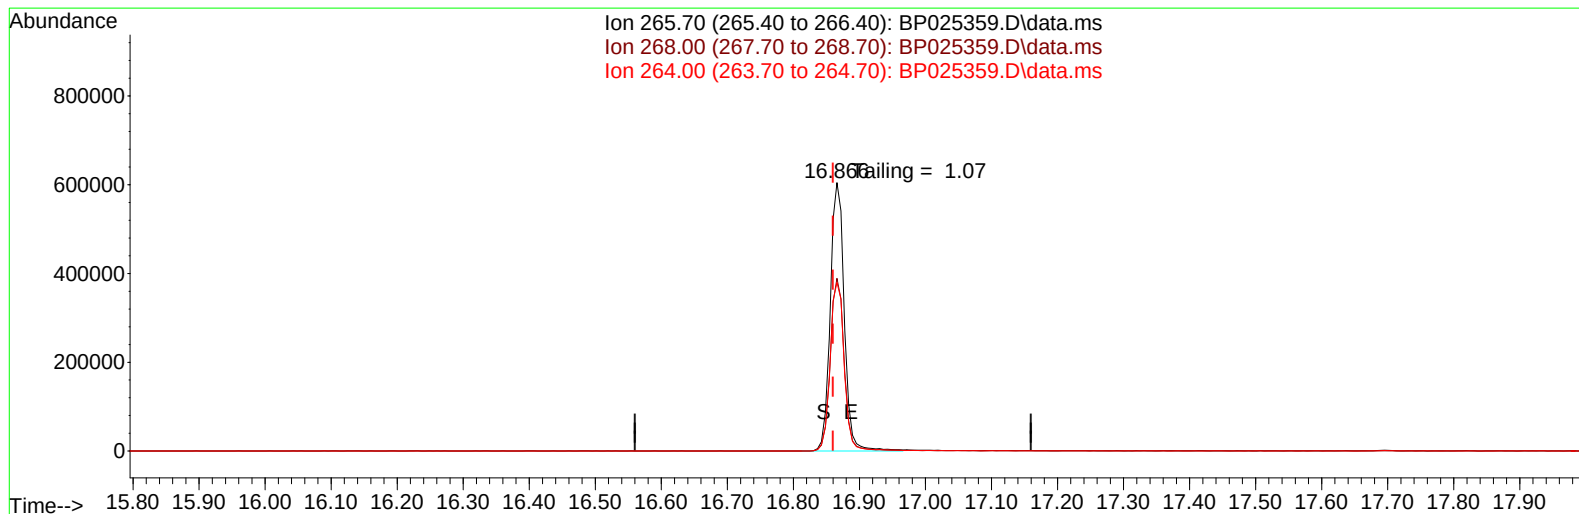

TIC: BP025359.D\data.ms

(70) Pentachlorophenol (C)




16.866min (+ 0.006) 2105985.22 ng

response 893734

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.31
264.00	63.90	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081225\
Data File : BP025359.D
Acq On : 12 Aug 2025 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 11:27:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

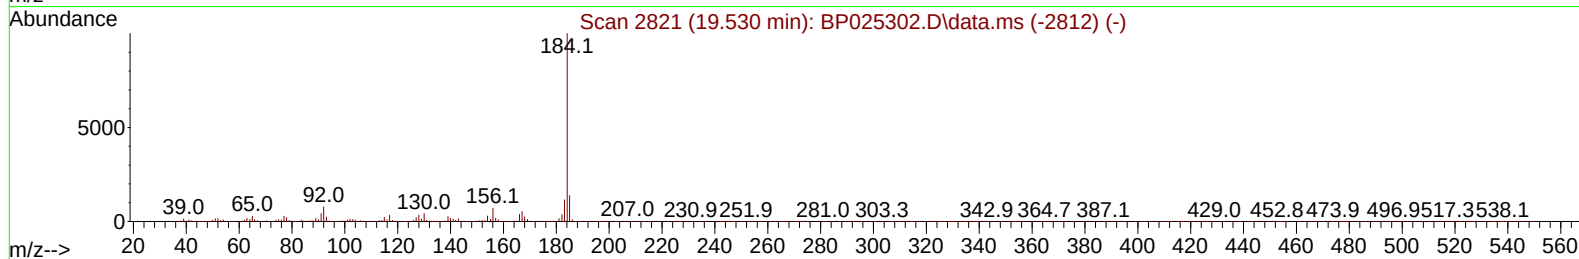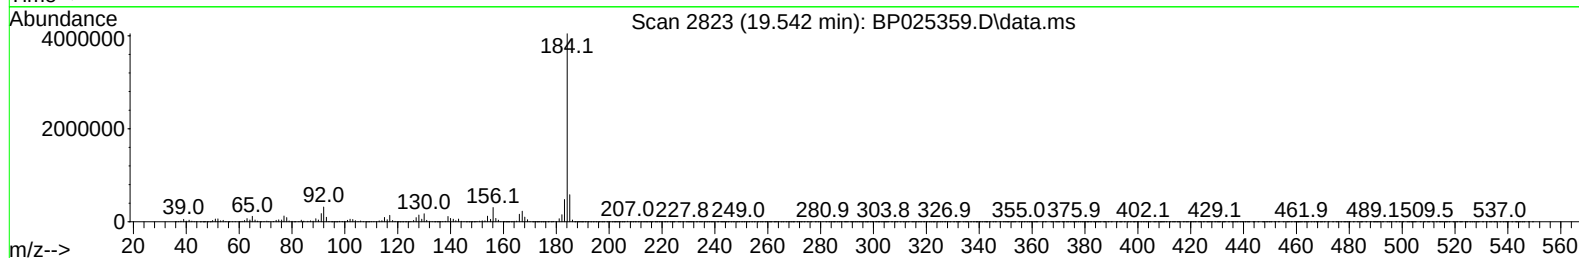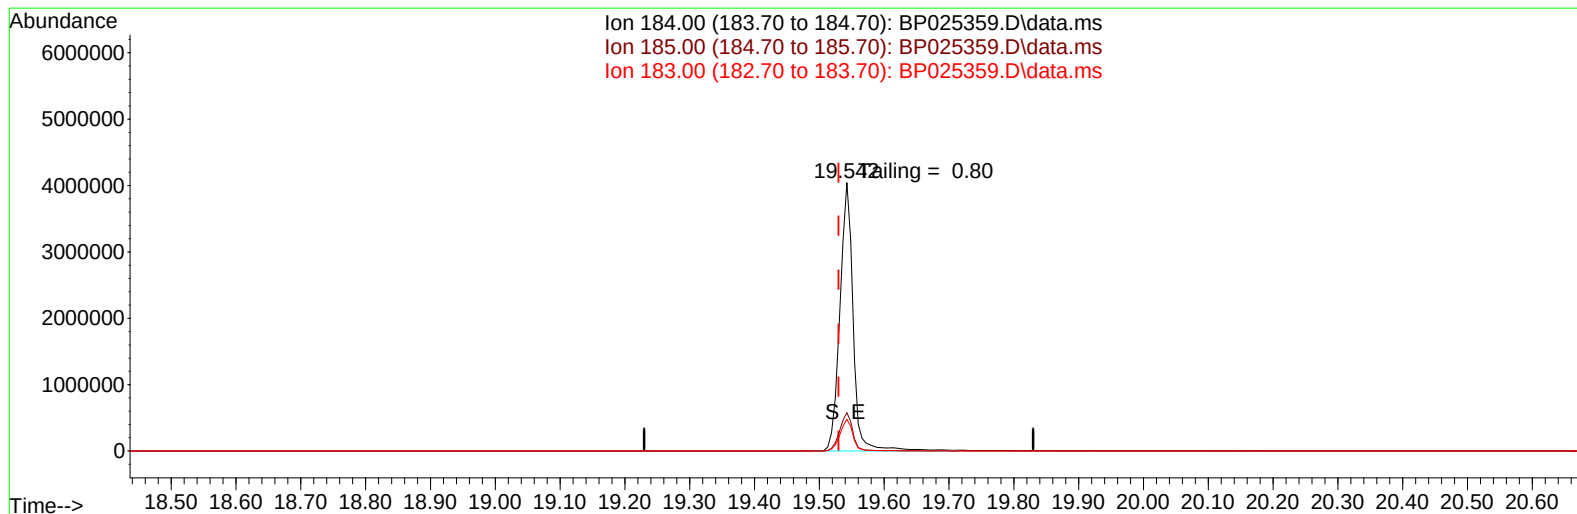

TIC: BP025359.D\data.ms

(77) Benzidine**19.542min (+ 0.012) 1326377.90 ng****response 5712896**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.35
183.00	11.50	11.85
0.00	0.00	0.00