
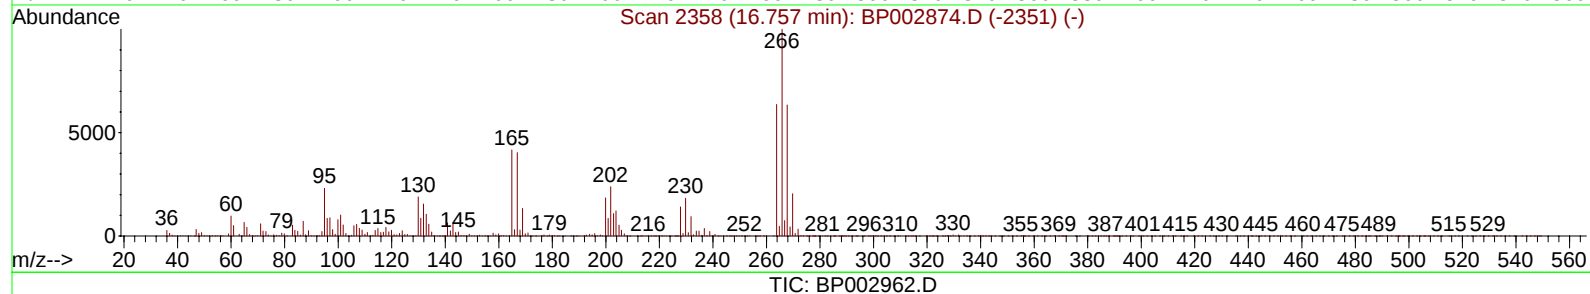
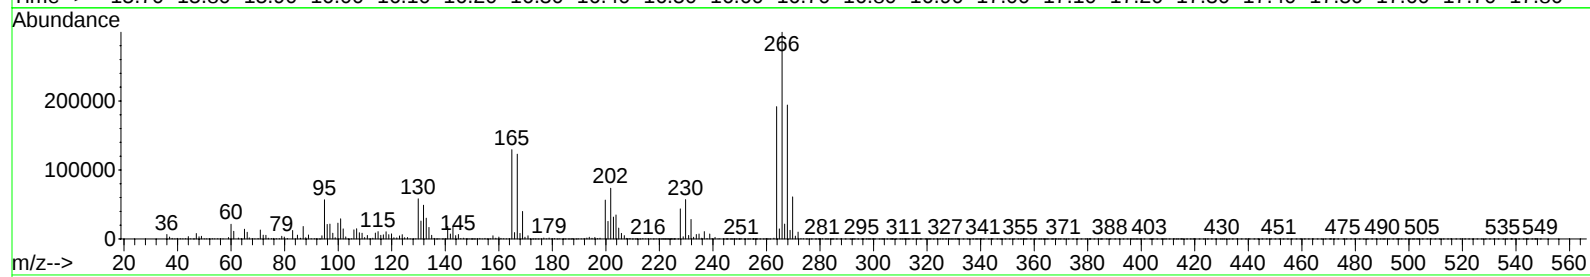


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081320\
Data File : BP002962.D
Acq On : 13 Aug 2020 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 18:25:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 11 17:14:14 2020
Response via : Initial Calibration

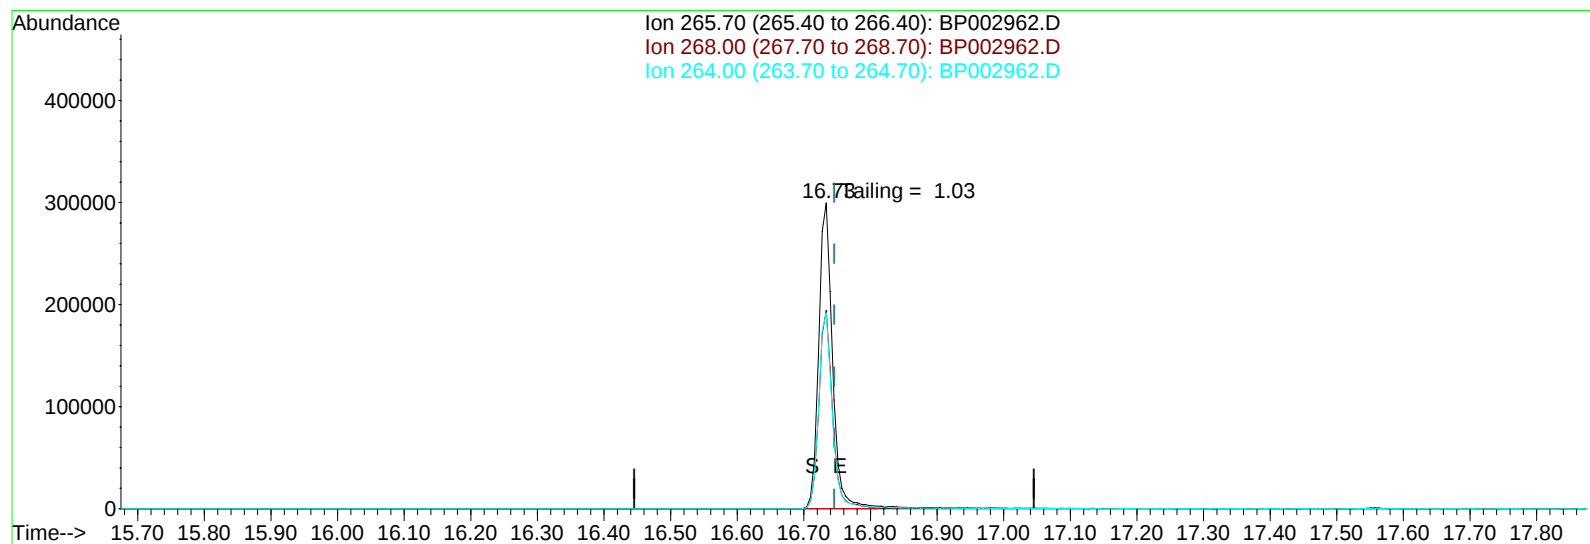

(70) Pentachlorophenol (C)




16.733min (-0.012) 51464.63ng

response 435253

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.82
264.00	63.90	64.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081320\
Data File : BP002962.D
Acq On : 13 Aug 2020 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 18:25:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 11 17:14:14 2020
Response via : Initial Calibration

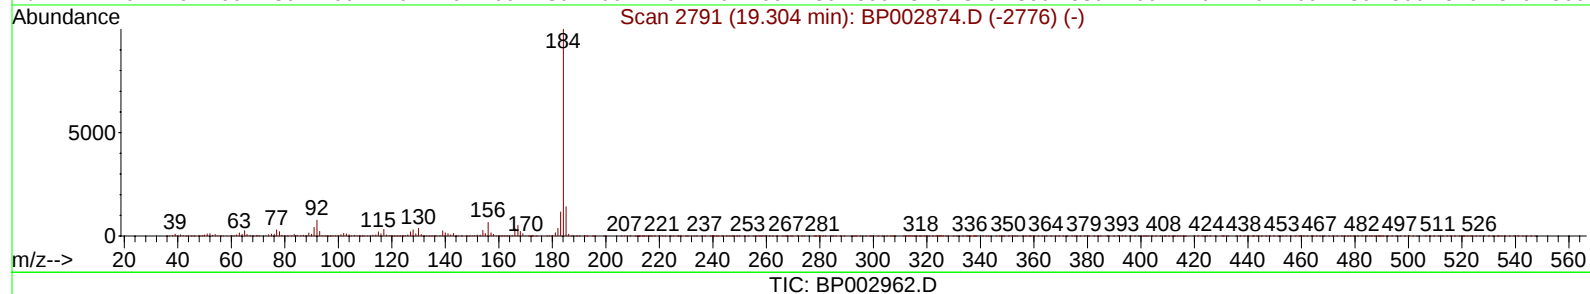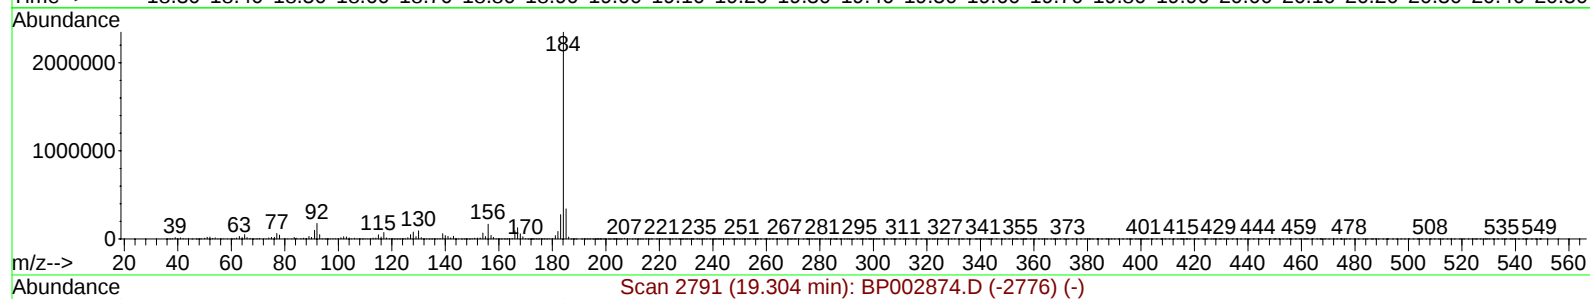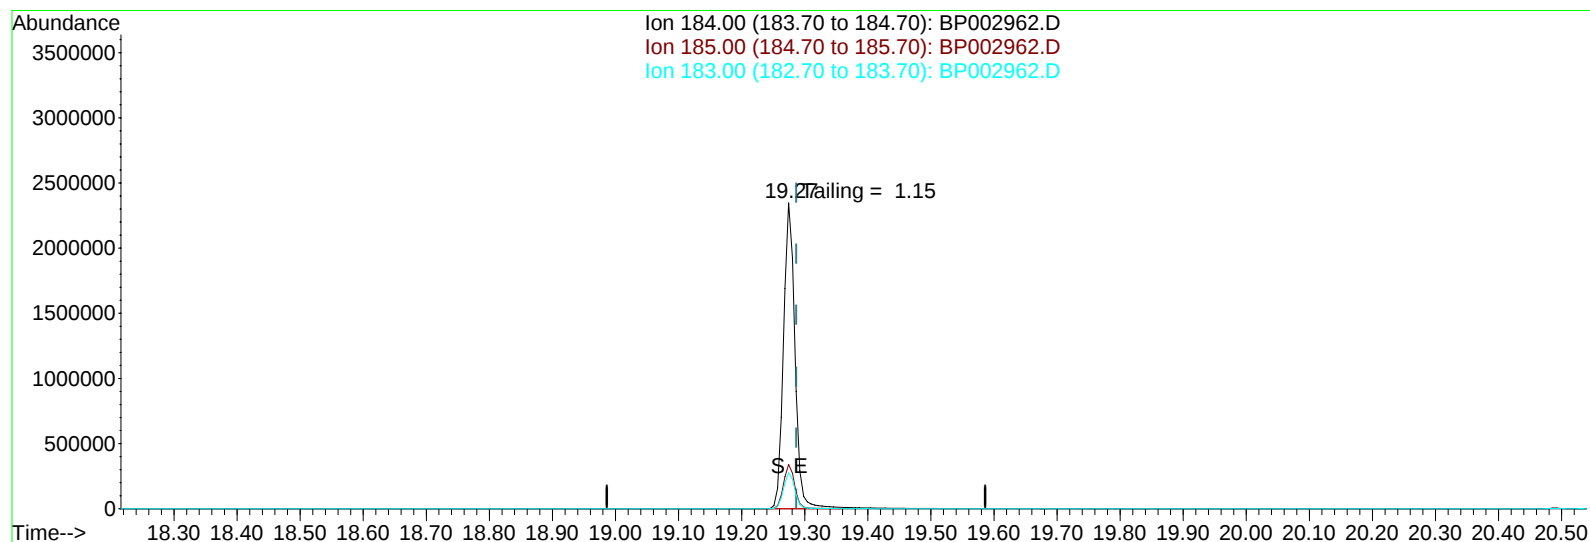

(77) Benzidine

19.275min (-0.012) 47954.40ng

response 2999175

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.52
183.00	11.90	11.74
0.00	0.00	0.00