


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081320\
 Data File : BP002962.D
 Acq On : 13 Aug 2020 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 11 17:14:14 2020

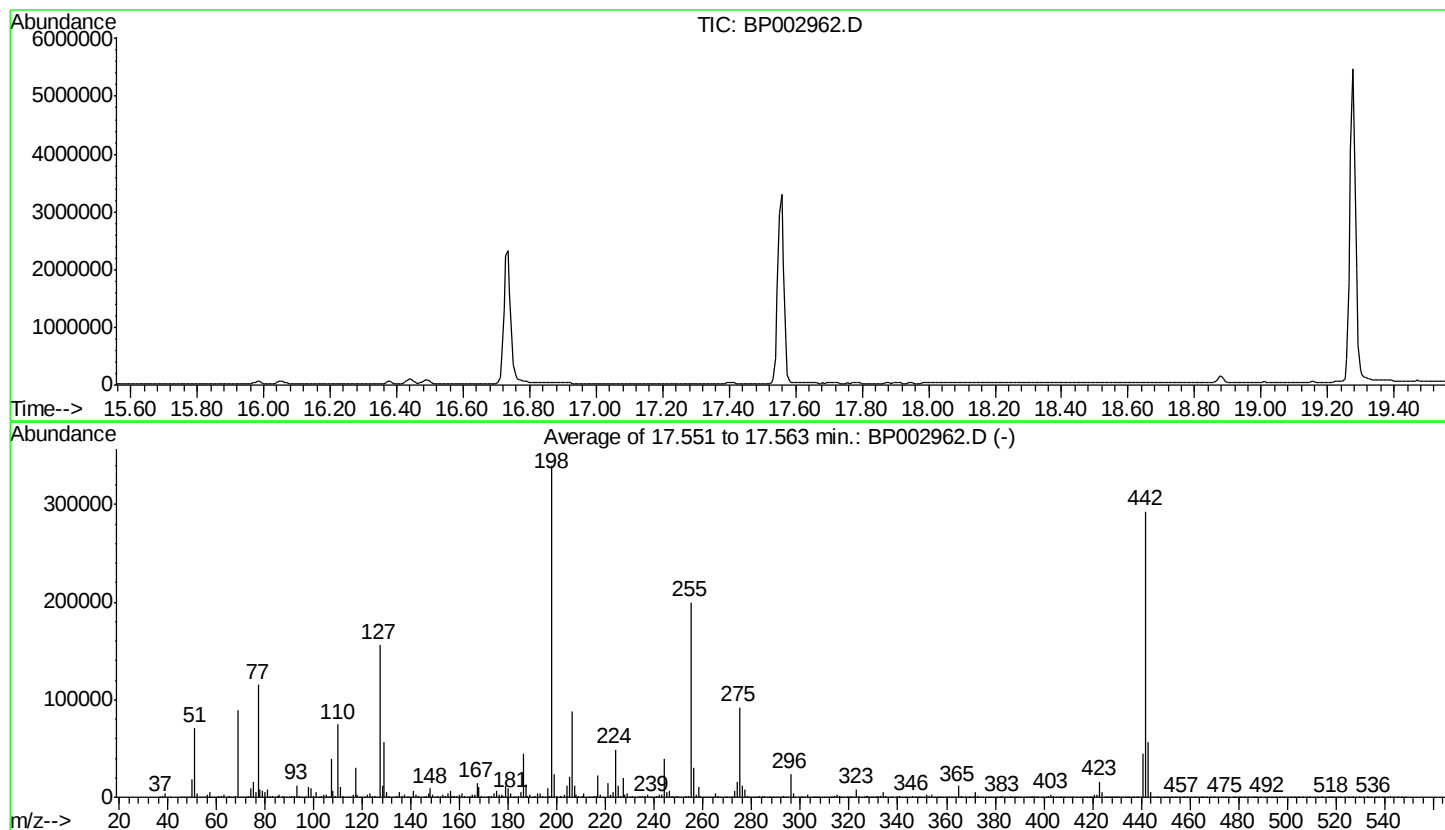

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.9	71142	PASS
68	69	0.00	2	1.5	1387	PASS
69	198	0.00	100	26.4	89517	PASS
70	69	0.00	2	0.5	449	PASS
127	198	10	80	46.1	156623	PASS
197	198	0.00	2	0.4	1357	PASS
198	198	100	100	100.0	339712	PASS
199	198	5	9	6.9	23403	PASS
275	198	10	60	27.0	91865	PASS
365	198	1	100	3.4	11668	PASS
441	198	0.01	100	13.2	44819	PASS
442	198	50	100	86.1	292624	PASS
443	442	15	24	19.3	56472	PASS