
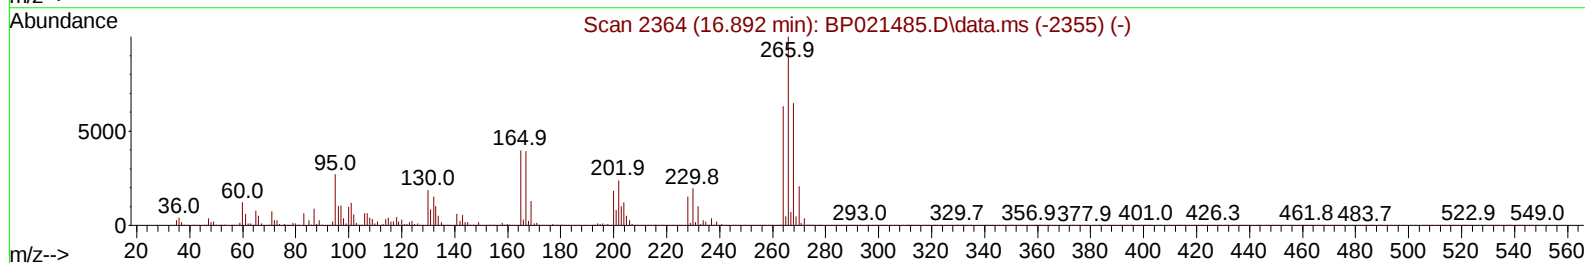
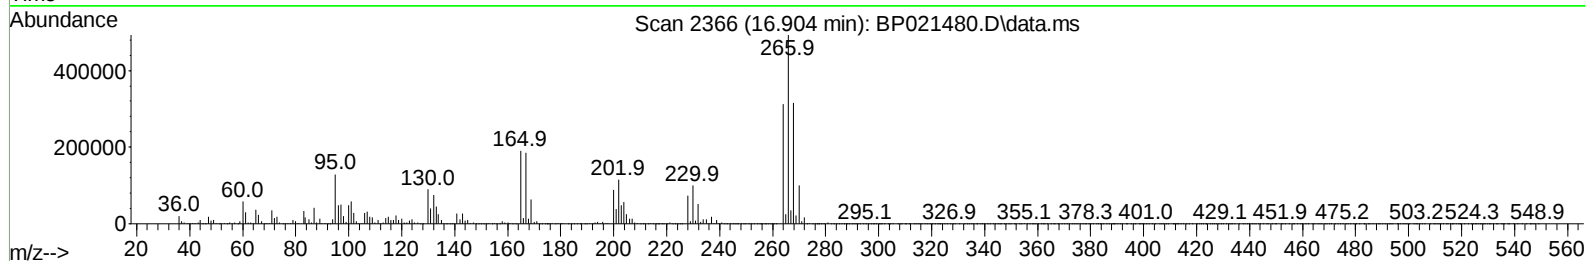


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081324\
Data File : BP021480.D
Acq On : 13 Aug 2024 11:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 00:14:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

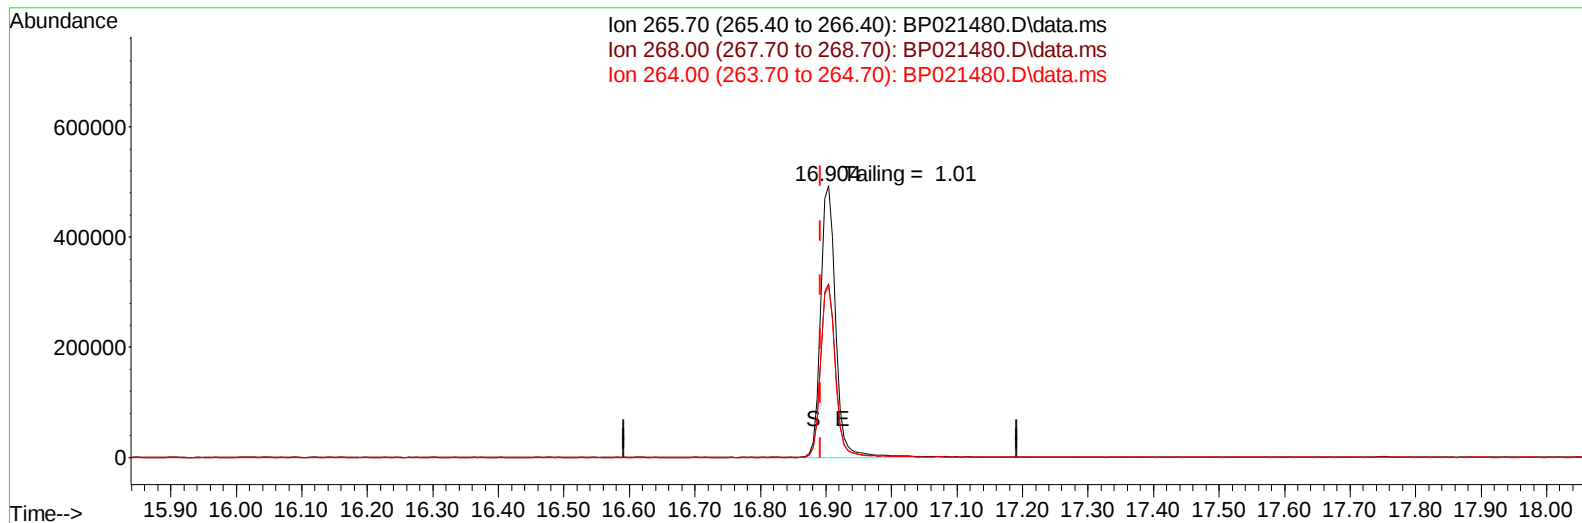




TIC: BP021480.D\data.ms

(70) Pentachlorophenol (C)**16.904min (+ 0.012) 6855729.98 ng****response 795611**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.10
264.00	63.10	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081324\
Data File : BP021480.D
Acq On : 13 Aug 2024 11:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 00:14:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

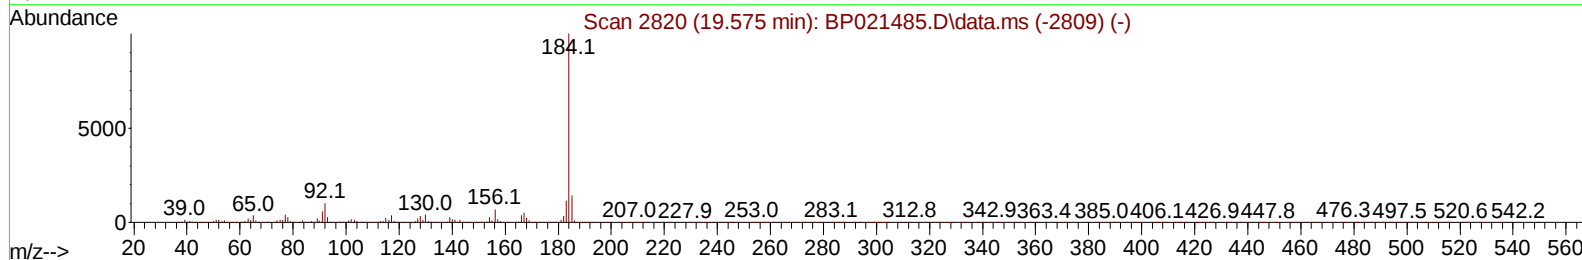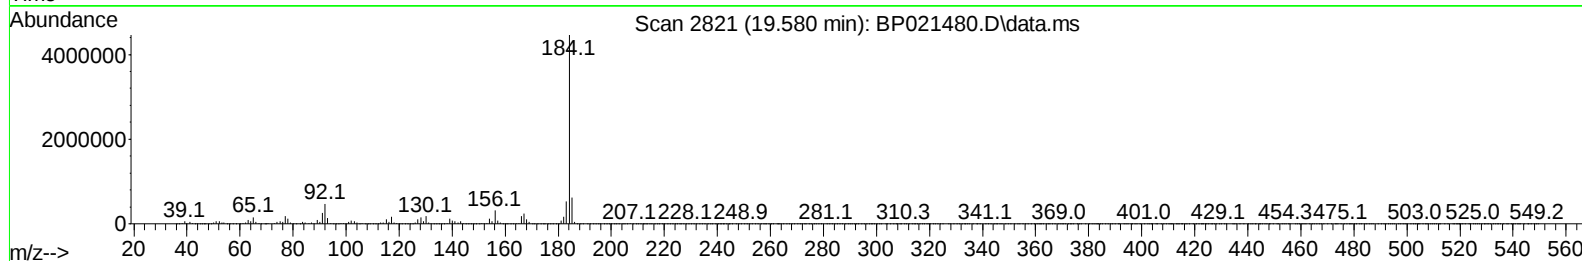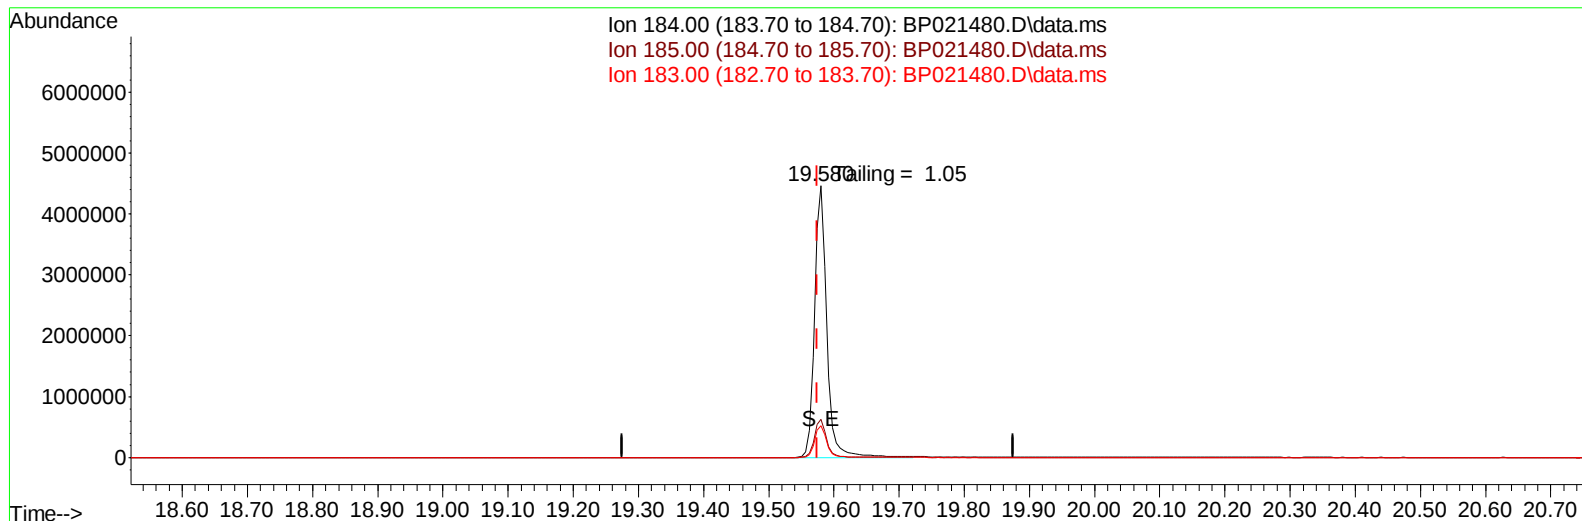

TIC: BP021480.D\data.ms

(77) Benzidine**19.580min (+ 0.005) -20.00 ng****response 5830874**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.05
183.00	11.60	11.75
0.00	0.00	0.00