
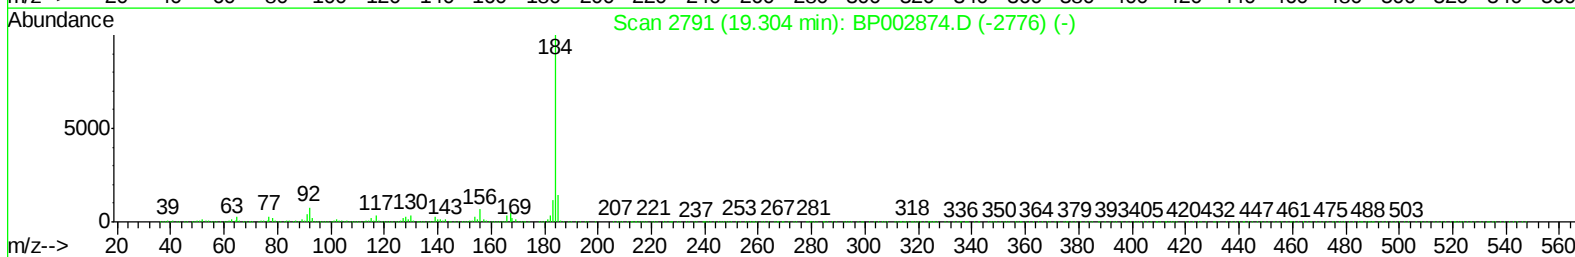
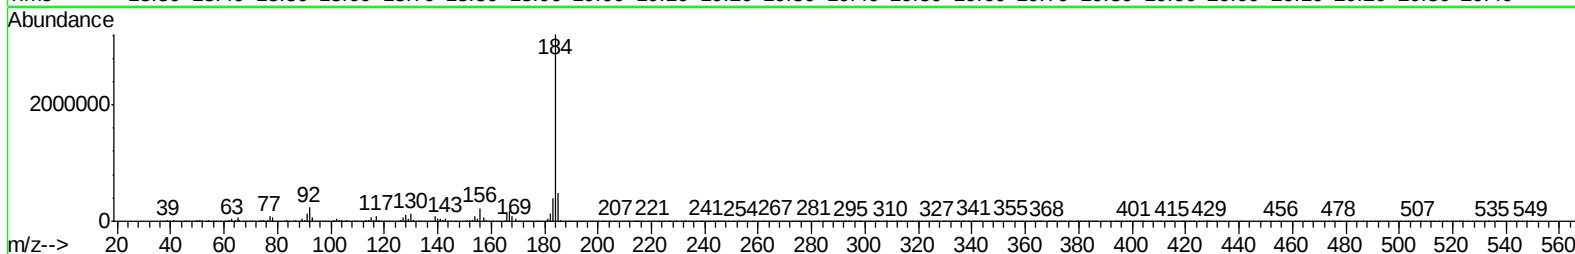


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081420\
 Data File : BP002977.D
 Acq On : 14 Aug 2020 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 04:31:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 11 17:14:14 2020
 Response via : Initial Calibration

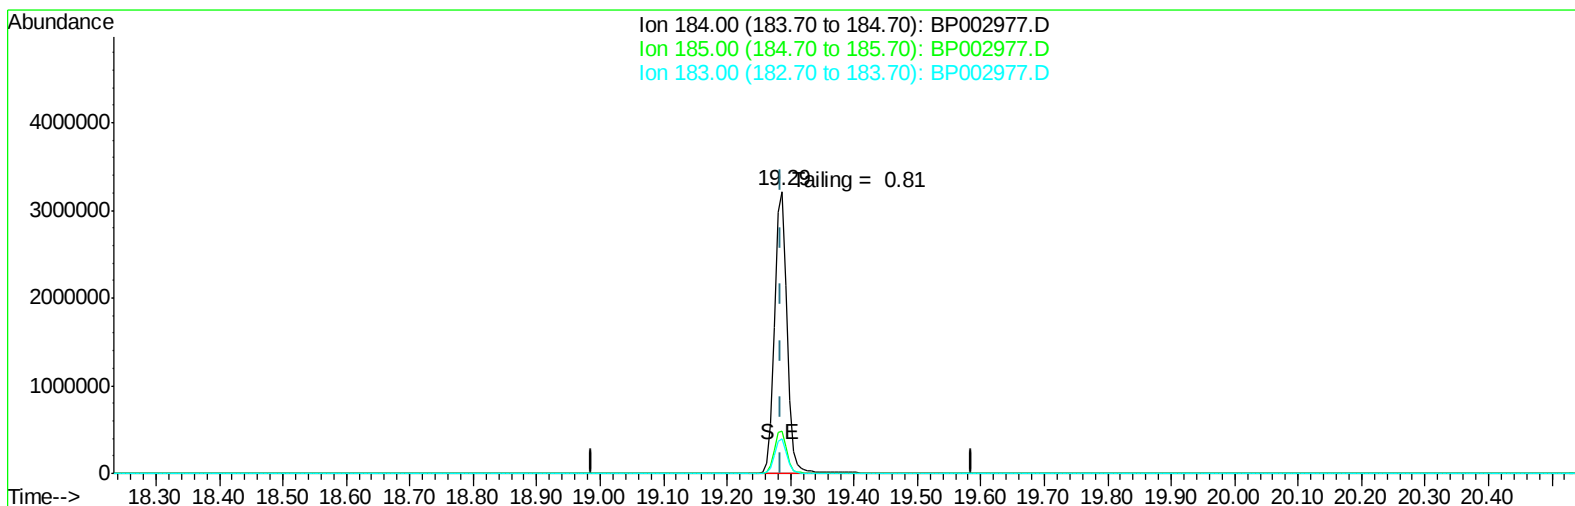

TIC: BP002977.D

(77) Benzidine

19.286min (+0.000) 40038.02ng

response 4337860

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.11
183.00	11.90	12.24
0.00	0.00	0.00