


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP081420\
 Data File : BP002977.D
 Acq On : 14 Aug 2020 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 11 17:14:14 2020

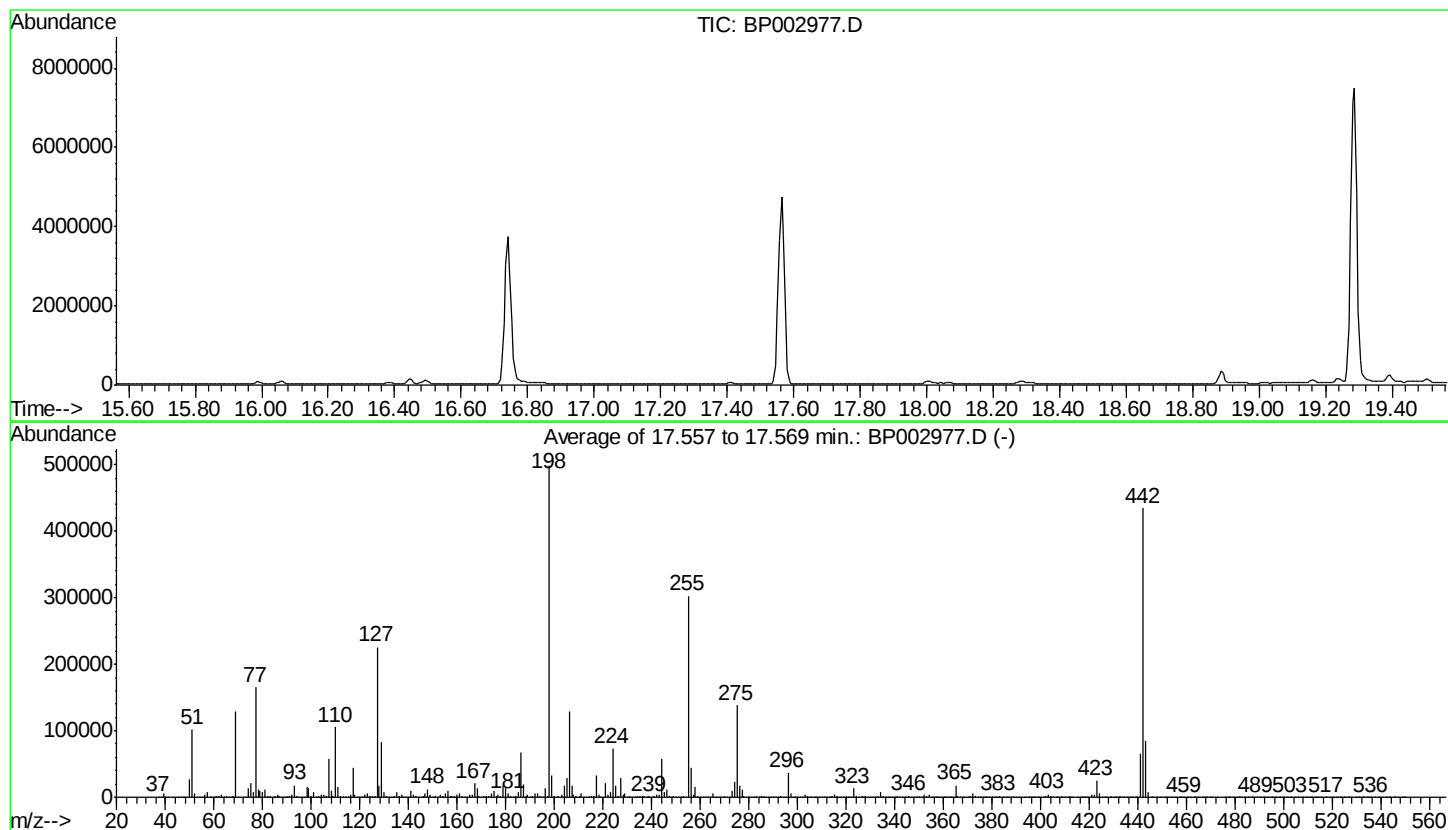

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.3	101403	PASS
68	69	0.00	2	1.7	2177	PASS
69	198	0.00	100	25.9	129132	PASS
70	69	0.00	2	0.5	609	PASS
127	198	10	80	45.2	225599	PASS
197	198	0.00	2	0.3	1741	PASS
198	198	100	100	100.0	498586	PASS
199	198	5	9	6.7	33597	PASS
275	198	10	60	27.6	137802	PASS
365	198	1	100	3.5	17698	PASS
441	198	0.01	100	13.0	65000	PASS
442	198	50	100	87.1	434154	PASS
443	442	15	24	19.4	84397	PASS