
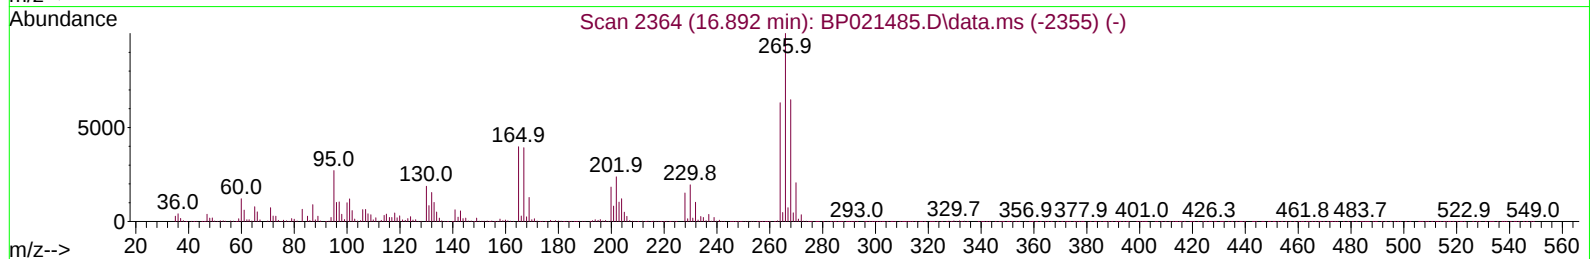
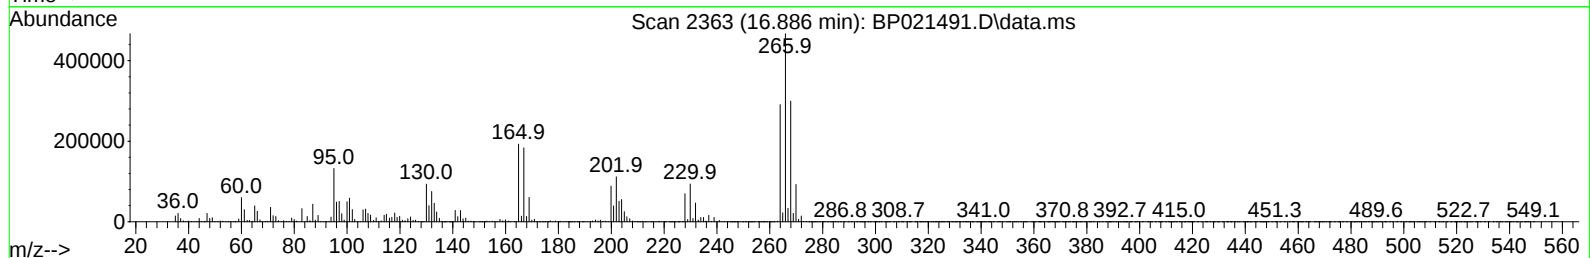


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081424\
Data File : BP021491.D
Acq On : 14 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:42:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

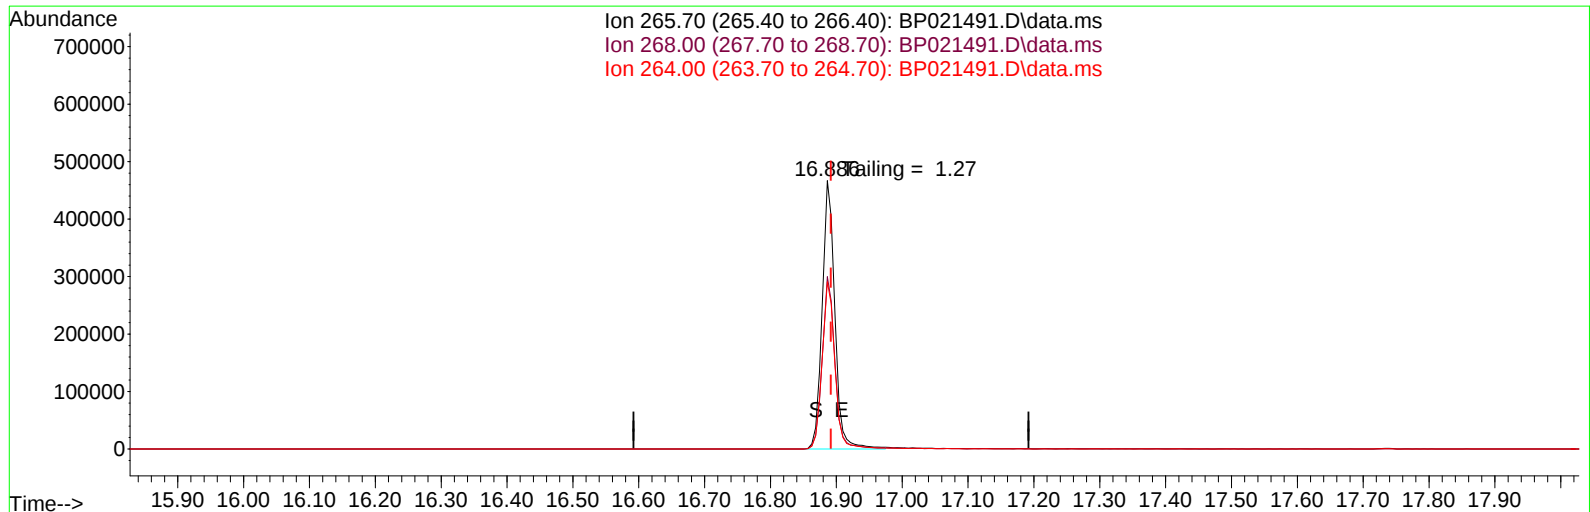

TIC: BP021491.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.006) 3545903.77 ng

response 629359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.19
264.00	63.10	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081424\
Data File : BP021491.D
Acq On : 14 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:42:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

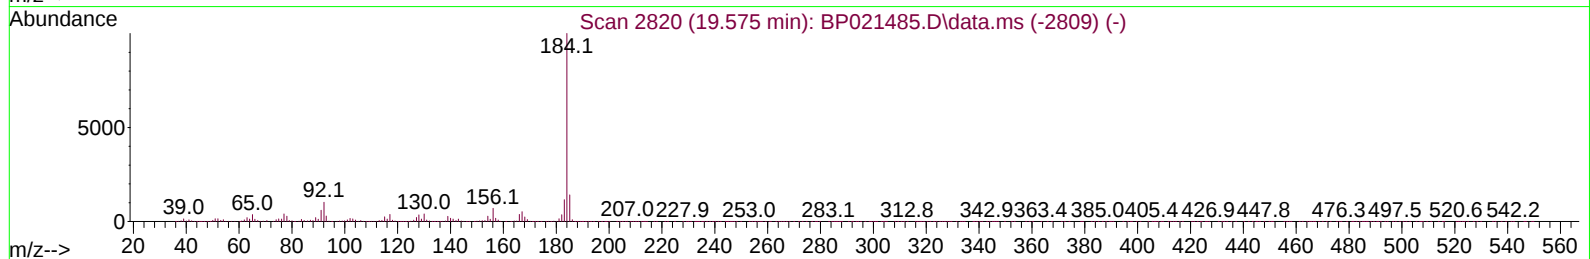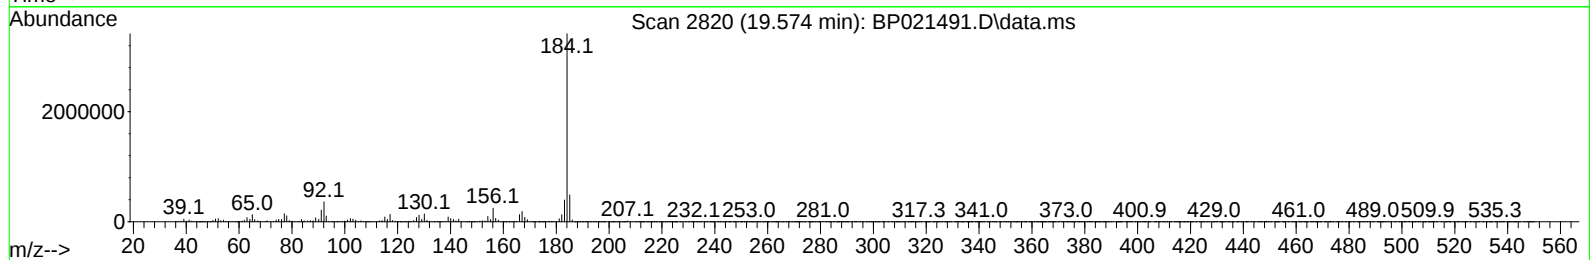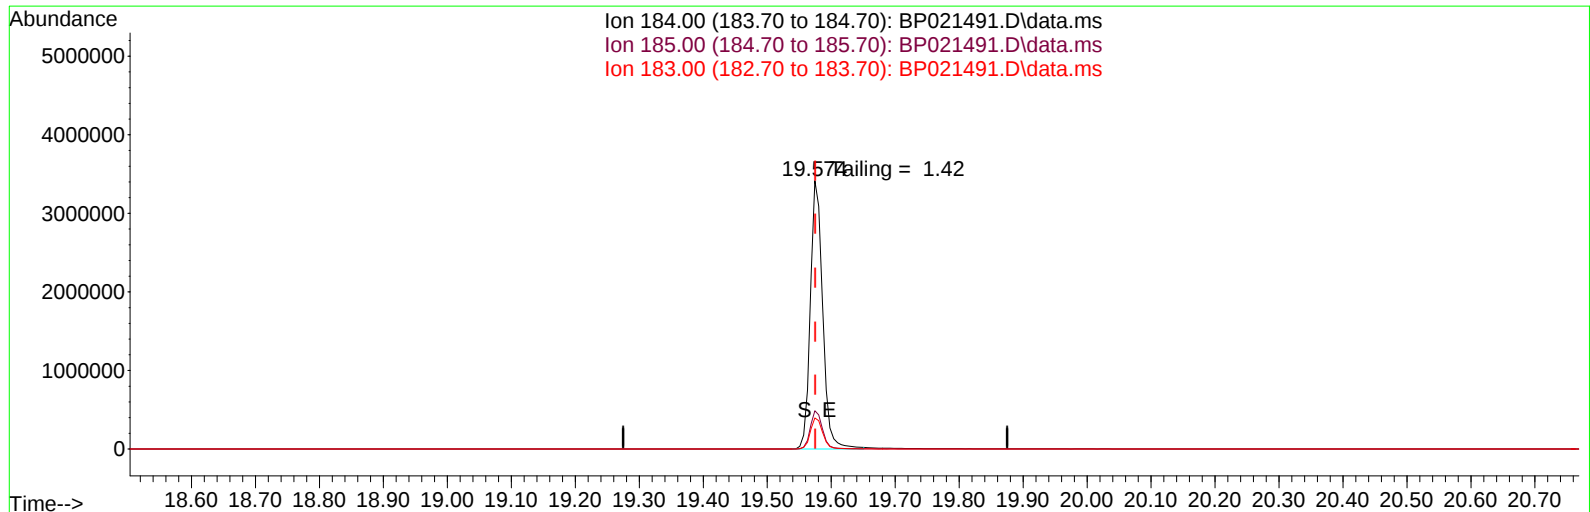

TIC: BP021491.D\data.ms

(77) Benzidine**19.574min (-0.001) -20.00 ng****response 4674021**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.26
183.00	11.60	11.58
0.00	0.00	0.00