
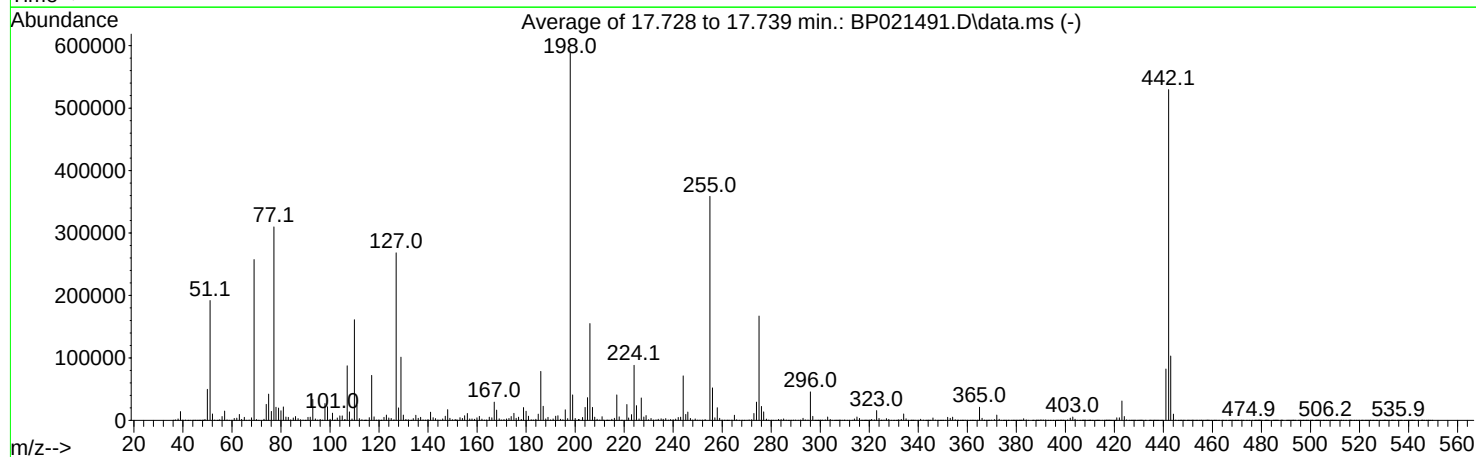


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081424\
Data File : BP021491.D
Acq On : 14 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

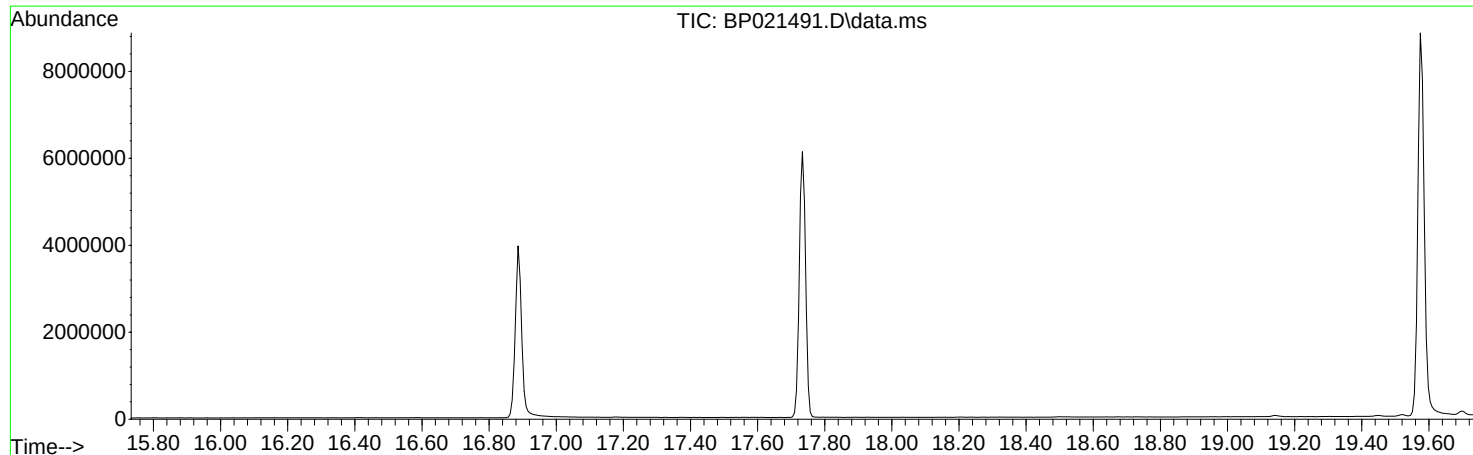

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	191979	PASS
68	69	0.00	2	1.6	4118	PASS
69	198	0.00	100	43.7	257460	PASS
70	69	0.00	2	0.5	1361	PASS
127	198	10	80	45.6	268328	PASS
197	198	0.00	2	0.5	2929	PASS
198	198	100	100	100.0	589056	PASS
199	198	5	9	6.9	40721	PASS
275	198	10	60	28.4	167079	PASS
365	198	1	100	3.6	21112	PASS
441	198	0.01	100	14.0	82397	PASS
442	442	100	100	100.0	529529	PASS
443	442	15	24	19.4	102914	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2024	BNA_P	<u>BP021491.D</u>
Compound Name	Response	Retention Time
DDT	1753680	20.886
DDD	23136	20.463
DDE	678	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23814	1777494	1.34

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081424\
Data File : BP021491.D
Acq On : 14 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:42:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

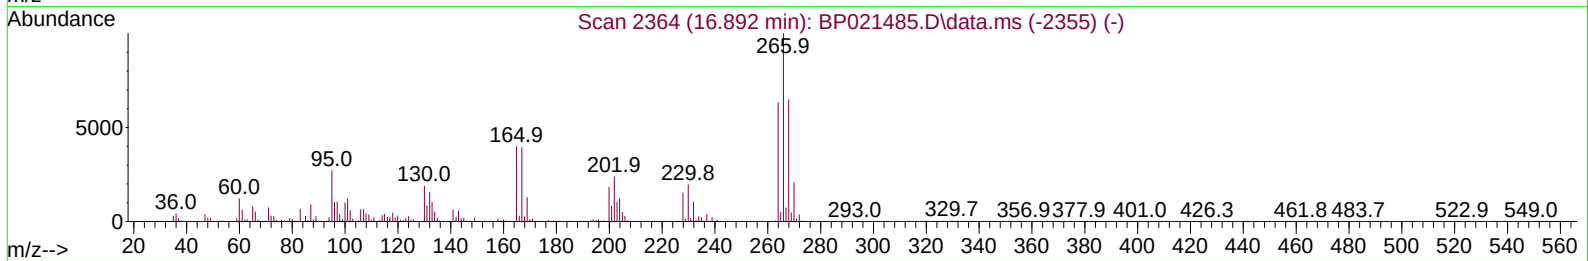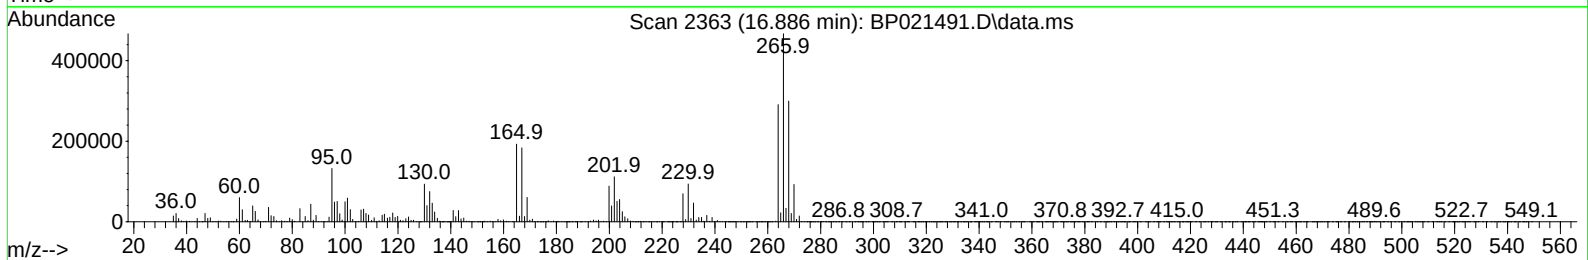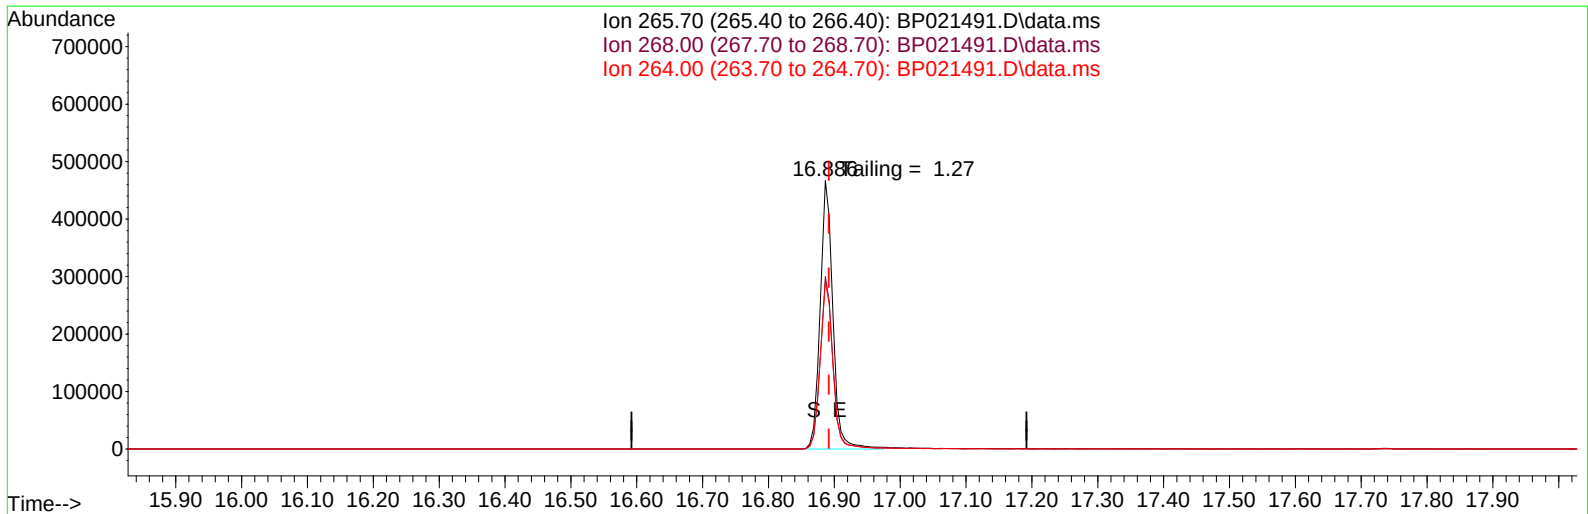

TIC: BP021491.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 3545903.77 ng




response 629359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.19
264.00	63.10	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081424\
Data File : BP021491.D
Acq On : 14 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:42:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

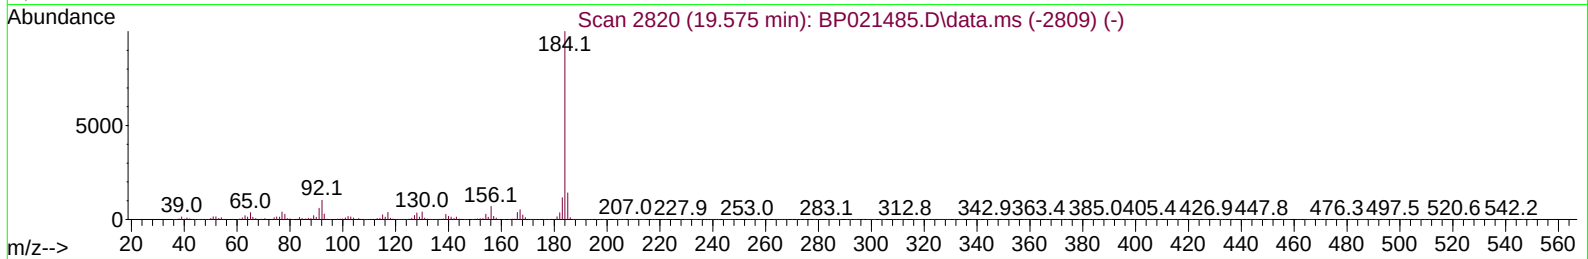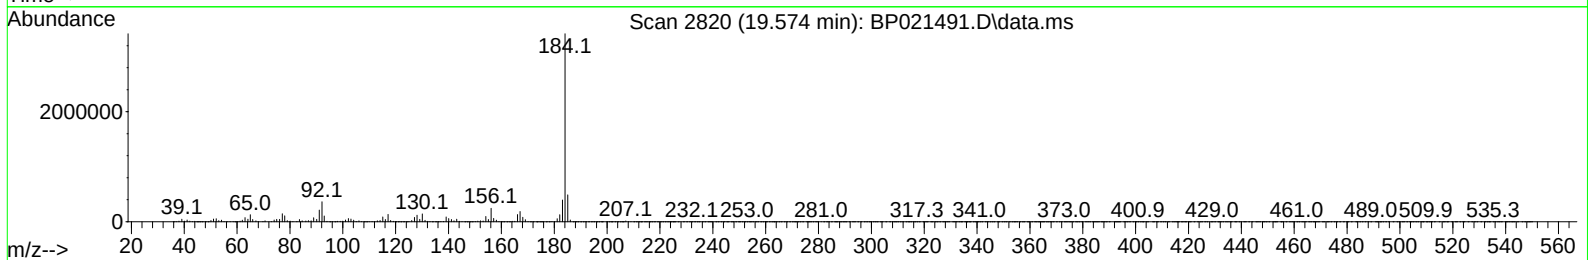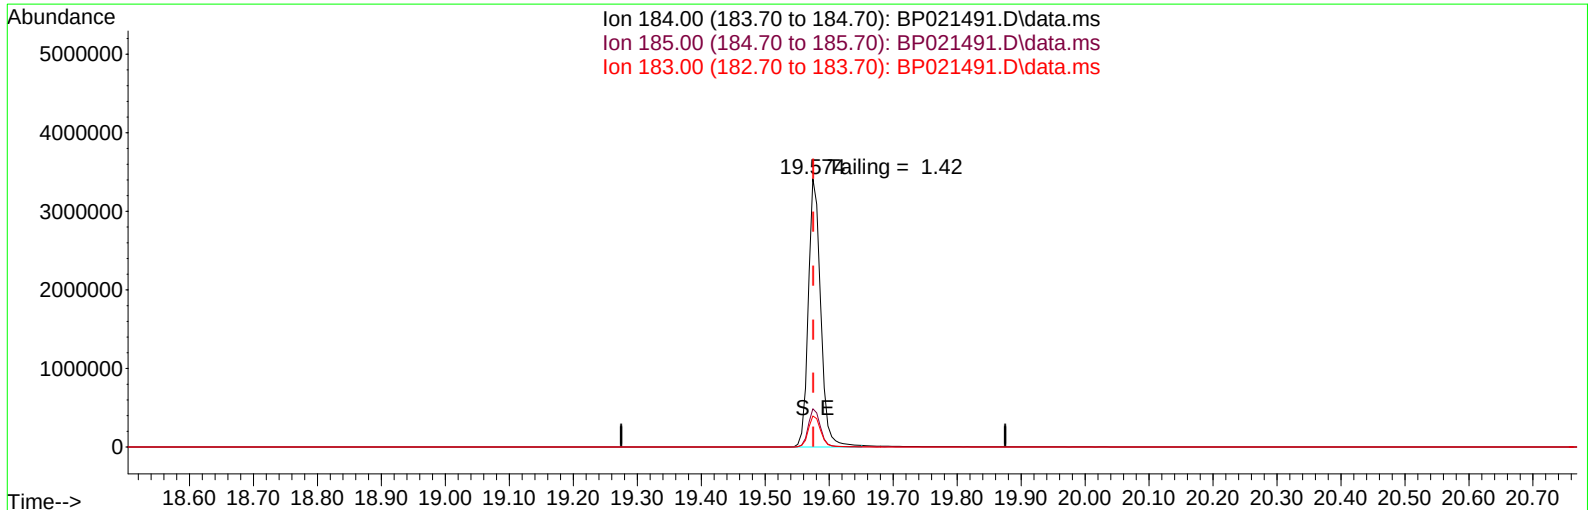

TIC: BP021491.D\data.ms

(77) Benzidine

19.574min (-0.001) -20.00 ng

response 4674021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.26
183.00	11.60	11.58
0.00	0.00	0.00