
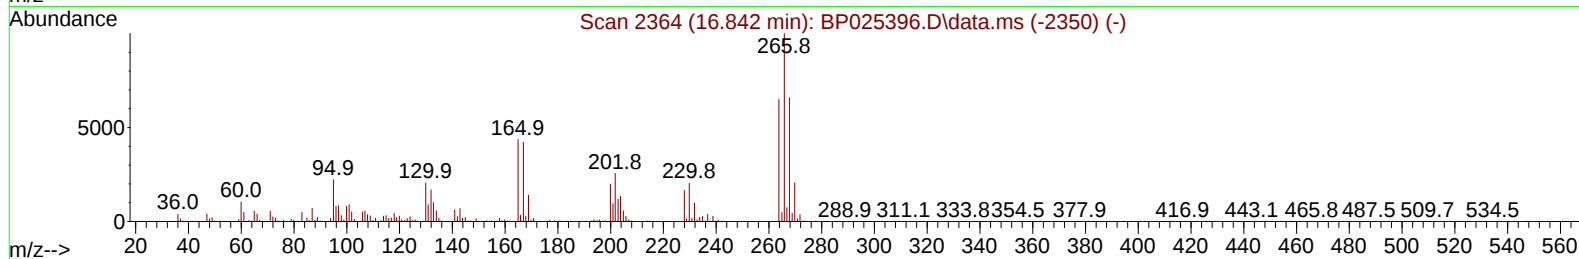
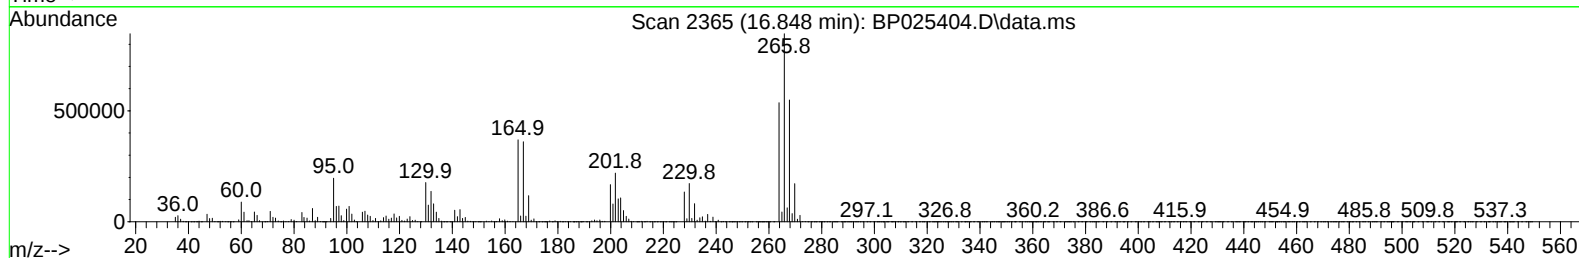


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025404.D
Acq On : 14 Aug 2025 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:47:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

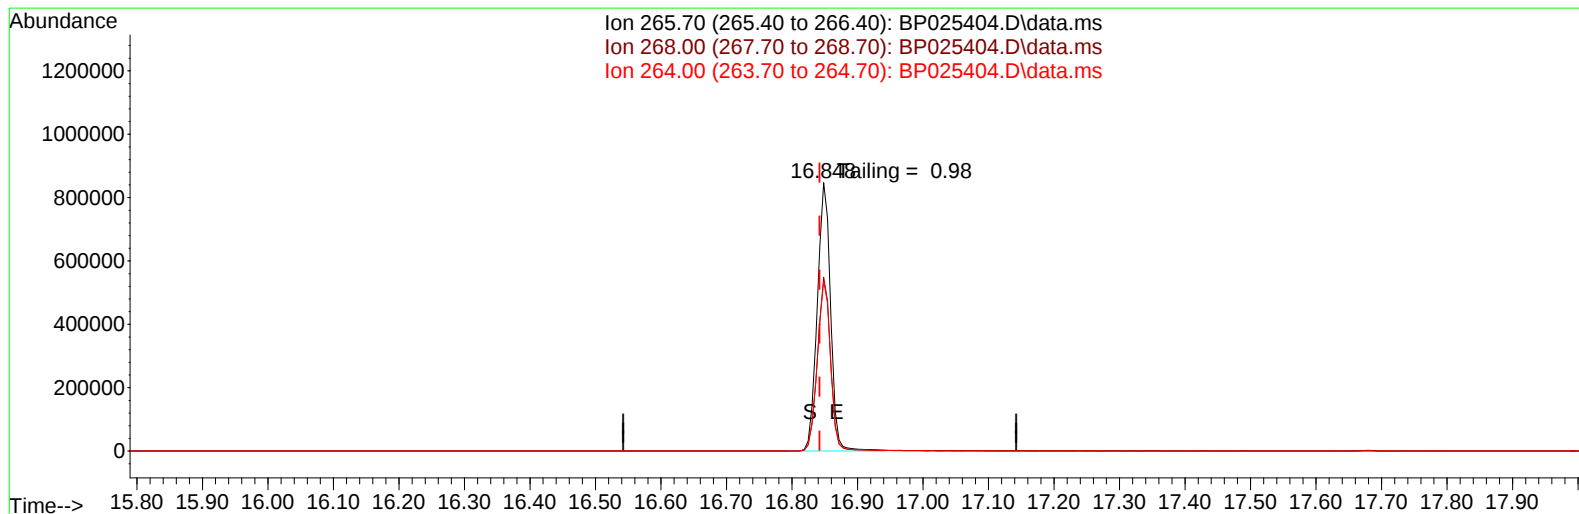

TIC: BP025404.D\data.ms

(70) Pentachlorophenol (C)




16.848min (+ 0.006) 31099.04 ng

response 1200354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.76
264.00	65.00	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025404.D
Acq On : 14 Aug 2025 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:47:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

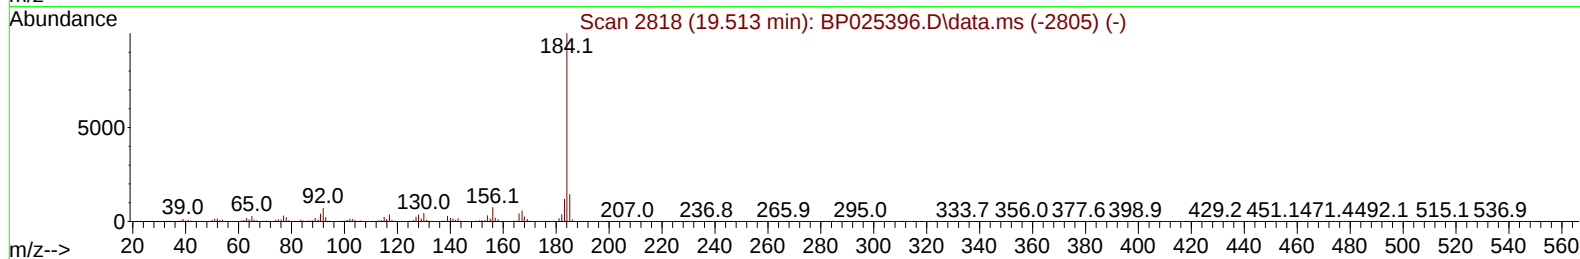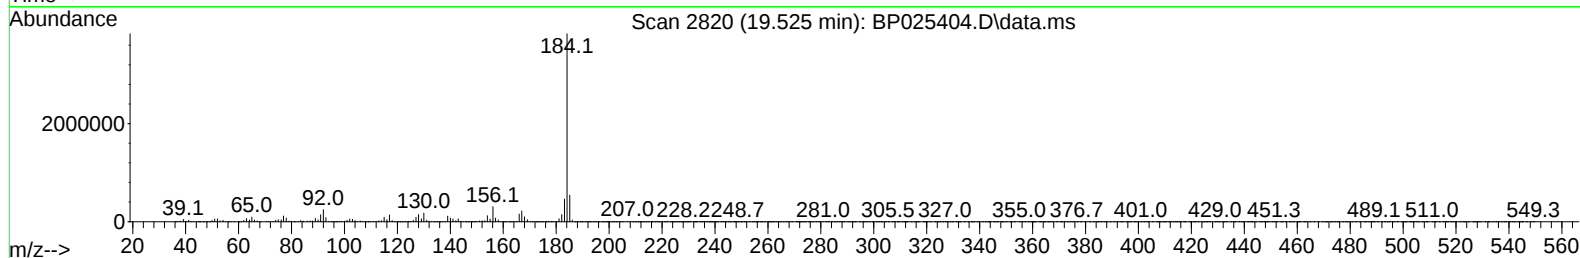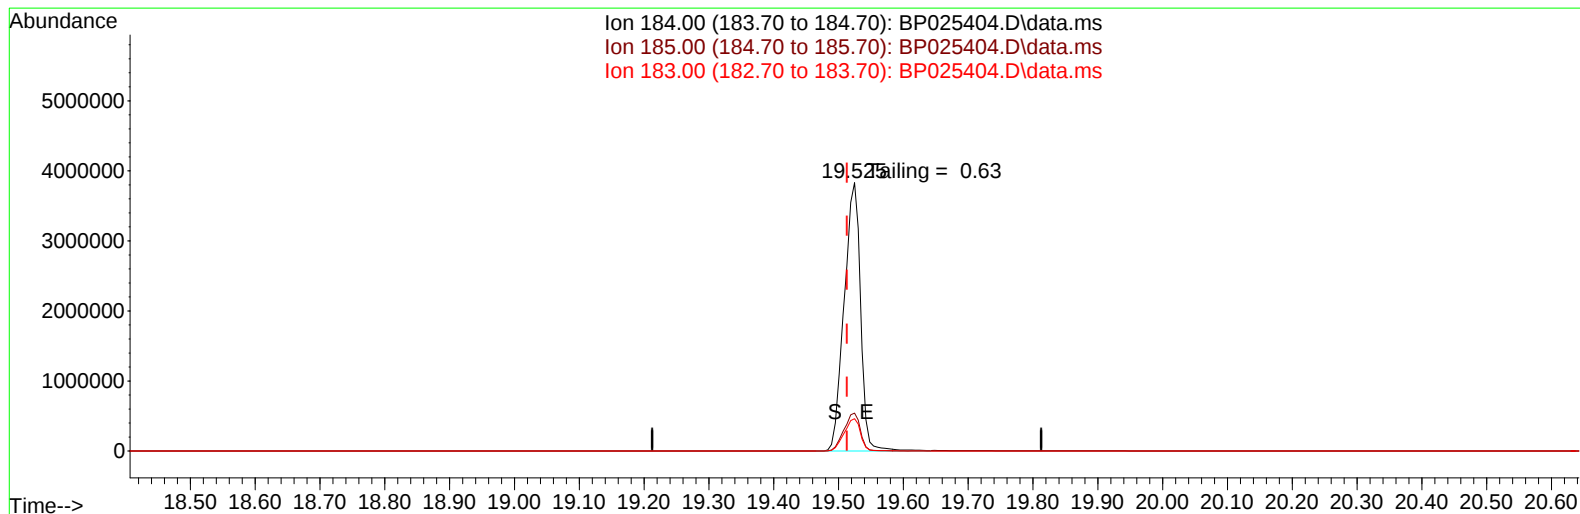

TIC: BP025404.D\data.ms

(77) Benzidine**19.525min (+ 0.012) 36687.84 ng****response 6768737**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.80	12.08
0.00	0.00	0.00