
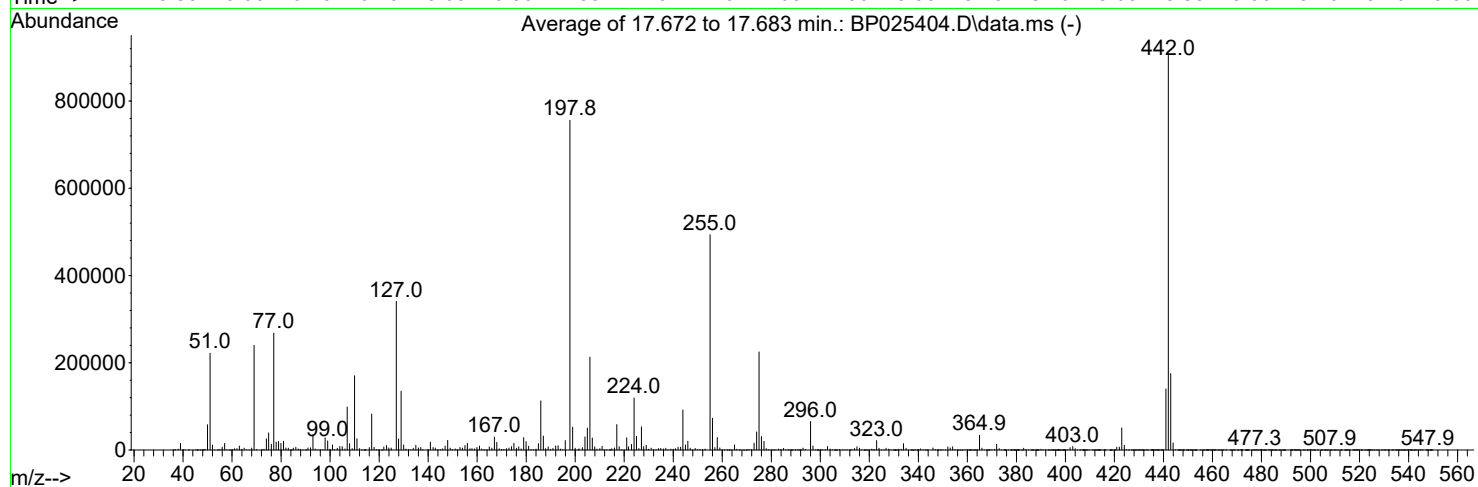


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025404.D
Acq On : 14 Aug 2025 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

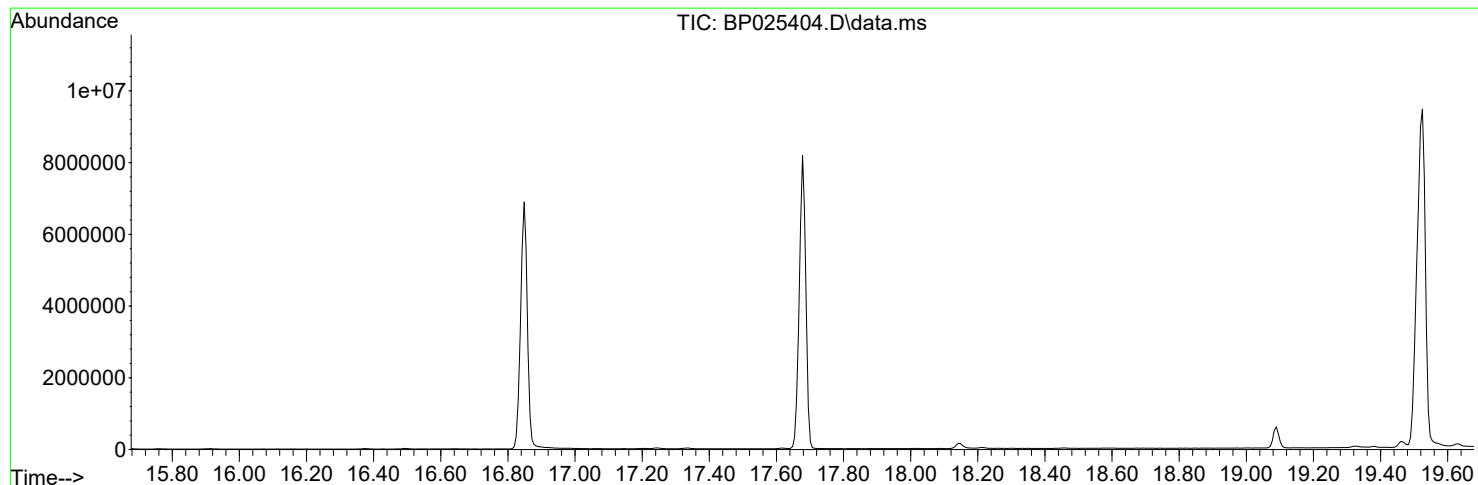

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2496

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4266	PASS
69	69	100	100	100.0	239963	PASS
70	69	0.00	2	0.5	1107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	756157	PASS
199	198	5	9	6.9	52397	PASS
365	198	1	100	4.5	33744	PASS
441	443	0.01	150	79.9	140197	PASS
442	442	100	100	100.0	905133	PASS
443	442	15	24	19.4	175487	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2025	BNA_P	<u>BP025404.D</u>
Compound Name	Response	Retention Time
DDT	3229321	20.813
DDD	27030	20.354
DDE	8790	19.824
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35820	3265141	1.10

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025404.D
Acq On : 14 Aug 2025 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:47:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

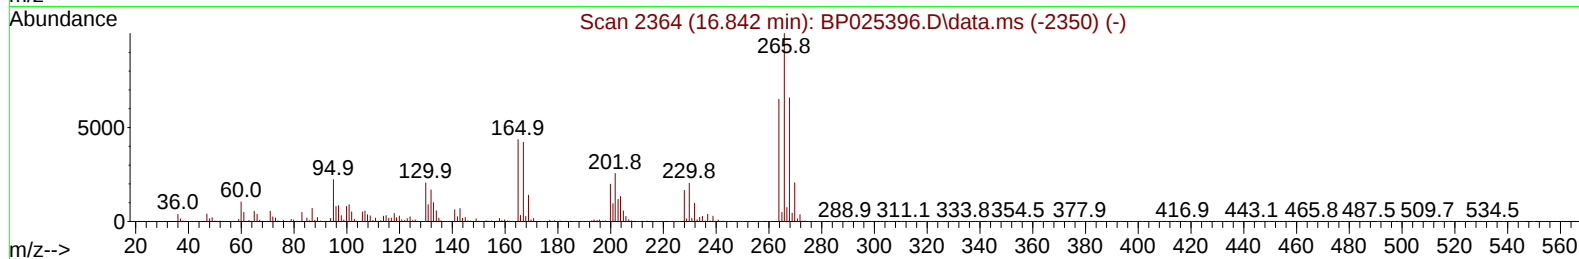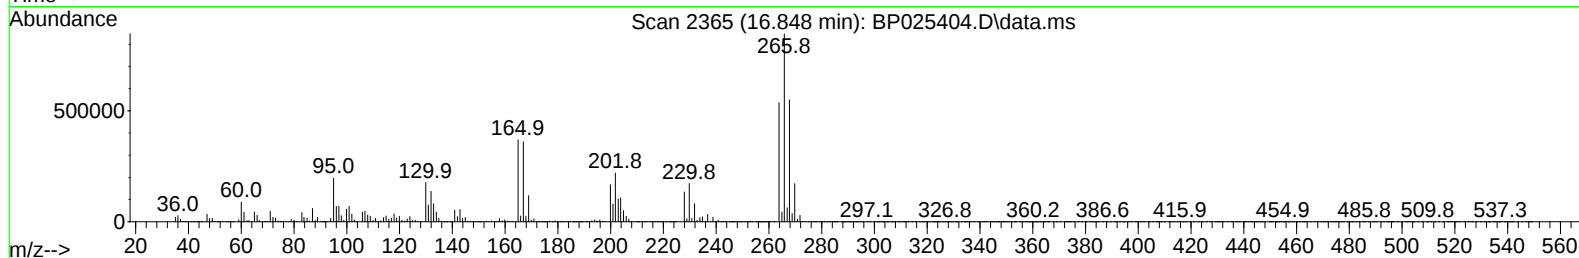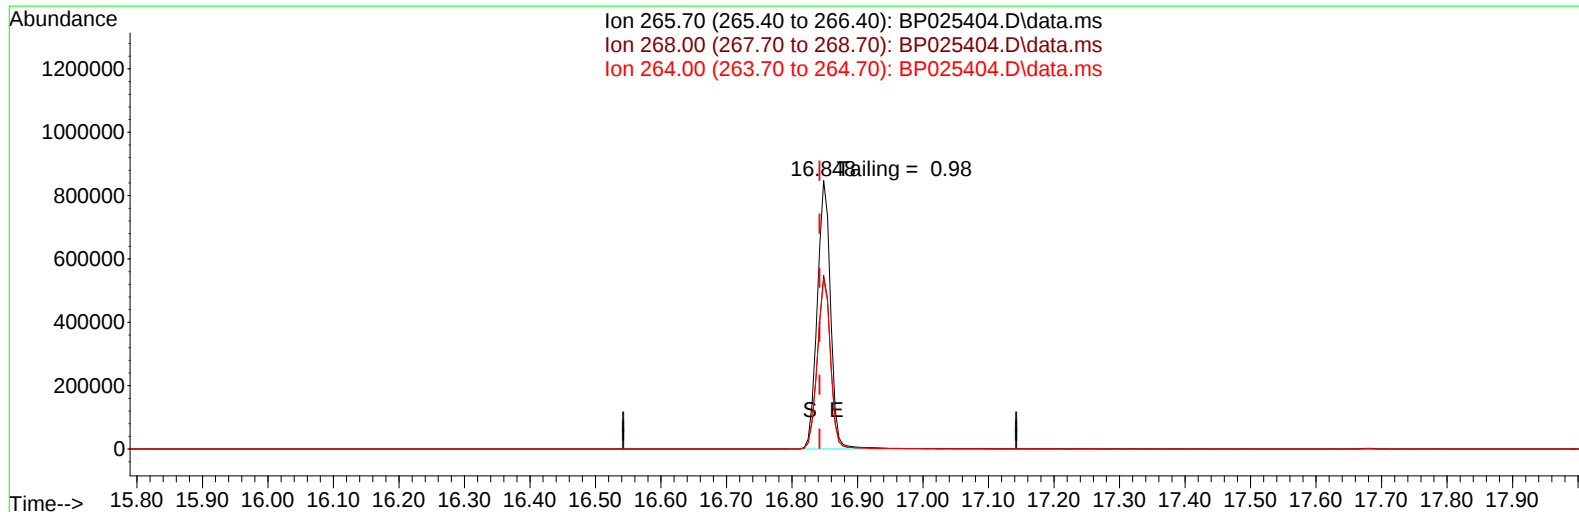

TIC: BP025404.D\data.ms

(70) Pentachlorophenol (C)

16.848min (+ 0.006) 31099.04 ng




response 1200354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.76
264.00	65.00	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081425\
Data File : BP025404.D
Acq On : 14 Aug 2025 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:47:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

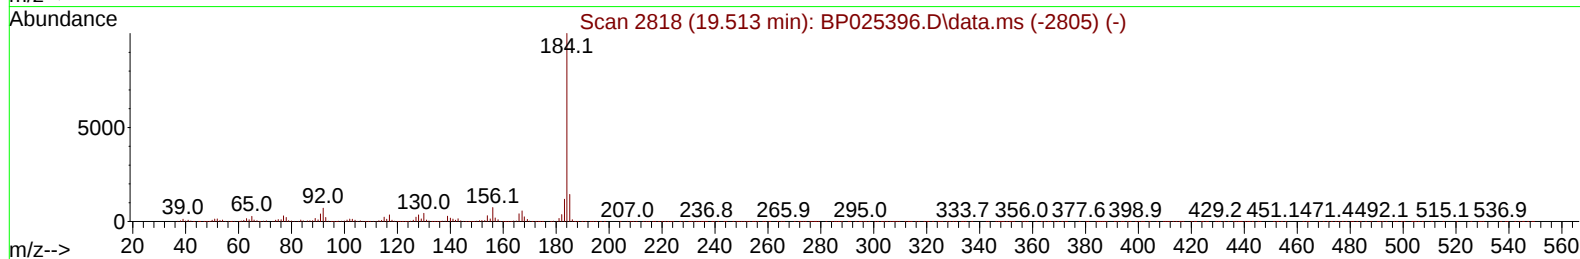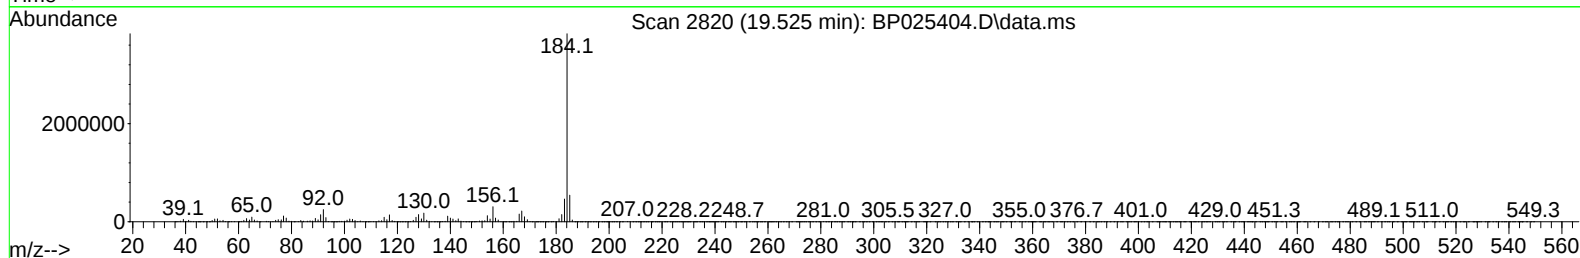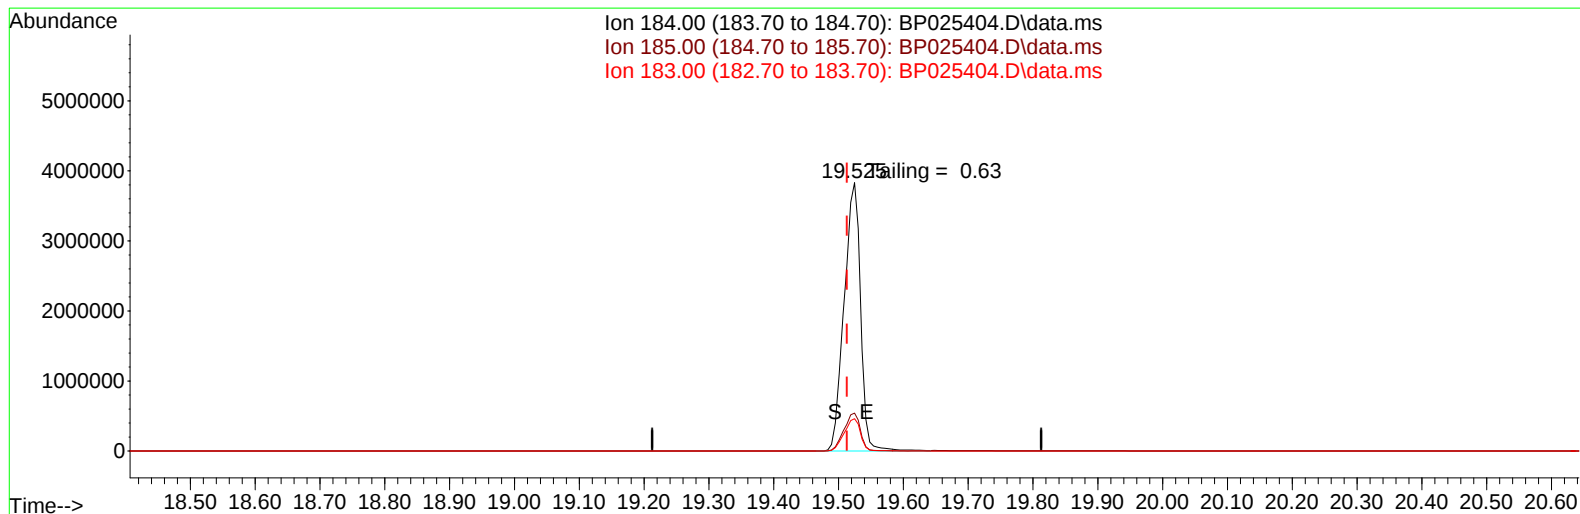

TIC: BP025404.D\data.ms

(77) Benzidine

19.525min (+ 0.012) 36687.84 ng

response 6768737

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.80	12.08
0.00	0.00	0.00