
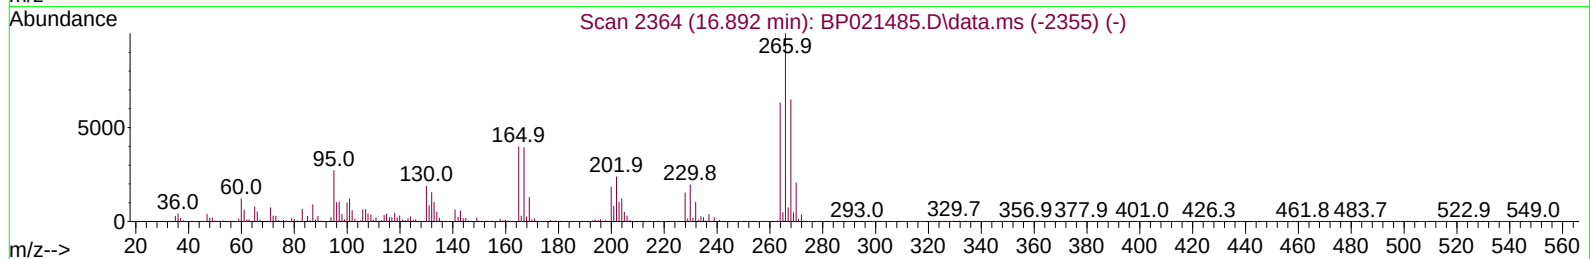
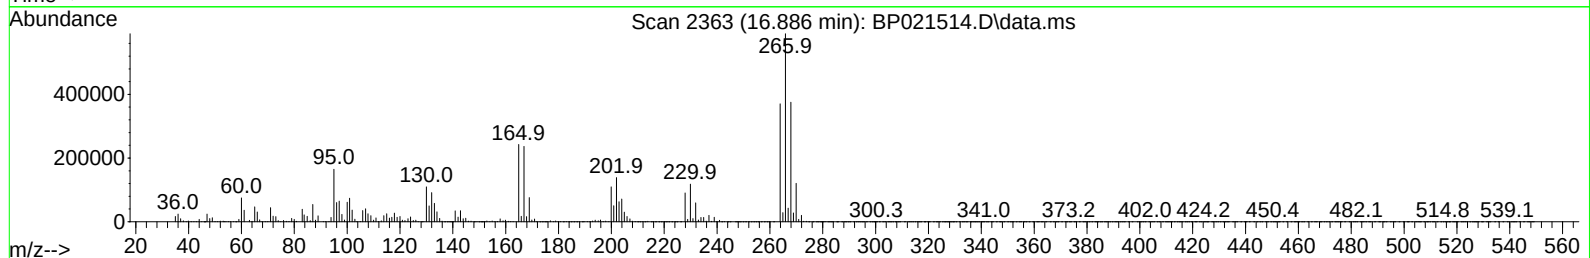


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081524\  
Data File : BP021514.D  
Acq On : 15 Aug 2024 14:54  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 02:36:33 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 14 00:00:30 2024  
Response via : Initial Calibration

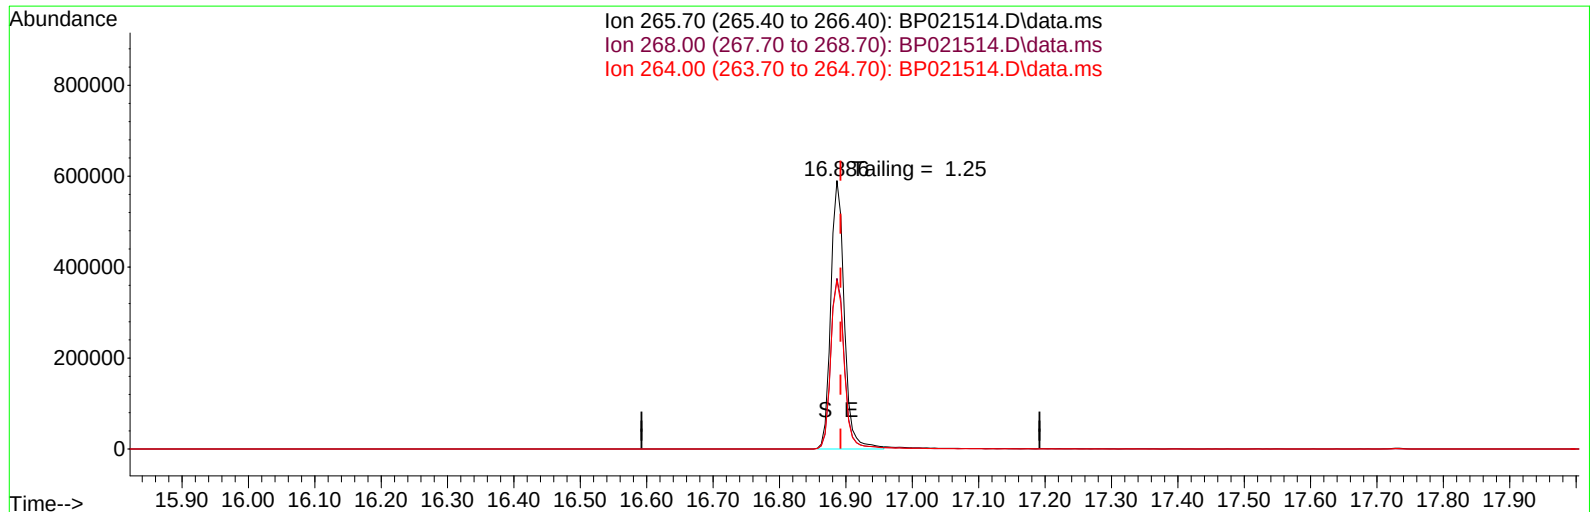

TIC: BP021514.D\data.ms

**(70) Pentachlorophenol (C)**




16.886min (-0.006) 525145.52 ng

response 842453

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.70  | 63.58  |
| 264.00 | 63.10  | 62.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP081524\  
Data File : BP021514.D  
Acq On : 15 Aug 2024 14:54  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 02:36:33 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP081324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 14 00:00:30 2024  
Response via : Initial Calibration

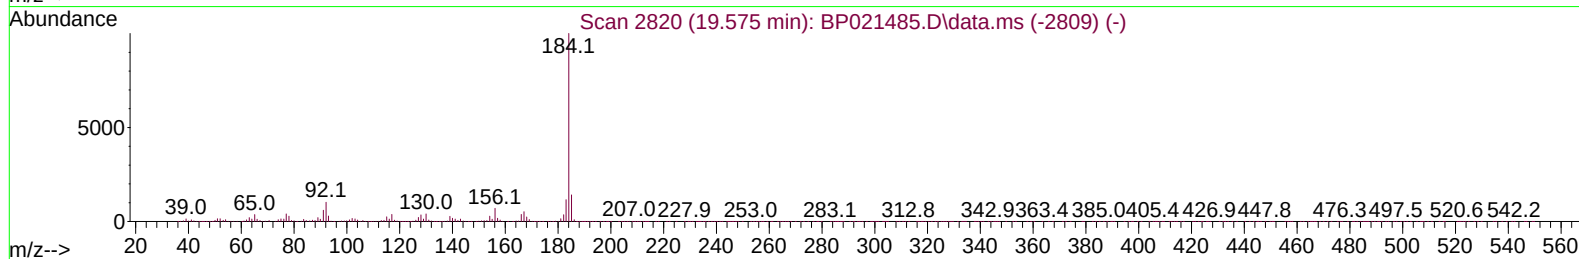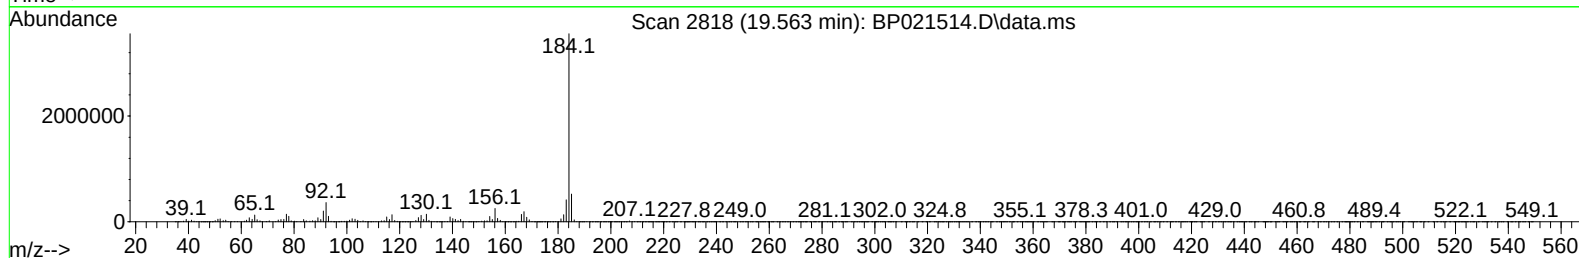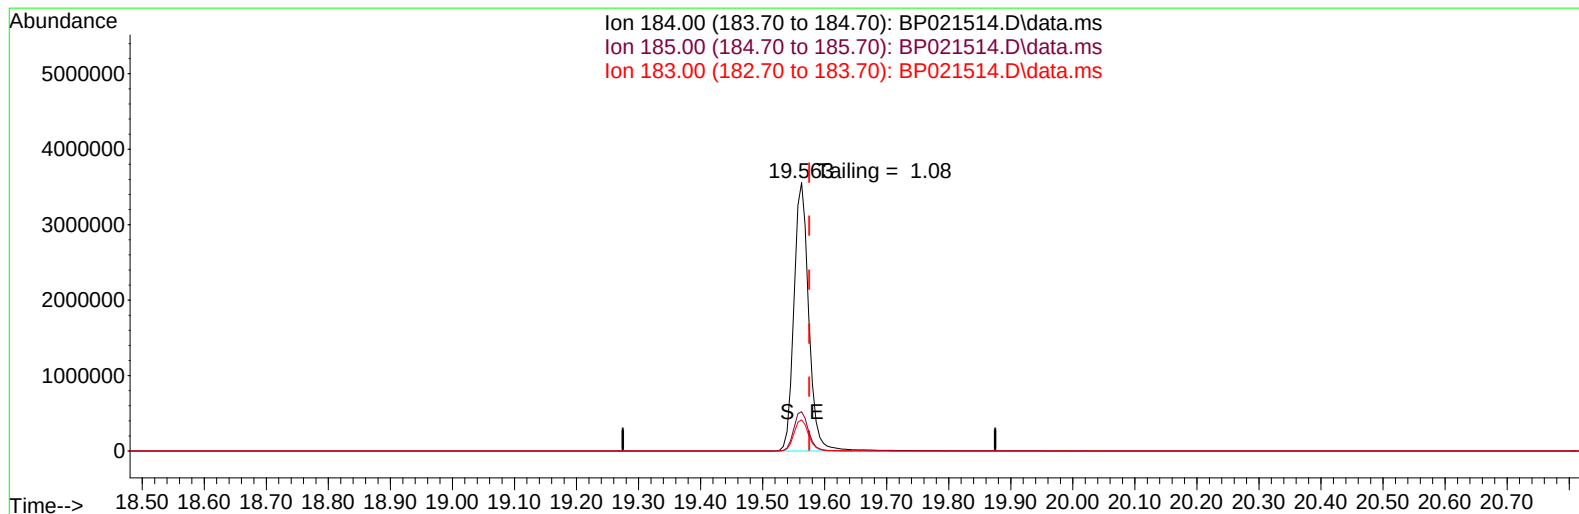

TIC: BP021514.D\data.ms

**(77) Benzidine**

19.563min (-0.012) -20.00 ng

response 5959833

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.70  |
| 183.00 | 11.60  | 11.67  |
| 0.00   | 0.00   | 0.00   |