


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081524\
Data File : BP021505.D
Acq On : 15 Aug 2024 08:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

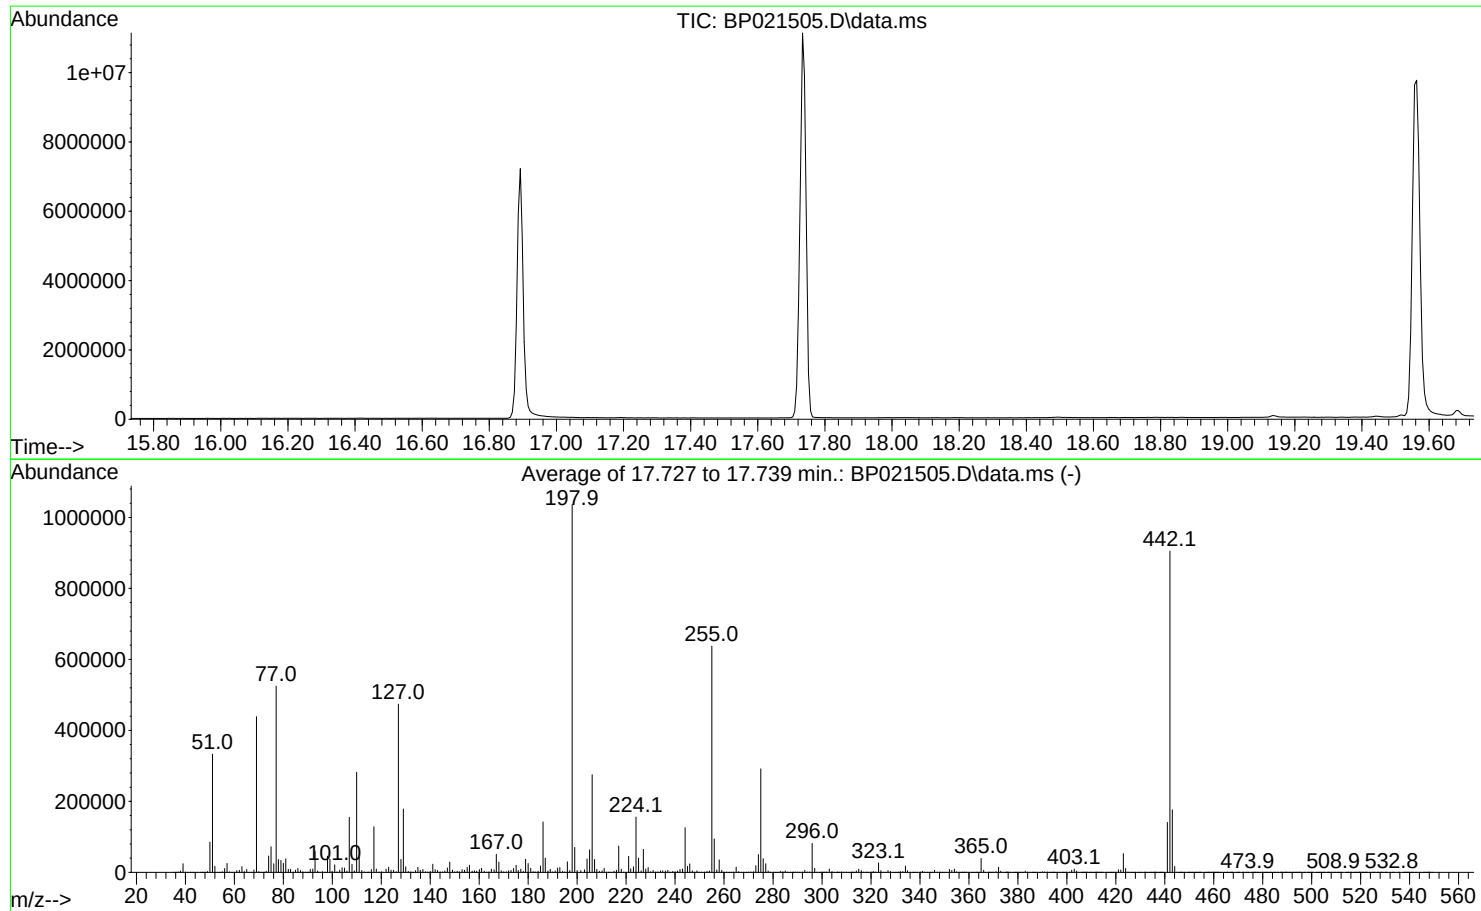

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	333437	PASS
68	69	0.00	2	1.5	6786	PASS
69	198	0.00	100	42.3	438868	PASS
70	69	0.00	2	0.5	2364	PASS
127	198	10	80	45.7	474019	PASS
197	198	0.00	2	0.5	5022	PASS
198	198	100	100	100.0	1036480	PASS
199	198	5	9	6.8	70258	PASS
275	198	10	60	28.2	291797	PASS
365	198	1	100	3.8	39338	PASS
441	198	0.01	100	13.6	140802	PASS
442	442	100	100	100.0	905024	PASS
443	442	15	24	19.5	176205	PASS