
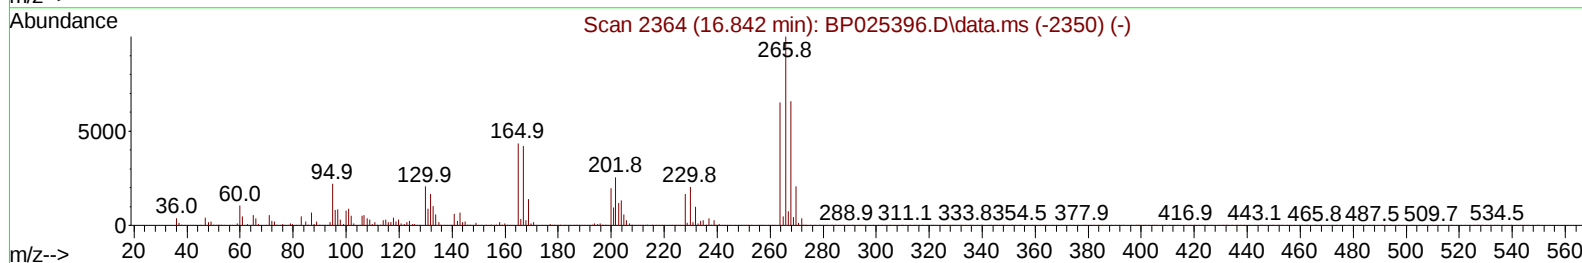
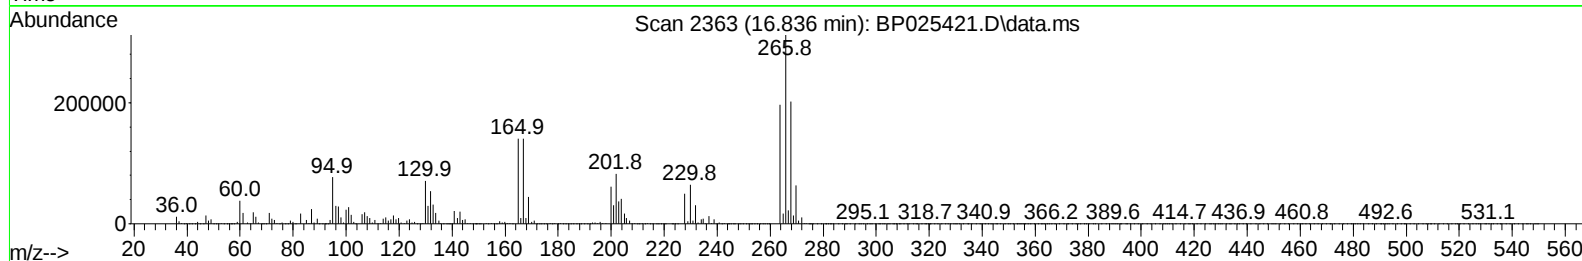


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025421.D
Acq On : 15 Aug 2025 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 11:28:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

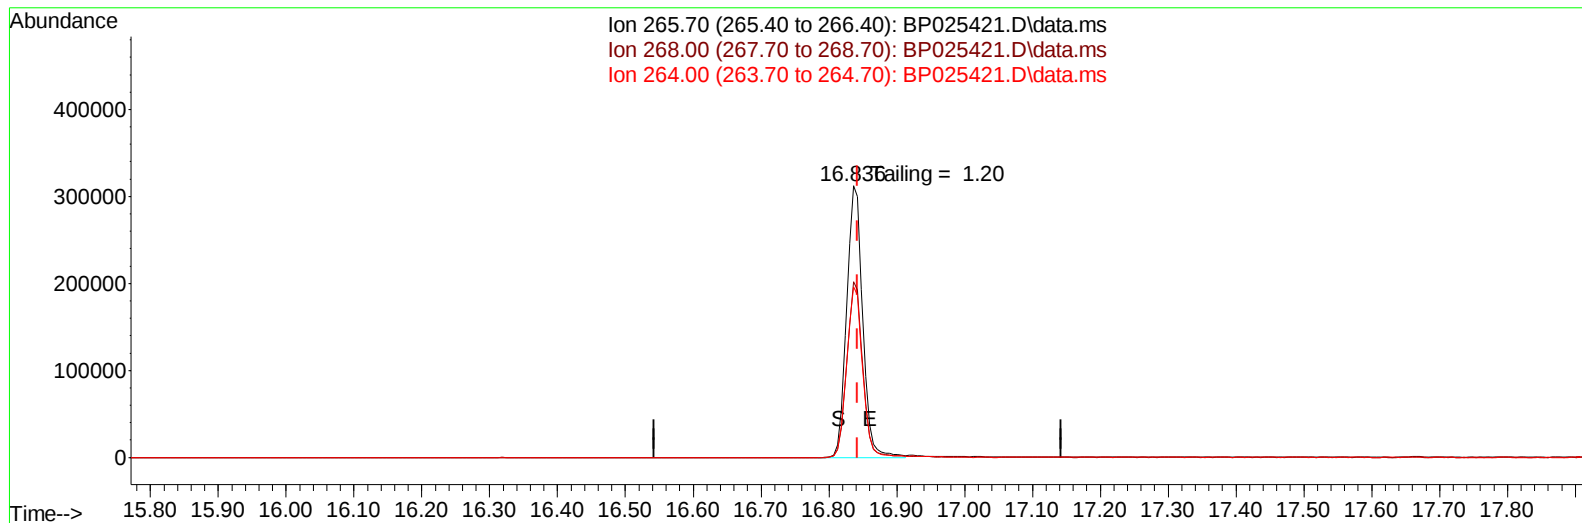

TIC: BP025421.D\data.ms

(70) Pentachlorophenol (C)




16.836min (-0.006) 99008.85 ng

response 510758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	64.63
264.00	65.00	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025421.D
Acq On : 15 Aug 2025 09:55
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 11:28:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

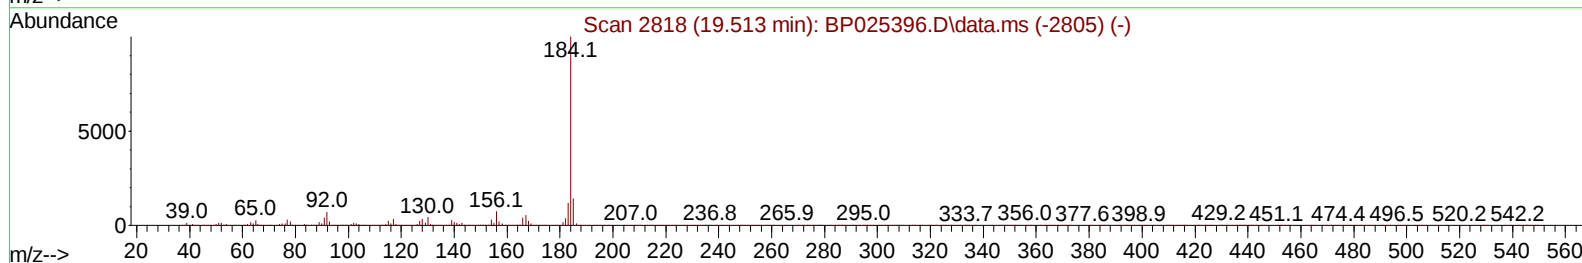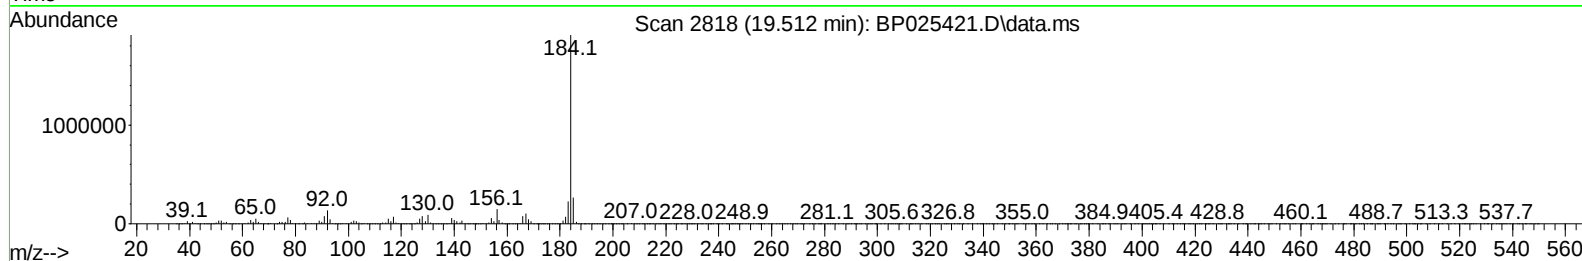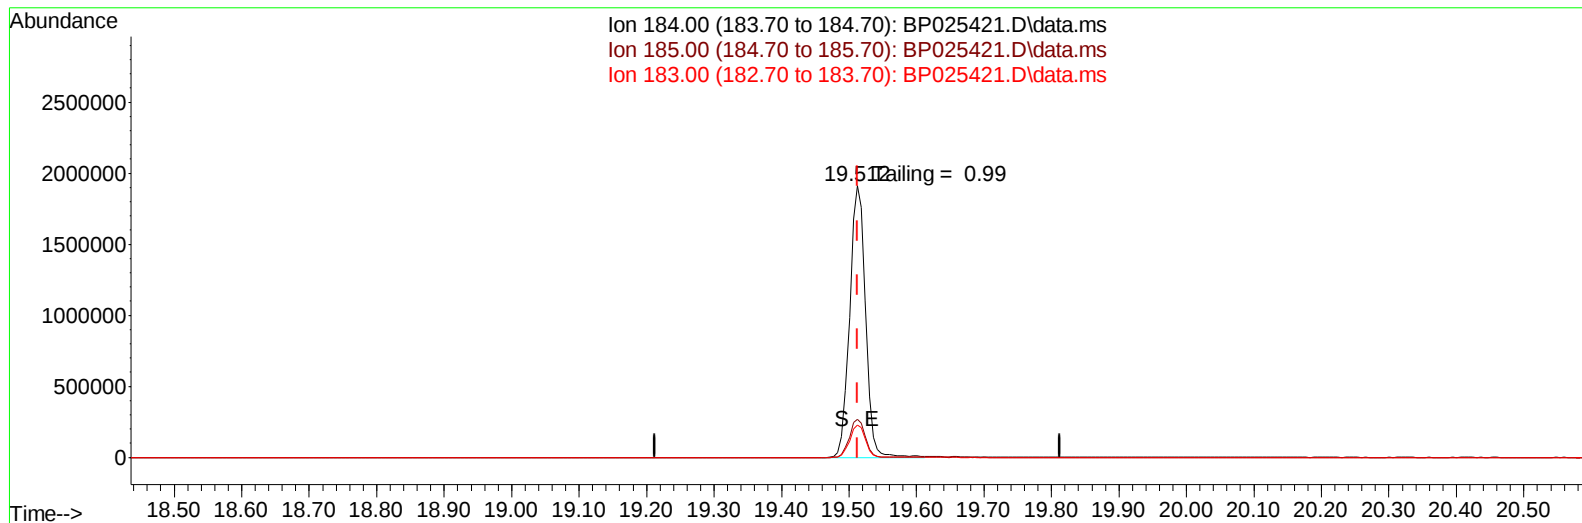

TIC: BP025421.D\data.ms

(77) Benzidine**19.512min (-0.000) 55650.72 ng****response 3124253**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.80	11.97
0.00	0.00	0.00