
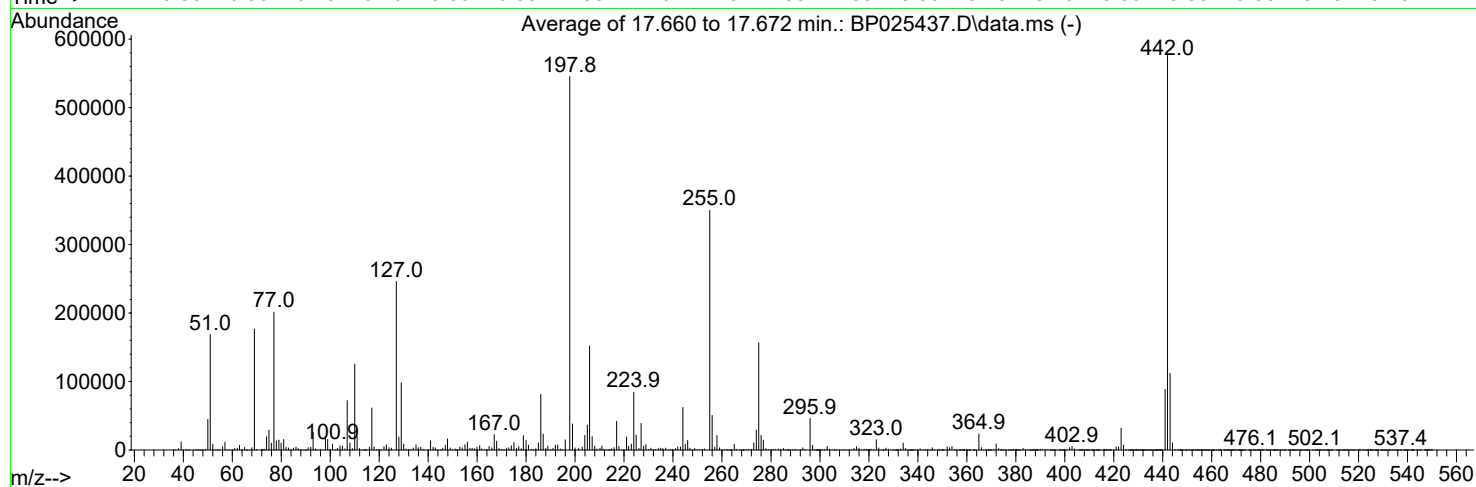


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025437.D
Acq On : 15 Aug 2025 23:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

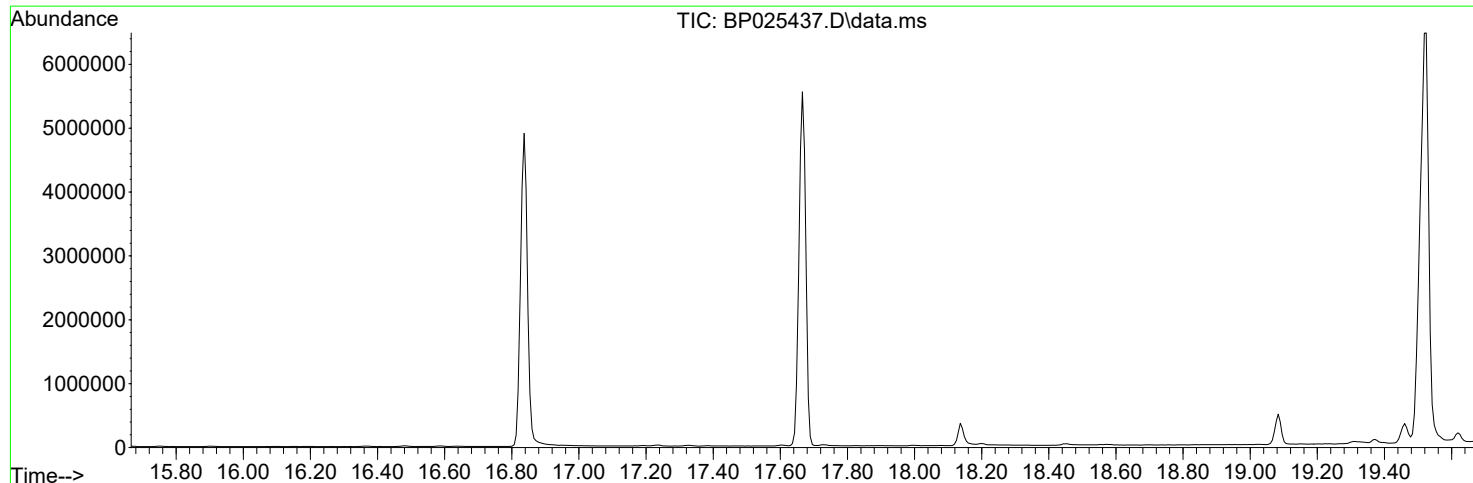

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	3221	PASS
69	69	100	100	100.0	176647	PASS
70	69	0.00	2	0.5	852	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	545515	PASS
199	198	5	9	7.0	38005	PASS
365	198	1	100	4.2	23066	PASS
441	443	0.01	150	79.0	88504	PASS
442	442	100	100	100.0	576619	PASS
443	442	15	24	19.4	111960	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/15/2025	BNA_P	<u>BP025437.D</u>
Compound Name	Response	Retention Time
DDT	1896735	20.813
DDD	379213	20.342
DDE	4481	19.825
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
383694	2280429	16.83

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025437.D
Acq On : 15 Aug 2025 23:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 18 01:55:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

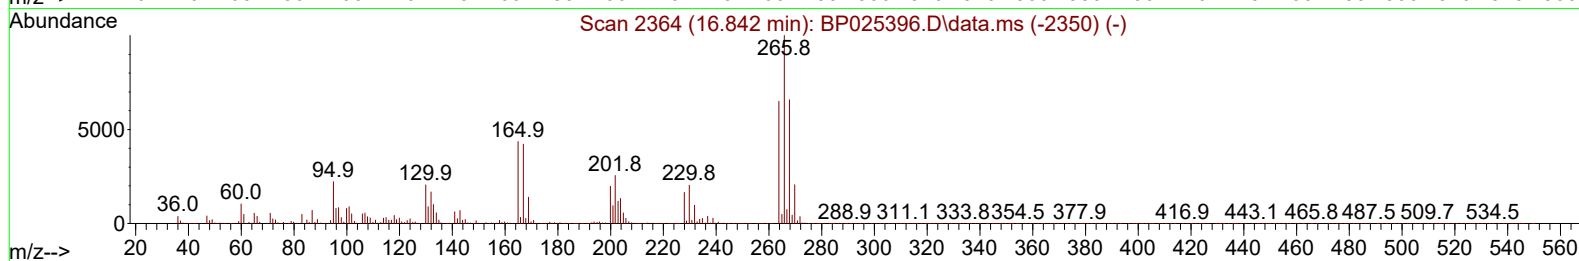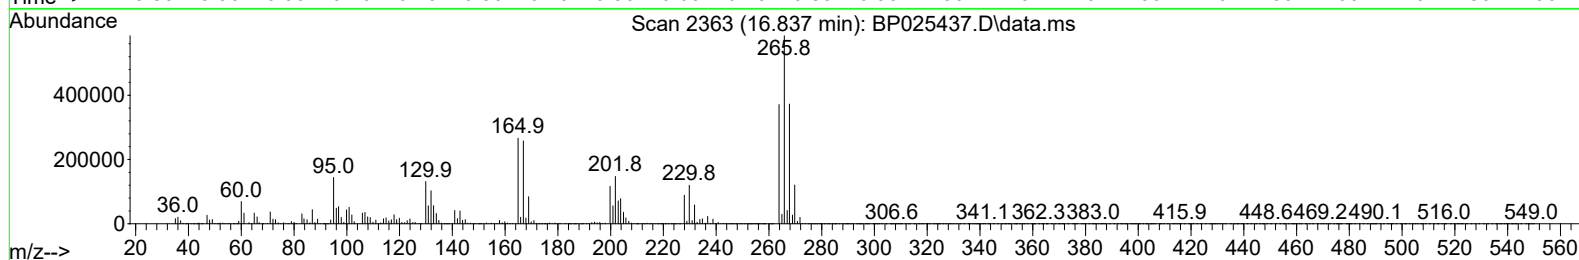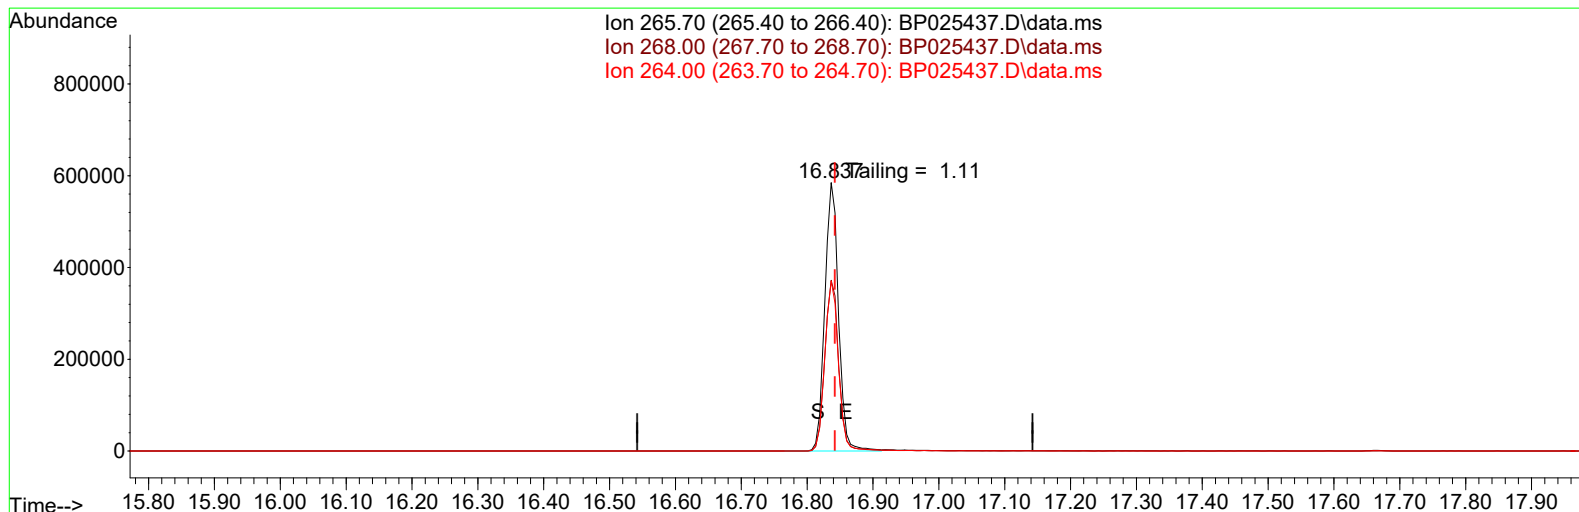

TIC: BP025437.D\data.ms

(70) Pentachlorophenol (C)

16.837min (-0.006) 31008.18 ng


response 855960

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.64
264.00	65.00	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081525\
Data File : BP025437.D
Acq On : 15 Aug 2025 23:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 18 01:55:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

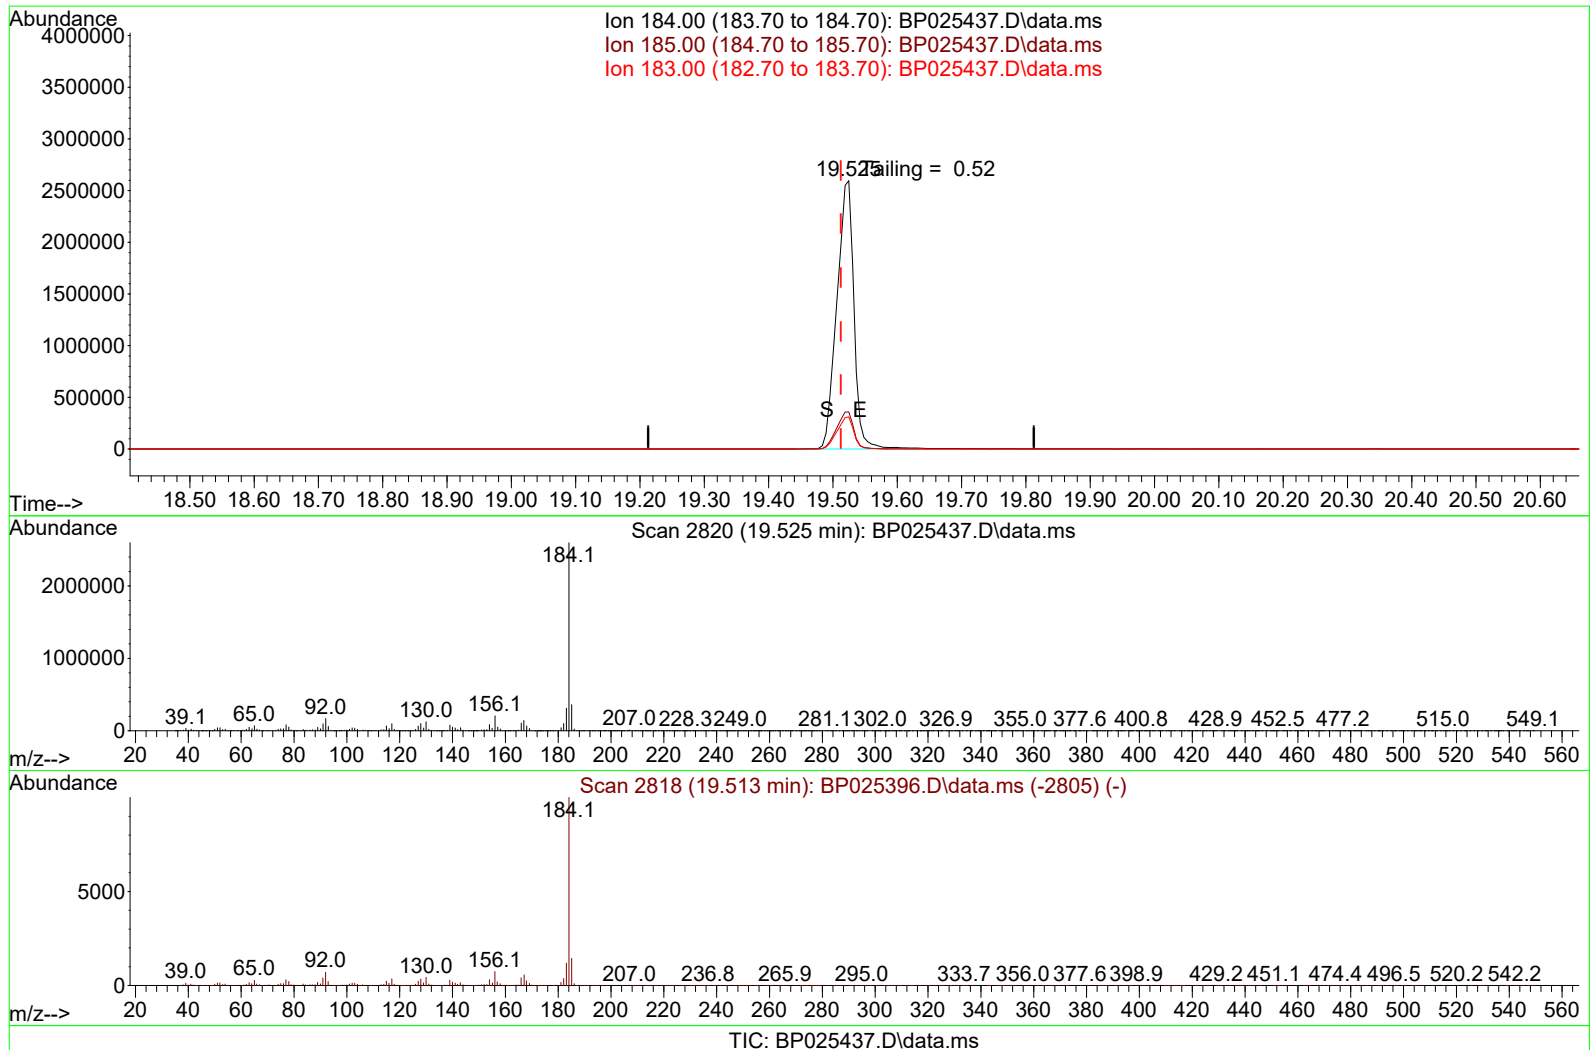

TIC: BP025437.D\data.ms

(77) Benzidine

19.525min (+ 0.012) 27113.16 ng

response 4803310

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.80	11.98
0.00	0.00	0.00