

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081622\
 Data File : BP011449.D
 Acq On : 16 Aug 2022 18:01
 Operator : CG/JU
 Sample : SST08047
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080649

Quant Time: Aug 17 01:09:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:01:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	76387	20.000	ng/u1	0.00
20) Naphthalene-d8	10.352	136	345439	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.234	164	207568	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.004	188	424168	20.000	ng/u1	0.00
79) Chrysene-d12	21.139	240	405619	20.000	ng/u1	0.00
88) Perylene-d12	23.427	264	393049	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	79933	32.079	ng/uL	0.00
4) Pyridine-d5	3.475	84	532116	84.659	ng/u1	0.00
7) Phenol-d5	6.746	99	601369	88.959	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.911	67	376751	78.601	ng/u1	0.00
11) 2-Chlorophenol-d4	7.093	132	465982	87.853	ng/u1	0.00
15) 4-Methylphenol-d8	8.293	113	477454	89.952	ng/u1	0.01
21) Nitrobenzene-d5	8.728	128	232616	98.945	ng/u1	0.00
24) 2-Nitrophenol-d4	9.446	143	248246	115.333	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	424369	97.629	ng/u1	0.00
31) 4-Chloroaniline-d4	10.504	131	662927	87.236	ng/u1	0.00
46) Dimethylphthalate-d6	13.663	166	1279375	88.833	ng/u1	0.00
49) Acenaphthylene-d8	13.928	160	1485112	85.663	ng/u1	0.00
54) 4-Nitrophenol-d4	14.475	143	259670	98.715	ng/u1	0.01
60) Fluorene-d10	15.240	176	1069100	86.801	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.381	200	213116	108.169	ng/u1	0.01
73) Anthracene-d10	17.110	188	1659869	87.062	ng/u1	0.00
81) Pyrene-d10	19.369	212	1808257	80.917	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.286	264	1744485	88.009	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.099	88	84126	31.785	ng/uL	99
5) Pyridine	3.493	79	534142	81.585	ng/u1	99
6) Benzaldehyde	6.716	77	251797	85.469	ng/u1	98
8) Phenol	6.775	94	618181	84.482	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.005	93	467156	79.273	ng/u1	99
12) 2-Chlorophenol	7.128	128	488678	88.418	ng/u1	97
13) 2-Methylphenol	8.016	108	457002	86.720	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.093	45	395011	44.691	ng/u1	99
16) Acetophenone	8.393	105	784951	91.404	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.393	70	413310	97.697	ng/u1	99
18) 4-Methylphenol	8.358	108	498564	88.264	ng/u1	100
19) Hexachloroethane	8.628	117	217081	93.020	ng/u1	99
22) Nitrobenzene	8.769	77	626782	95.237	ng/u1	97
23) Isophorone	9.305	82	1118480	92.650	ng/u1	99
25) 2-Nitrophenol	9.475	139	272685	108.705	ng/u1	96
26) 2,4-Dimethylphenol	9.546	107	610773	96.361	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.787	93	641888	83.201	ng/u1	97
29) 2,4-Dichlorophenol	10.005	162	426111	93.742	ng/u1	98
30) Naphthalene	10.399	128	1547271	82.328	ng/u1	99
32) 4-Chloroaniline	10.528	127	685854	90.041	ng/u1	99
33) Hexachlorobutadiene	10.681	225	256249	91.891	ng/u1	97
34) Caprolactam	11.346	113	84943	55.881	ng/u1	99
35) 4-Chloro-3-methylphenol	11.675	107	551495	103.191	ng/u1	98
36) 2-Methylnaphthalene	12.028	142	1021550	87.690	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081622\
 Data File : BP011449.D
 Acq On : 16 Aug 2022 18:01
 Operator : CG/JU
 Sample : SST08047
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080649

Quant Time: Aug 17 01:09:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:01:09 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.251	142	1035984	87.671	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.398	216	458732	83.948	ng/ul	97
40) Hexachlorocyclopentadiene	12.375	237	300019	102.457	ng/ul	99
41) 2,4,6-Trichlorophenol	12.657	196	322219	97.455	ng/ul	98
42) 2,4,5-Trichlorophenol	12.728	196	344635	97.662	ng/ul	99
43) 1,1'-Biphenyl	13.063	154	1341802	82.323	ng/ul	99
44) 2-Chloronaphthalene	13.098	162	1009199	82.523	ng/ul	98
45) 2-Nitroaniline	13.328	65	407385	131.163	ng/ul	97
47) Dimethylphthalate	13.710	163	1311144	89.883	ng/ul	100
48) 2,6-Dinitrotoluene	13.834	165	271587	119.075	ng/ul	100
50) Acenaphthylene	13.957	152	1720353	86.085	ng/ul	99
51) 3-Nitroaniline	14.163	138	274505	109.408	ng/ul	100
52) Acenaphthene	14.298	153	1123783	84.316	ng/ul	100
53) 2,4-Dinitrophenol	14.375	184	164110	121.271	ng/ul	98
55) 4-Nitrophenol	14.493	109	307893	126.173	ng/ul	94
56) Dibenzofuran	14.640	168	1525383	84.419	ng/ul	99
57) 2,4-Dinitrotoluene	14.628	165	399560	114.292	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	14.875	232	273728	99.711	ng/ul	98
59) Diethylphthalate	15.092	149	1458578	96.520	ng/ul	99
61) Fluorene	15.298	166	1289289	87.861	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.298	204	572502	89.251	ng/ul	99
63) 4-Nitroaniline	15.345	138	238277	97.599	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.392	198	216998	106.962	ng/ul	93
67) N-Nitrosodiphenylamine	15.516	169	1084228	86.743	ng/ul	98
68) 4-Bromophenyl-phenylether	16.198	248	332704	88.637	ng/ul	97
69) Hexachlorobenzene	16.298	284	378693	86.358	ng/ul	98
70) Atrazine	16.498	200	400178	96.052	ng/ul	97
71) Pentachlorophenol	16.657	266	244858	96.185	ng/ul	99
72) Phenanthrene	17.051	178	1959880	82.402	ng/ul	99
74) Anthracene	17.145	178	2012205	84.983	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.016	216	470800	77.314	ng/ul	97
76) Pentachlorobenzene	14.551	250	446762	84.244	ng/ul	99
77) Carbazole	17.428	167	1854031	83.795	ng/ul	99
78) Di-n-butylphthalate	17.998	149	2534109	104.742	ng/ul	99
80) Fluoranthene	19.045	202	2259178	83.057	ng/ul	98
82) Pyrene	19.398	202	2324214	80.956	ng/ul	99
83) Butylbenzylphthalate	20.298	149	1176093	128.551	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.063	252	672656	91.122	ng/ul	99
85) Benzo(a)anthracene	21.122	228	2166272	83.245	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.063	149	1768753	120.430	ng/ul	100
87) Chrysene	21.174	228	2111609	81.971	ng/ul	99
89) Di-n-octyl phthalate	21.957	149	2908495	106.652	ng/ul	100
90) Benzo(b)fluoranthene	22.739	252	2188940	84.616	ng/ul	99
91) Benzo(k)fluoranthene	22.786	252	2122218	83.848	ng/ul	98
93) Benzo(a)pyrene	23.333	252	2161487	86.631	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.804	276	2441287	88.508	ng/ul	99
95) Dibenzo(a,h)anthracene	25.821	278	2111618	90.016	ng/ul	98
96) Benzo(g,h,i)perylene	26.533	276	2028607	87.160	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081622\
 Data File : BP011449.D
 Acq On : 16 Aug 2022 18:01
 Operator : CG/JU
 Sample : SSTD08047
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080649

Quant Time: Aug 17 01:09:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 01:01:09 2022
 Response via : Initial Calibration




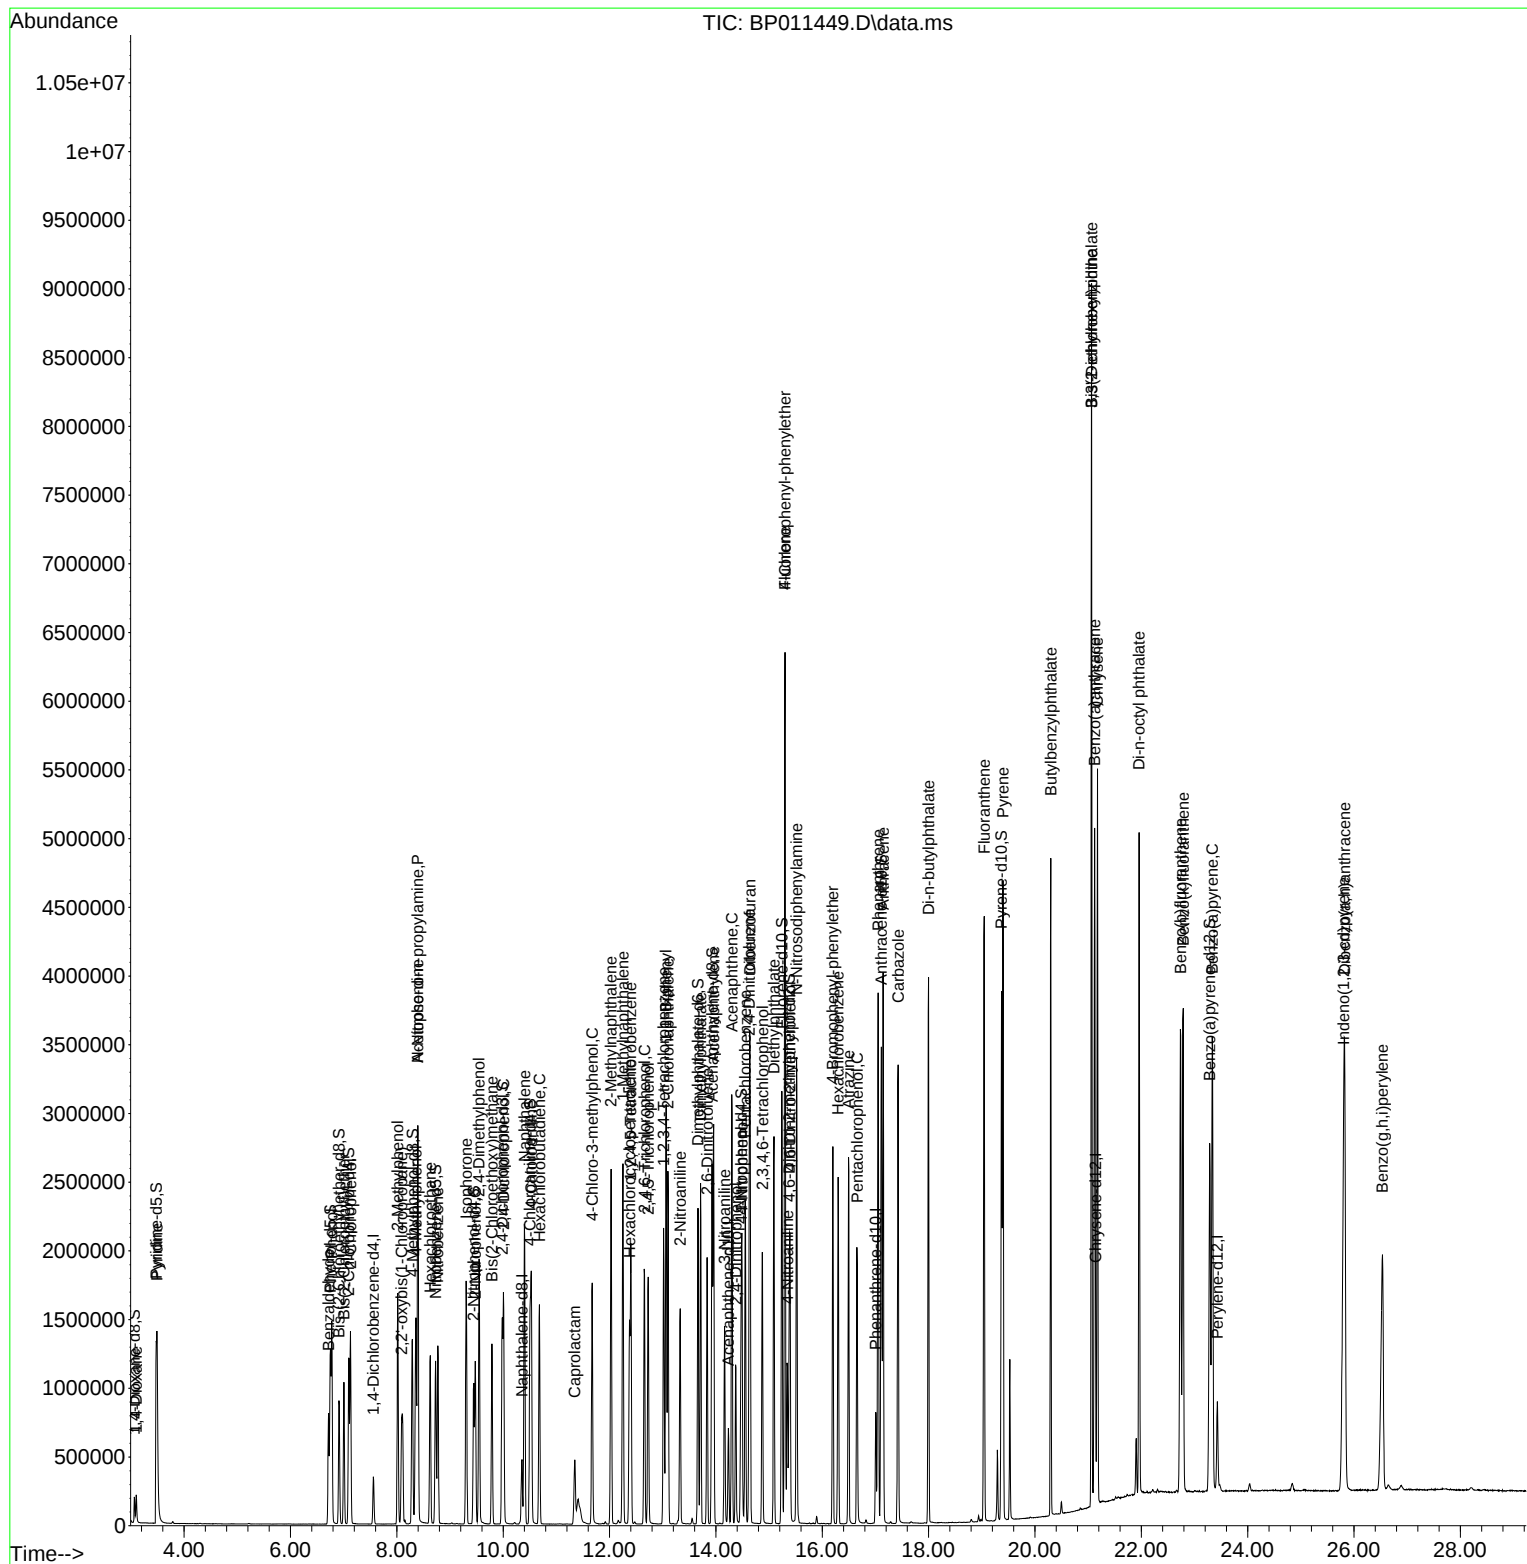




#2
1,4-Dioxane
Concen: 31.785 ng/uL
RT: 3.099 min Scan# 19
Delta R.T. -0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion: 88	Resp: 84126
Ion Ratio	Lower Upper
88 100	
43 36.9	29.0 43.4
58 81.3	64.7 97.1

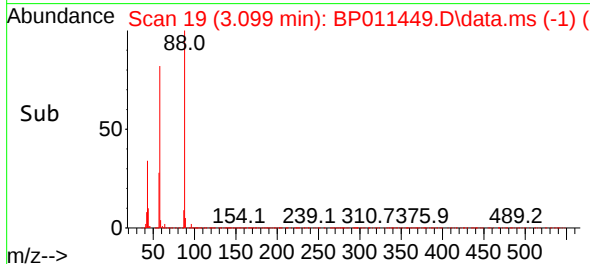

#5
Pyridine
Concen: 81.585 ng/uL
RT: 3.493 min Scan# 86
Delta R.T. -0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 79	Resp: 534142
Ion Ratio	Lower Upper
79 100	
52 86.7	70.2 105.2
51 44.5	36.1 54.1


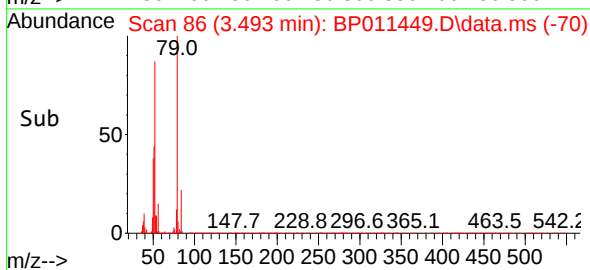

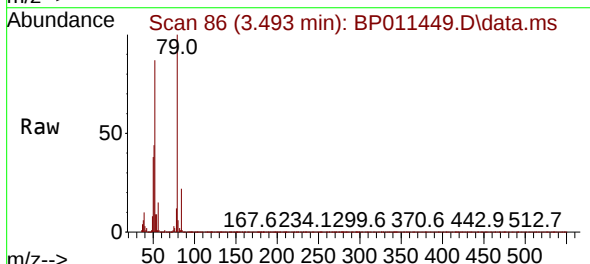




#6
Benzaldehyde
Concen: 85.469 ng/ul
RT: 6.716 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion: 77 Resp: 251797
Ion Ratio Lower Upper
77 100
105 90.8 72.0 108.0
106 87.7 67.4 101.0



#8
Phenol
Concen: 84.482 ng/ul
RT: 6.775 min Scan# 644
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 94 Resp: 618181
Ion Ratio Lower Upper
94 100
65 35.0 28.9 43.3
66 49.8 39.4 59.0



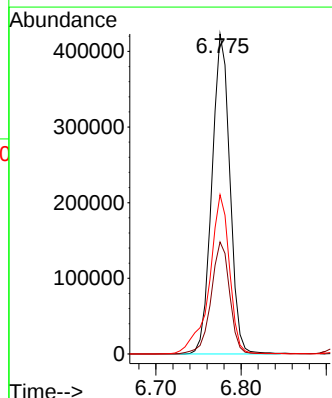





#10
Bis(2-Chloroethyl)ether
Concen: 79.273 ng/ul
RT: 7.005 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion: 93 Resp: 467156
Ion Ratio Lower Upper
93 100
63 84.5 67.8 101.6
95 32.1 25.0 37.6



#12
2-Chlorophenol
Concen: 88.418 ng/ul
RT: 7.128 min Scan# 704
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 128 Resp: 488678
Ion Ratio Lower Upper
128 100
64 52.0 40.2 60.2
130 32.8 24.6 37.0





#13

2-Methylphenol

Concen: 86.720 ng/ul

RT: 8.016 min Scan# 8

Delta R.T. -0.000 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :





SSTD080649

Tgt Ion:108 Resp: 457002

Ion Ratio Lower Upper

108 100

107 91.4 73.2 109.8

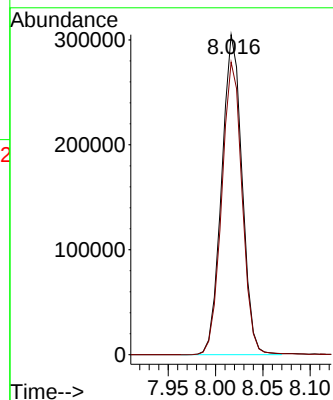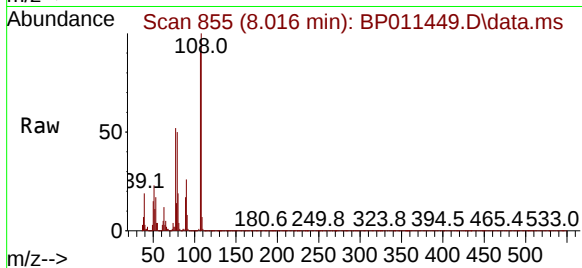

#14

2,2'-oxybis(1-Chloropropane)

Concen: 44.691 ng/ul

RT: 8.093 min Scan# 868

Delta R.T. -0.012 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion: 45 Resp: 395011


Ion Ratio Lower Upper

45 100

77 13.8 11.4 17.0

79 10.6 8.6 13.0



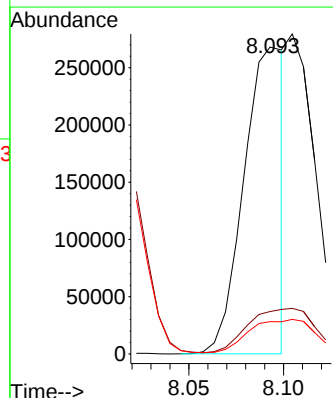
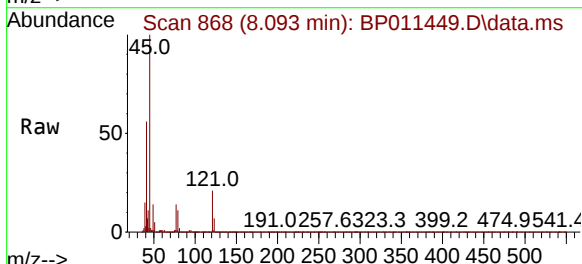




#16
Acetophenone
Concen: 91.404 ng/ul
RT: 8.393 min Scan# 919
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:105 Resp: 784951
Ion Ratio Lower Upper
105 100
77 85.2 66.4 99.6
51 35.9 28.2 42.4



#17
N-Nitroso-di-n-propylamine
Concen: 97.697 ng/ul
RT: 8.393 min Scan# 919
Delta R.T. 0.012 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 70 Resp: 413310
Ion Ratio Lower Upper
70 100
42 71.4 57.0 85.4
101 9.9 7.6 11.4
130 19.7 15.2 22.8









#18
4-Methylphenol
Concen: 88.264 ng/ul
RT: 8.358 min Scan# 911
Delta R.T. 0.012 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:108 Resp: 498564
Ion Ratio Lower Upper
108 100
107 110.0 87.7 131.5



#19
Hexachloroethane
Concen: 93.020 ng/ul
RT: 8.628 min Scan# 959
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:117 Resp: 217081
Ion Ratio Lower Upper
117 100
201 79.4 64.2 96.4
199 49.8 41.0 61.6









#22
Nitrobenzene
Concen: 95.237 ng/ul
RT: 8.769 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion: 77 Resp: 626782
Ion Ratio Lower Upper
77 100
123 39.8 30.4 45.6
65 15.3 11.5 17.3



#23
Isophorone
Concen: 92.650 ng/ul
RT: 9.305 min Scan# 1074
Delta R.T. 0.012 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 82 Resp: 1118480
Ion Ratio Lower Upper
82 100
95 8.6 7.1 10.7
138 16.3 12.6 19.0









#25
2-Nitrophenol
Concen: 108.705 ng/ul
RT: 9.475 min Scan# 1103
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:139 Resp: 272685
Ion Ratio Lower Upper
139 100
65 66.8 50.4 75.6
109 43.0 35.5 53.3



#26
2,4-Dimethylphenol
Concen: 96.361 ng/ul
RT: 9.546 min Scan# 1115
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:107 Resp: 610773
Ion Ratio Lower Upper
107 100
121 45.9 36.6 55.0
122 76.3 58.7 88.1

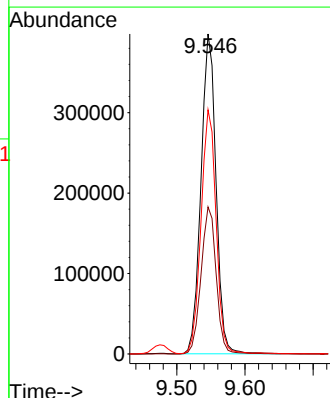



#27

Bis(2-Chloroethoxy)methane

Concen: 83.201 ng/ul

RT: 9.787 min Scan# 1155

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion: 93 Resp: 641888

Ion Ratio Lower Upper

93 100

95 33.2 24.8 37.2

123 11.0 8.2 12.4



#29

2,4-Dichlorophenol

Concen: 93.742 ng/ul

RT: 10.005 min Scan# 1193

Delta R.T. -0.000 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:162 Resp: 426111


Ion Ratio Lower Upper

162 100

164 63.3 50.2 75.2

98 43.9 32.9 49.3



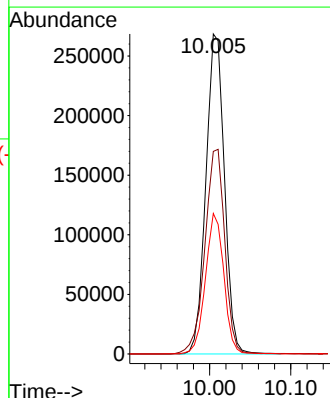





#30
Naphthalene
Concen: 82.328 ng/ul
RT: 10.399 min Scan# 1260
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:128 Resp: 1547271
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.6
127 13.2 10.3 15.5

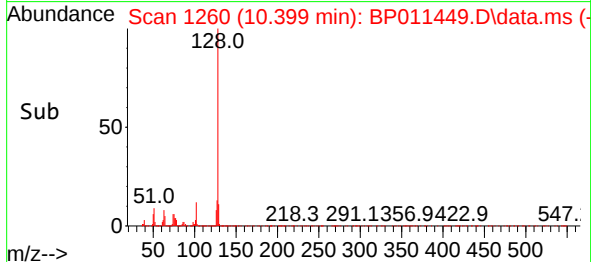

#32
4-Chloroaniline
Concen: 90.041 ng/ul
RT: 10.528 min Scan# 1282
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:127 Resp: 685854
Ion Ratio Lower Upper
127 100
129 31.8 25.1 37.7


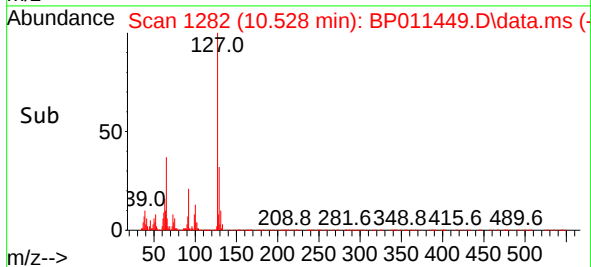

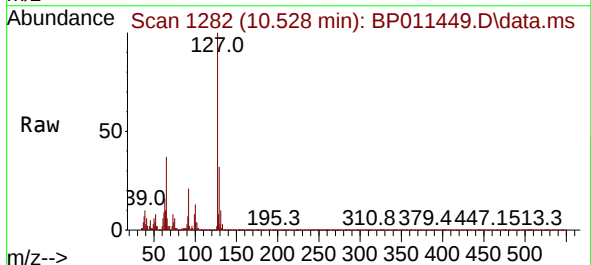




#33
Hexachlorobutadiene
Concen: 91.891 ng/ul
RT: 10.681 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:225 Resp: 256249
Ion Ratio Lower Upper
225 100
223 63.7 47.8 71.8
227 63.3 50.0 75.0

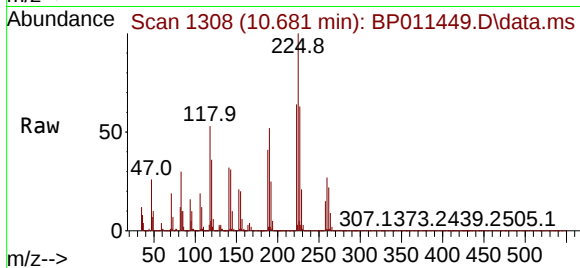

#34
Caprolactam
Concen: 55.881 ng/ul
RT: 11.346 min Scan# 1421
Delta R.T. 0.023 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:113 Resp: 84943
Ion Ratio Lower Upper
113 100
55 189.8 153.4 230.2
56 147.4 119.6 179.4


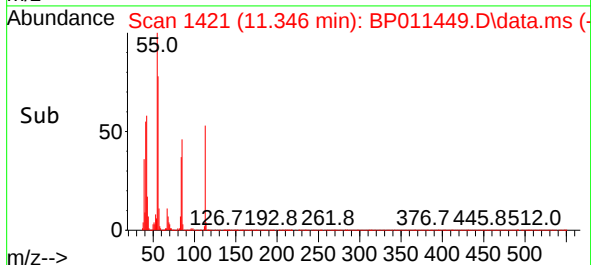
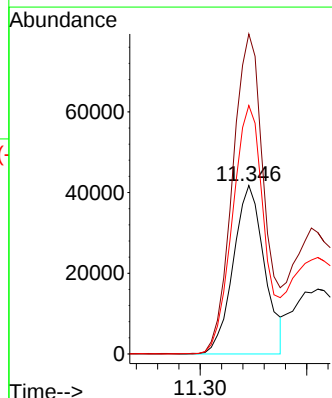
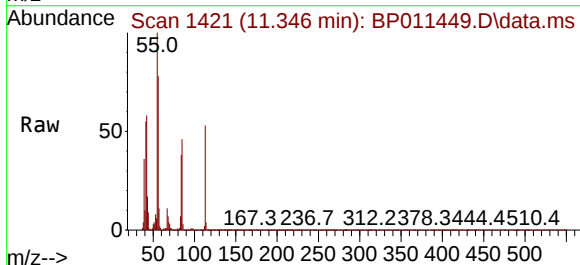




#35
4-Chloro-3-methylphenol
Concen: 103.191 ng/ul
RT: 11.675 min Scan# 1475
Delta R.T. 0.012 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:107 Resp: 551495
Ion Ratio Lower Upper
107 100
144 23.2 18.3 27.5
142 71.4 55.8 83.8



#36
2-Methylnaphthalene
Concen: 87.690 ng/ul
RT: 12.028 min Scan# 1537
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:142 Resp: 1021550
Ion Ratio Lower Upper
142 100
141 89.7 73.4 110.0









#37
1-Methylnaphthalene
Concen: 87.671 ng/ul
RT: 12.251 min Scan# 1575
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:142 Resp: 1035984
Ion Ratio Lower Upper
142 100
141 94.6 73.0 109.6
116 5.2 4.0 6.0



#39
1,2,4,5-Tetrachlorobenzene
Concen: 83.948 ng/ul
RT: 12.398 min Scan# 1600
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:216 Resp: 458732
Ion Ratio Lower Upper
216 100
214 77.6 60.4 90.6
179 26.5 20.0 30.0
108 26.5 20.2 30.4





#40

Hexachlorocyclopentadiene

Concen: 102.457 ng/ul

RT: 12.375 min Scan# 1596

Delta R.T. -0.000 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion:237 Resp: 300019

Ion Ratio Lower Upper

237 100

235 63.8 50.9 76.3

272 12.0 11.0 16.4

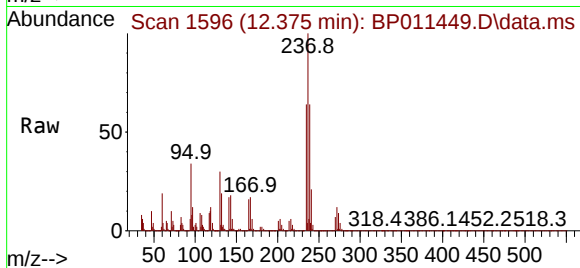

#41

2,4,6-Trichlorophenol

Concen: 97.455 ng/ul

RT: 12.657 min Scan# 1644

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:196 Resp: 322219


Ion Ratio Lower Upper

196 100

198 96.3 75.6 113.4

200 29.8 23.1 34.7









#42
2,4,5-Trichlorophenol
Concen: 97.662 ng/ul
RT: 12.728 min Scan# 1655
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:196 Resp: 344635
Ion Ratio Lower Upper
196 100
198 96.0 75.6 113.4
200 30.3 23.8 35.6



#43
1,1'-Biphenyl
Concen: 82.323 ng/ul
RT: 13.063 min Scan# 1713
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:154 Resp: 1341802
Ion Ratio Lower Upper
154 100
153 40.2 32.2 48.4
76 13.7 11.6 17.4









#44
2-Chloronaphthalene
Concen: 82.523 ng/ul
RT: 13.098 min Scan# 1719
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:162 Resp: 1009199
Ion Ratio Lower Upper
162 100
164 32.3 26.4 39.6
127 48.4 37.4 56.2

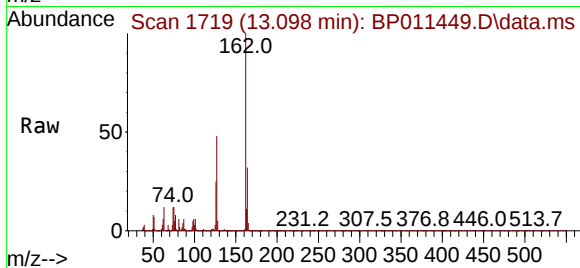

#45
2-Nitroaniline
Concen: 131.163 ng/ul
RT: 13.328 min Scan# 1758
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion: 65 Resp: 407385
Ion Ratio Lower Upper
65 100
92 63.2 50.8 76.2
138 88.5 66.7 100.1


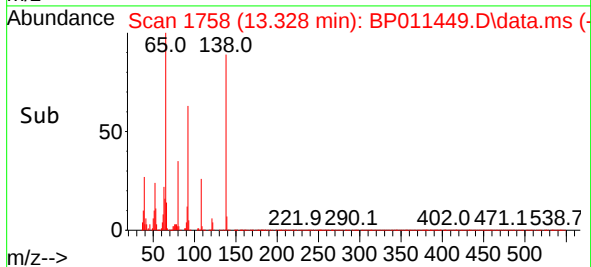

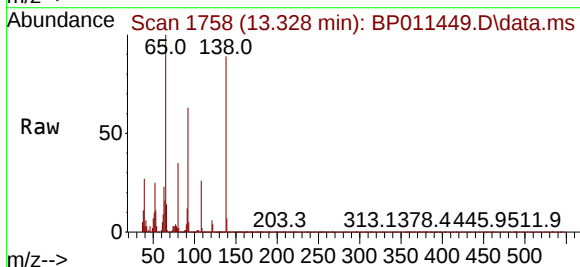


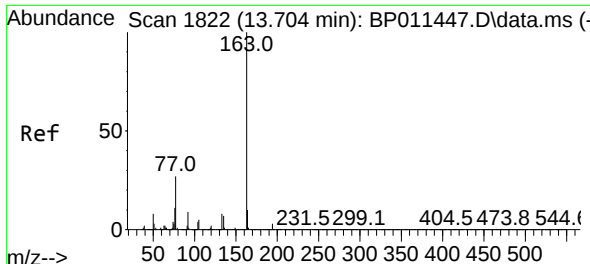

#47
Dimethylphthalate
Concen: 89.883 ng/ul
RT: 13.710 min Scan# 1823
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:163 Resp: 1311144
Ion Ratio Lower Upper
163 100
194 3.5 2.6 3.8
164 10.4 8.3 12.5



#48
2,6-Dinitrotoluene
Concen: 119.075 ng/ul
RT: 13.834 min Scan# 1844
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:165 Resp: 271587
Ion Ratio Lower Upper
165 100
89 83.1 66.6 99.8
121 27.0 21.0 31.6


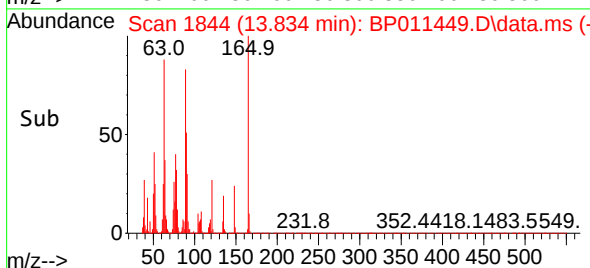
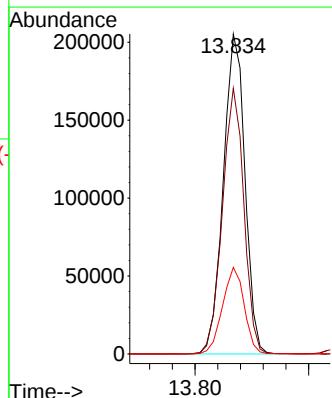
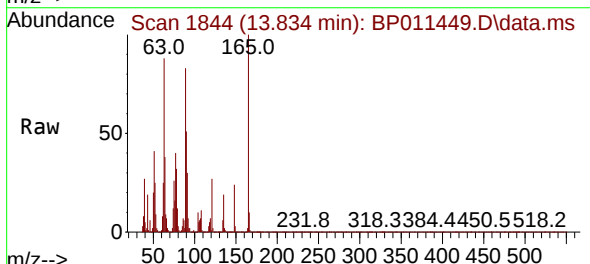




#50
Acenaphthylene
Concen: 86.085 ng/ul
RT: 13.957 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:152 Resp: 1720353
Ion Ratio Lower Upper
152 100
151 20.4 16.9 25.3
153 13.0 10.6 15.8



#51
3-Nitroaniline
Concen: 109.408 ng/ul
RT: 14.163 min Scan# 1900
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:138 Resp: 274505
Ion Ratio Lower Upper
138 100
108 11.8 8.6 13.0
92 130.3 104.2 156.2









#52
Acenaphthene
Concen: 84.316 ng/ul
RT: 14.298 min Scan# 1923
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:153 Resp: 1123783
Ion Ratio Lower Upper
153 100
152 47.1 37.7 56.5
154 87.0 69.4 104.0

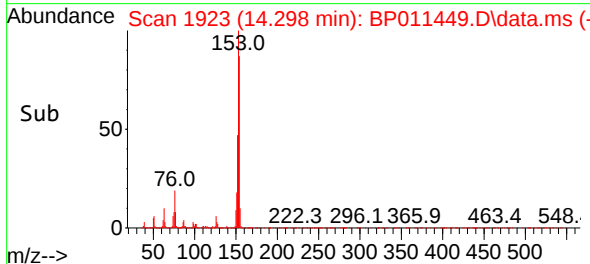

#53
2,4-Dinitrophenol
Concen: 121.271 ng/ul
RT: 14.375 min Scan# 1936
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:184 Resp: 164110
Ion Ratio Lower Upper
184 100
63 99.8 82.5 123.7
154 84.3 66.6 100.0


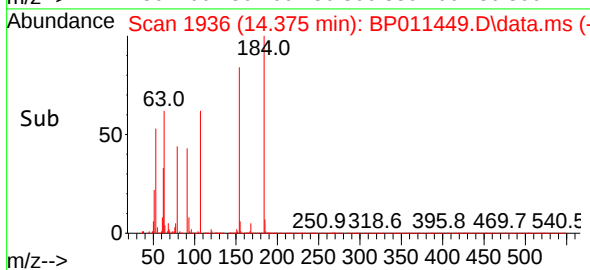

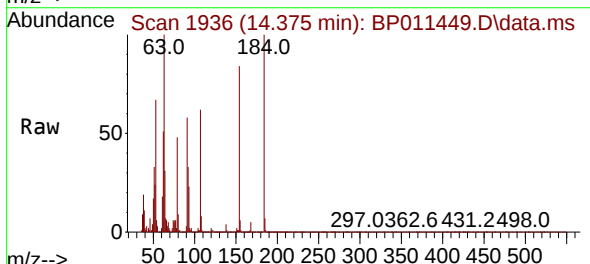




#55
4-Nitrophenol
Concen: 126.173 ng/ul
RT: 14.493 min Scan# 1956
Delta R.T. 0.018 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:109 Resp: 307893
Ion Ratio Lower Upper
109 100
139 92.1 76.0 114.0
65 113.5 98.8 148.2



#56
Dibenzofuran
Concen: 84.419 ng/ul
RT: 14.640 min Scan# 1981
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:168 Resp: 1525383
Ion Ratio Lower Upper
168 100
139 48.5 38.4 57.6









#57
2,4-Dinitrotoluene
Concen: 114.292 ng/ul
RT: 14.628 min Scan# 1978
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:165 Resp: 399560
Ion Ratio Lower Upper
165 100
63 75.7 60.2 90.2
182 2.5 1.8 2.8



#58
2,3,4,6-Tetrachlorophenol
Concen: 99.711 ng/ul
RT: 14.875 min Scan# 2021
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:232 Resp: 273728
Ion Ratio Lower Upper
232 100
131 67.9 55.4 83.0
130 4.0 3.6 5.4
166 39.9 31.0 46.4


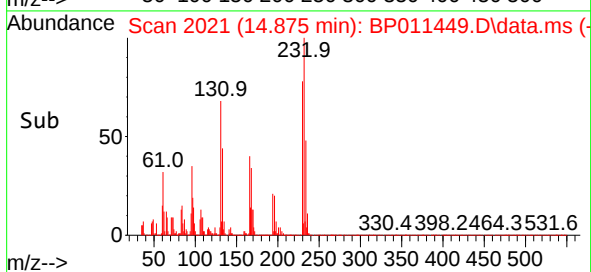






#59
Diethylphthalate
Concen: 96.520 ng/ul
RT: 15.092 min Scan# 2058
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:149 Resp: 1458578
Ion Ratio Lower Upper
149 100
177 19.1 15.7 23.5
150 12.5 10.1 15.1

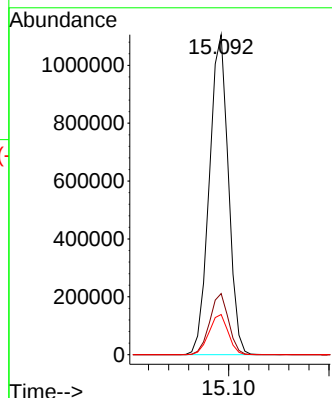

#61
Fluorene
Concen: 87.861 ng/ul
RT: 15.298 min Scan# 2093
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:166 Resp: 1289289
Ion Ratio Lower Upper
166 100
165 100.1 78.2 117.2
167 13.4 10.3 15.5



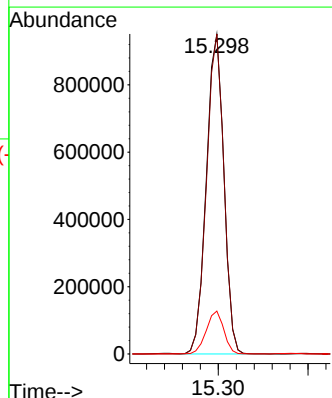





#62
4-Chlorophenyl-phenylether
Concen: 89.251 ng/ul
RT: 15.298 min Scan# 2100
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:204 Resp: 572502
Ion Ratio Lower Upper
204 100
206 33.2 25.4 38.0
141 83.6 66.5 99.7

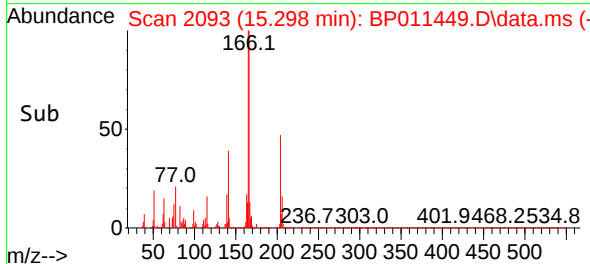

#63
4-Nitroaniline
Concen: 97.599 ng/ul
RT: 15.345 min Scan# 2101
Delta R.T. 0.018 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:138 Resp: 238277
Ion Ratio Lower Upper
138 100
92 56.8 49.5 74.3
108 112.9 93.7 140.5


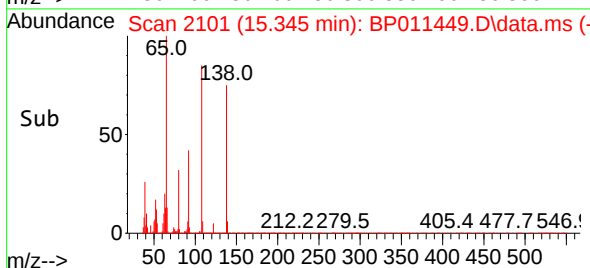
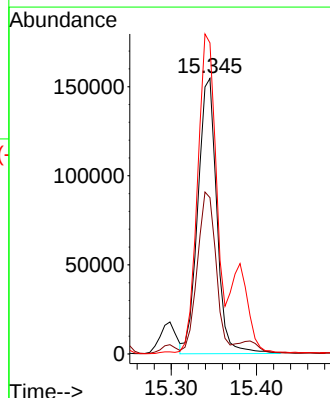





#66
4,6-Dinitro-2-methylphenol
Concen: 106.962 ng/ul
RT: 15.392 min Scan# 2109
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:198 Resp: 216998
Ion Ratio Lower Upper
198 100
182 4.3 3.9 5.9
77 42.5 30.1 45.1



#67
N-Nitrosodiphenylamine
Concen: 86.743 ng/ul
RT: 15.516 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:169 Resp: 1084228
Ion Ratio Lower Upper
169 100
168 66.9 54.6 82.0
167 36.8 30.2 45.4



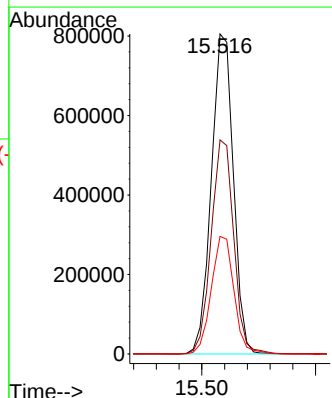





#68
4-Bromophenyl-phenylether
Concen: 88.637 ng/ul
RT: 16.198 min Scan# 211
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:248 Resp: 332704
Ion Ratio Lower Upper
248 100
250 98.9 82.8 124.2
141 116.1 90.8 136.2



#69
Hexachlorobenzene
Concen: 86.358 ng/ul
RT: 16.298 min Scan# 2263
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:284 Resp: 378693
Ion Ratio Lower Upper
284 100
142 55.7 43.5 65.3
249 34.0 28.4 42.6

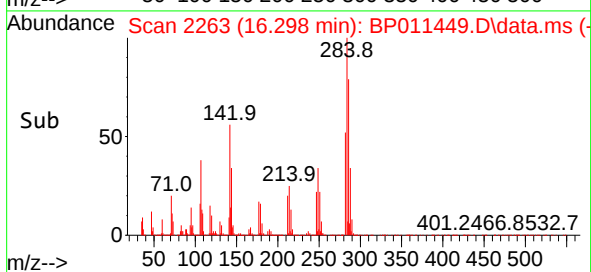



#70

Atrazine

Concen: 96.052 ng/ul

RT: 16.498 min Scan# 21

Delta R.T. 0.012 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion:200 Resp: 400178

Ion Ratio Lower Upper

200 100

173 26.2 22.0 33.0

215 43.1 36.3 54.5

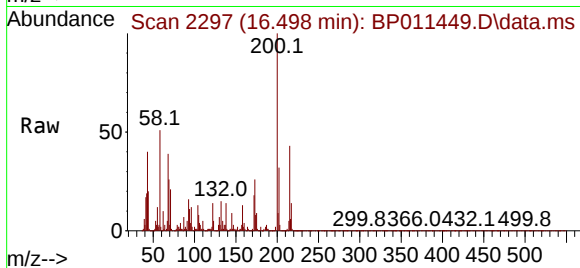

#71

Pentachlorophenol

Concen: 96.185 ng/ul

RT: 16.657 min Scan# 2324

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:266 Resp: 244858


Ion Ratio Lower Upper

266 100

264 63.8 50.6 76.0

268 65.8 51.3 76.9

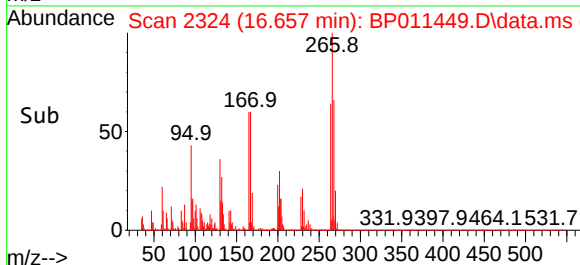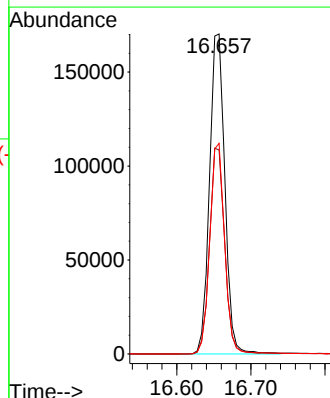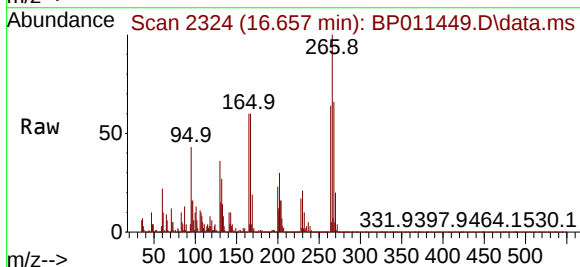



#72

Phenanthrene

Concen: 82.402 ng/u1

RT: 17.051 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion:178 Resp: 1959880

Ion Ratio Lower Upper

178 100

179 15.1 12.6 18.8

176 19.5 15.8 23.8

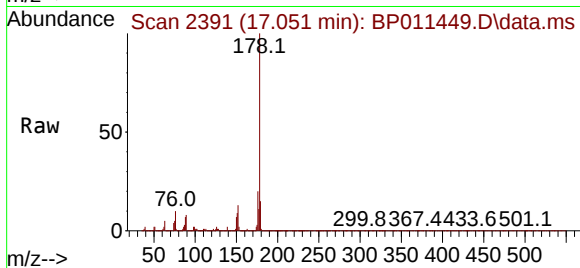

#74

Anthracene

Concen: 84.983 ng/u1

RT: 17.145 min Scan# 2407

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:178 Resp: 2012205


Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.2

176 18.9 15.4 23.0


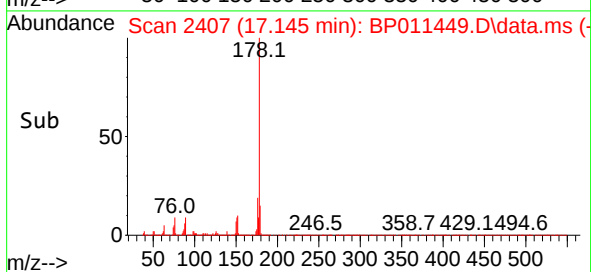




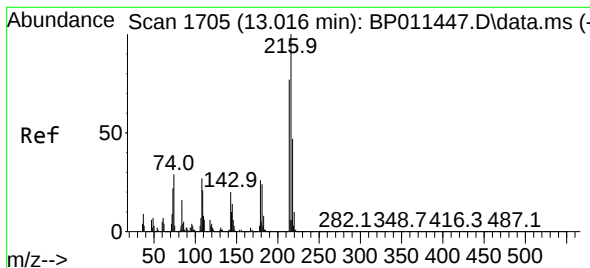

#75
1,2,3,4-Tetrachlorobenzene
Concen: 77.314 ng/uL
RT: 13.016 min Scan# 1705
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:216 Resp: 470800
Ion Ratio Lower Upper
216 100
214 79.6 61.8 92.6
218 48.4 37.4 56.0

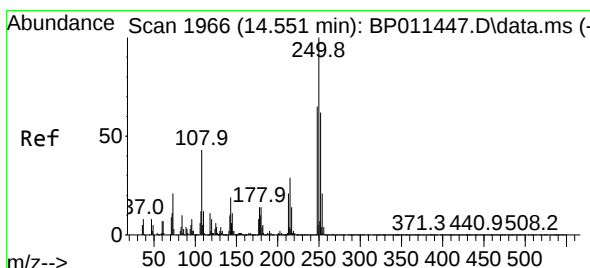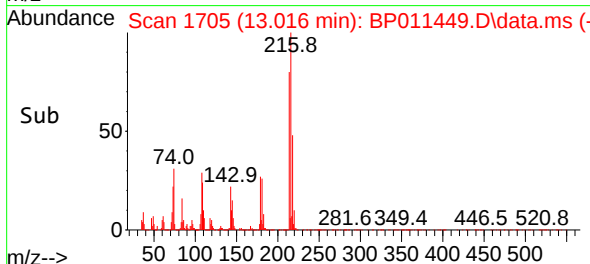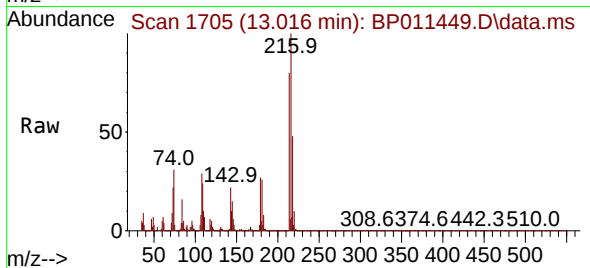

#76
Pentachlorobenzene
Concen: 84.244 ng/uL
RT: 14.551 min Scan# 1966
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:250 Resp: 446762
Ion Ratio Lower Upper
250 100
248 63.7 51.7 77.5
252 62.5 50.0 75.0


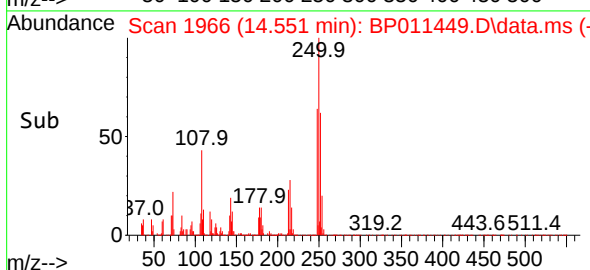






#77
 Carbazole
 Concen: 83.795 ng/ul
 RT: 17.428 min Scan# 2454
 Delta R.T. 0.006 min
 Lab File: BP011449.D
 Acq: 16 Aug 2022 18:01




Instrument :
 BNA_P
 ClientSampleId :
 SSTD080649


Tgt Ion:167 Resp: 1854031
 Ion Ratio Lower Upper
 167 100
 166 21.8 17.5 26.3
 139 16.1 12.1 18.1



#78
 Di-n-butylphthalate
 Concen: 104.742 ng/ul
 RT: 17.998 min Scan# 2552
 Delta R.T. 0.006 min
 Lab File: BP011449.D
 Acq: 16 Aug 2022 18:01

Tgt Ion:149 Resp: 2534109
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.4 11.2
 104 6.7 5.5 8.3









#80
Fluoranthene
Concen: 83.057 ng/ul
RT: 19.045 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:202 Resp: 2259178
Ion Ratio Lower Upper
202 100
101 11.2 9.5 14.3
100 8.9 7.9 11.9



#82
Pyrene
Concen: 80.956 ng/ul
RT: 19.398 min Scan# 2790
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:202 Resp: 2324214
Ion Ratio Lower Upper
202 100
101 14.0 11.4 17.2
100 12.1 9.4 14.0









#83
Butylbenzylphthalate
Concen: 128.551 ng/ul
RT: 20.298 min Scan# 2942
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:149 Resp: 1176093
Ion Ratio Lower Upper
149 100
91 80.6 68.5 102.7
206 17.1 12.6 18.8



#84
3,3'-Dichlorobenzidine
Concen: 91.122 ng/ul
RT: 21.063 min Scan# 3073
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:252 Resp: 672656
Ion Ratio Lower Upper
252 100
254 65.3 51.2 76.8
126 14.9 12.2 18.2





#85

Benzo(a)anthracene

Concen: 83.245 ng/ul

RT: 21.122 min Scan# 3082

Delta R.T. 0.006 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion:228 Resp: 2166272

Ion Ratio Lower Upper

228 100

229 20.0 16.0 24.0

226 27.7 22.6 33.8

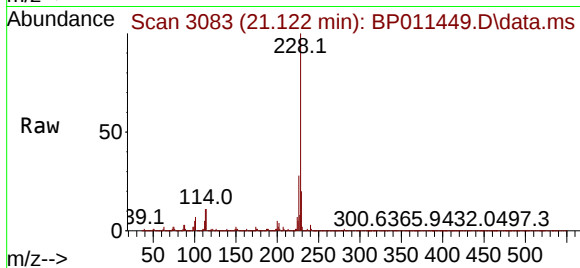

#86

Bis(2-ethylhexyl)phthalate

Concen: 120.430 ng/ul

RT: 21.063 min Scan# 3073

Delta R.T. -0.000 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:149 Resp: 1768753


Ion Ratio Lower Upper

149 100

167 24.8 19.8 29.8

279 3.3 2.7 4.1









#87
Chrysene
Concen: 81.971 ng/ul
RT: 21.174 min Scan# 3091
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:228 Resp: 2111609
Ion Ratio Lower Upper
228 100
226 30.6 23.9 35.9
229 19.6 16.0 24.0



#89
Di-n-octyl phthalate
Concen: 106.652 ng/ul
RT: 21.957 min Scan# 3225
Delta R.T. -0.000 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:149 Resp: 2908495





#90

Benzo(b)fluoranthene

Concen: 84.616 ng/ul

RT: 22.739 min Scan# 31

Delta R.T. 0.012 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01

Instrument :

BNA_P

ClientSampleId :

SSTD080649





Tgt Ion:252 Resp: 2188940

Ion Ratio Lower Upper

252 100

253 21.7 17.5 26.3

125 10.3 9.0 13.4



#91

Benzo(k)fluoranthene

Concen: 83.848 ng/ul

RT: 22.786 min Scan# 3366

Delta R.T. 0.012 min

Lab File: BP011449.D

Acq: 16 Aug 2022 18:01




Tgt Ion:252 Resp: 2122218


Ion Ratio Lower Upper

252 100

253 21.6 17.9 26.9

125 10.9 9.8 14.8


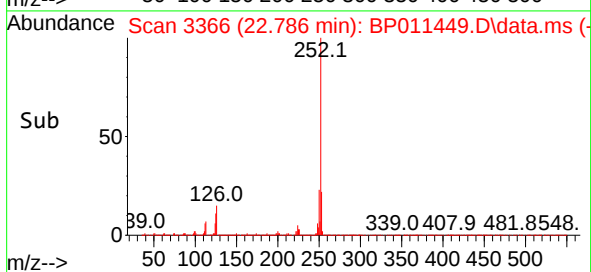






#93
Benzo(a)pyrene
Concen: 86.631 ng/ul
RT: 23.333 min Scan# 3458
Delta R.T. 0.006 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01




Instrument :
BNA_P
ClientSampleId :
SSTD080649


Tgt Ion:252 Resp: 2161487
Ion Ratio Lower Upper
252 100
253 21.8 16.8 25.2
125 12.6 9.9 14.9



#94
Indeno(1,2,3-cd)pyrene
Concen: 88.508 ng/ul
RT: 25.804 min Scan# 3879
Delta R.T. 0.018 min
Lab File: BP011449.D
Acq: 16 Aug 2022 18:01

Tgt Ion:276 Resp: 2441287
Ion Ratio Lower Upper
276 100
138 25.9 20.2 30.4
277 25.2 20.1 30.1



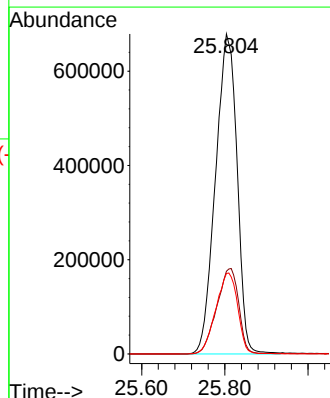





#95
 Dibenzo(a,h)anthracene
 Concen: 90.016 ng/ul
 RT: 25.821 min Scan# 3882
 Delta R.T. 0.018 min
 Lab File: BP011449.D
 Acq: 16 Aug 2022 18:01

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080649

Tgt Ion:278 Resp: 2111618
 Ion Ratio Lower Upper
 278 100
 139 17.4 15.4 23.0
 279 23.5 19.3 28.9

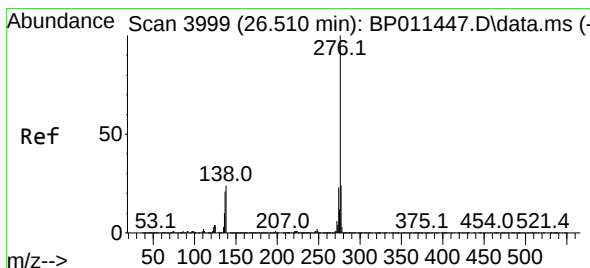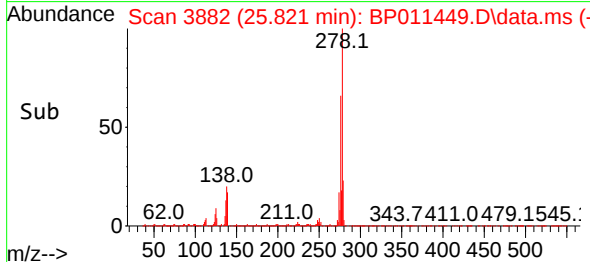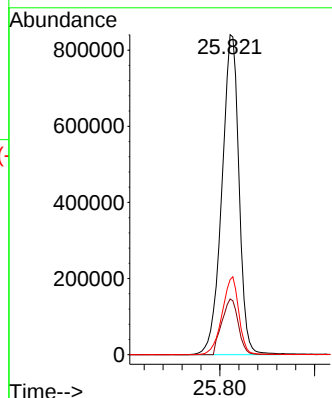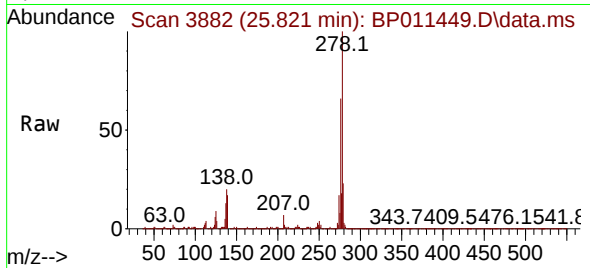

#96
 Benzo(g,h,i)perylene
 Concen: 87.160 ng/ul
 RT: 26.533 min Scan# 4003
 Delta R.T. 0.023 min
 Lab File: BP011449.D
 Acq: 16 Aug 2022 18:01

Tgt Ion:276 Resp: 2028607
 Ion Ratio Lower Upper
 276 100
 138 24.1 19.4 29.2
 277 24.1 19.1 28.7

