
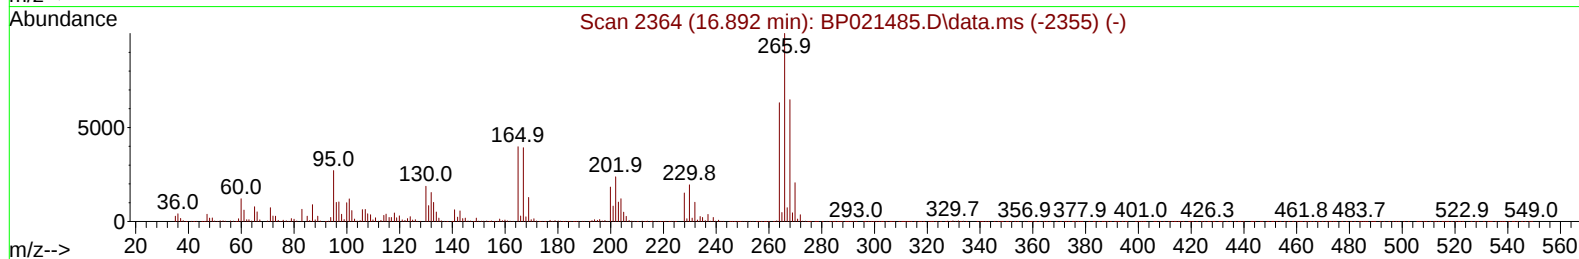
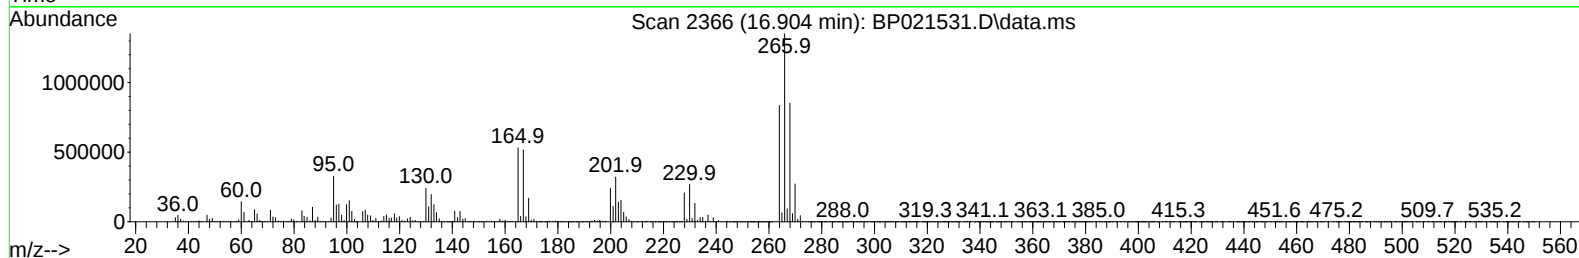


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081624\
Data File : BP021531.D
Acq On : 16 Aug 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 11:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

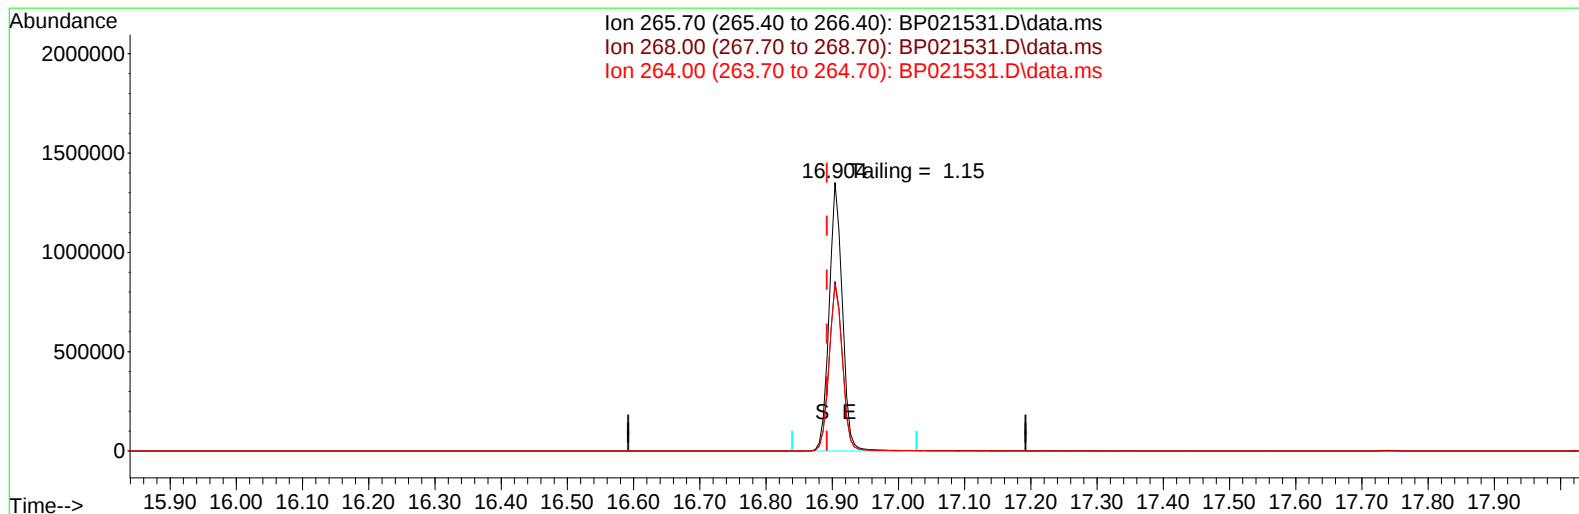

TIC: BP021531.D\data.ms

(70) Pentachlorophenol (C)




16.904min (+ 0.012) 1554275.02 ng

response 1878016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.14
264.00	63.10	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081624\
Data File : BP021531.D
Acq On : 16 Aug 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 11:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

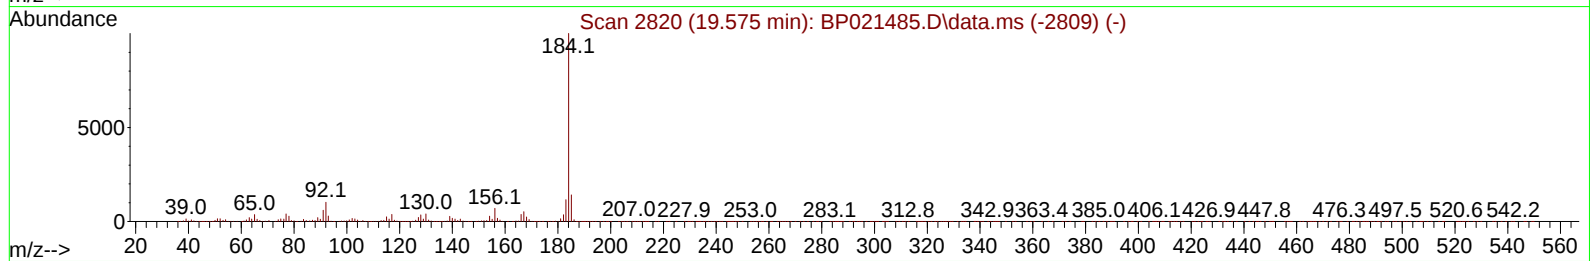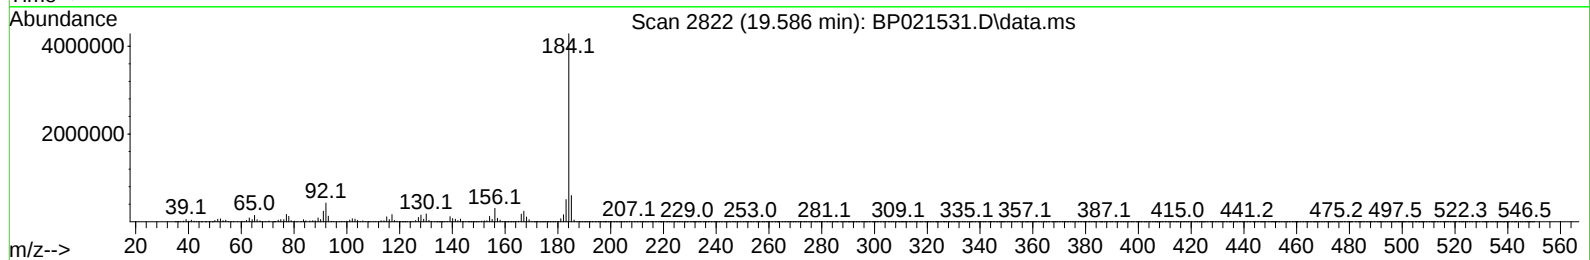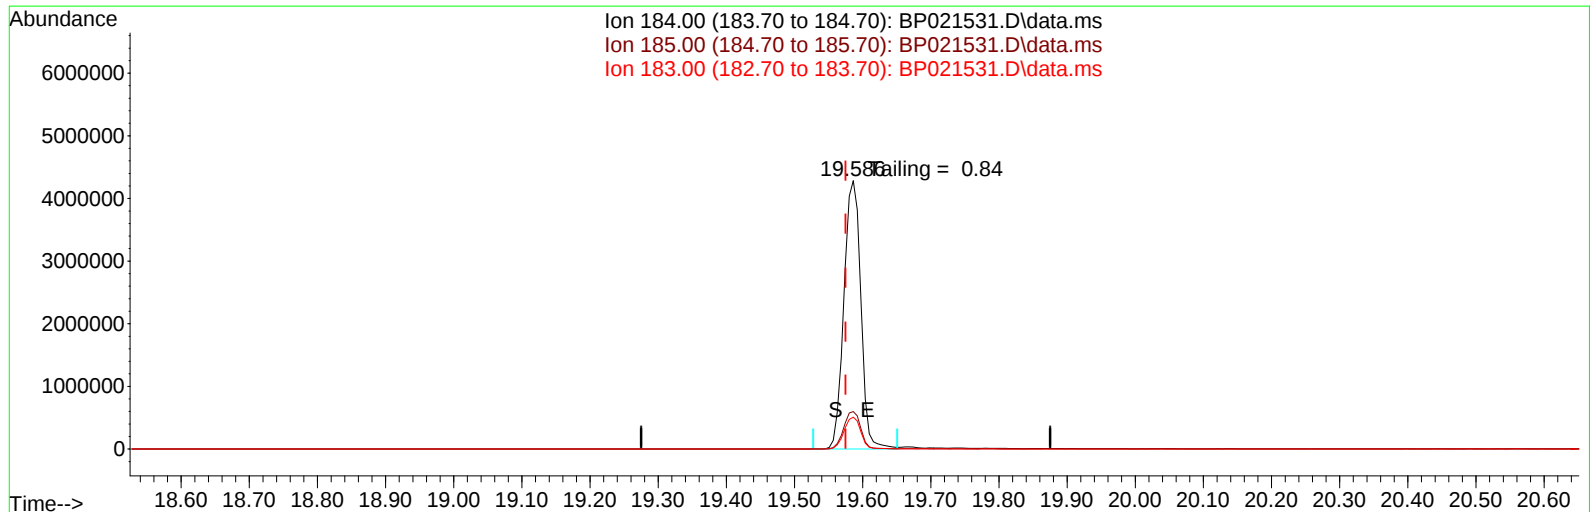

TIC: BP021531.D\data.ms

(77) Benzidine**19.586min (+ 0.011) -20.00 ng****response 7414128**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.97
183.00	11.60	11.88
0.00	0.00	0.00