
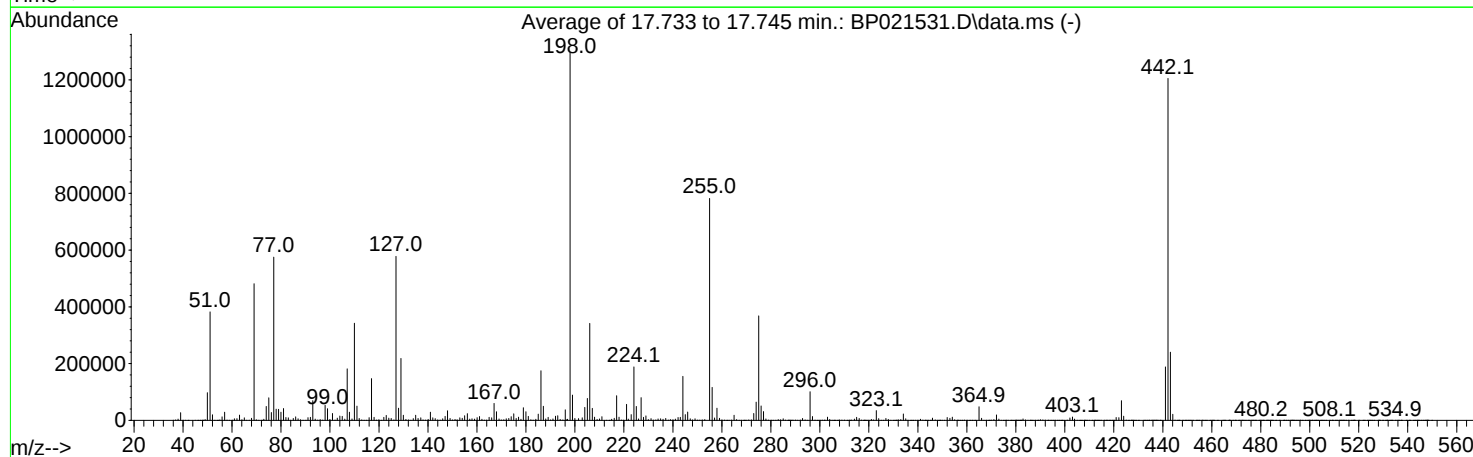


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081624\
Data File : BP021531.D
Acq On : 16 Aug 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 14 00:00:30 2024

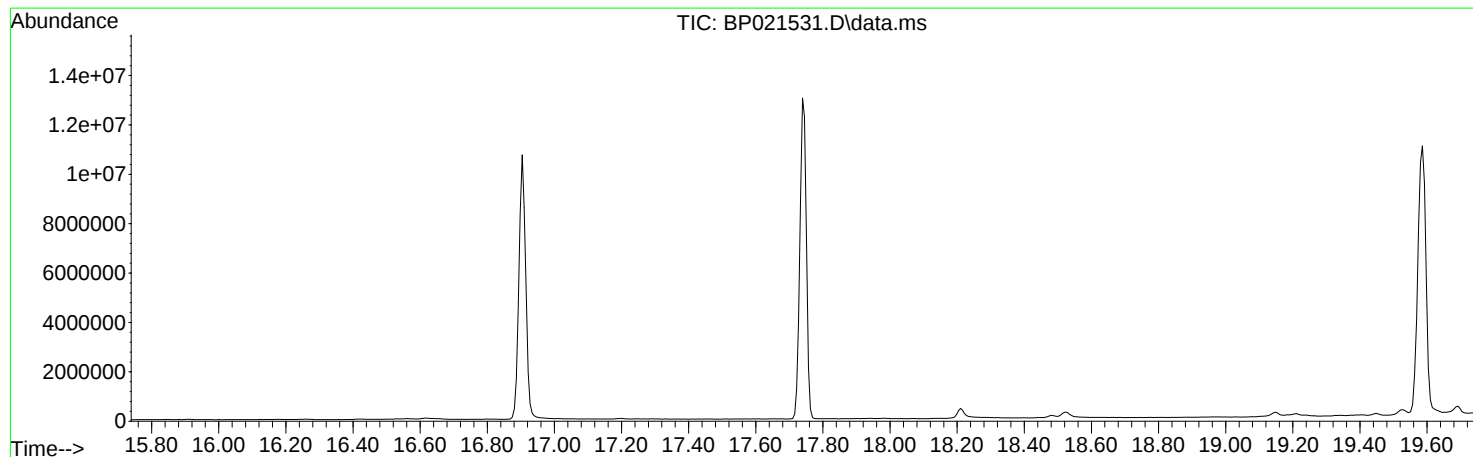

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	382307	PASS
68	69	0.00	2	1.6	7598	PASS
69	198	0.00	100	37.1	481377	PASS
70	69	0.00	2	0.5	2547	PASS
127	198	10	80	44.6	578019	PASS
197	198	0.00	2	0.3	4162	PASS
198	198	100	100	100.0	1296403	PASS
199	198	5	9	6.9	89402	PASS
275	198	10	60	28.4	368349	PASS
365	198	1	100	3.7	48220	PASS
441	198	0.01	100	14.5	188260	PASS
442	442	100	100	100.0	1204955	PASS
443	442	15	24	19.9	240171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2024	BNA_P	<u>BP021531.D</u>
Compound Name	Response	Retention Time
DDT	4111049	20.886
DDD	73605	20.463
DDE	2145	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
75750	4186799	1.81

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081624\
Data File : BP021531.D
Acq On : 16 Aug 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 16 11:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

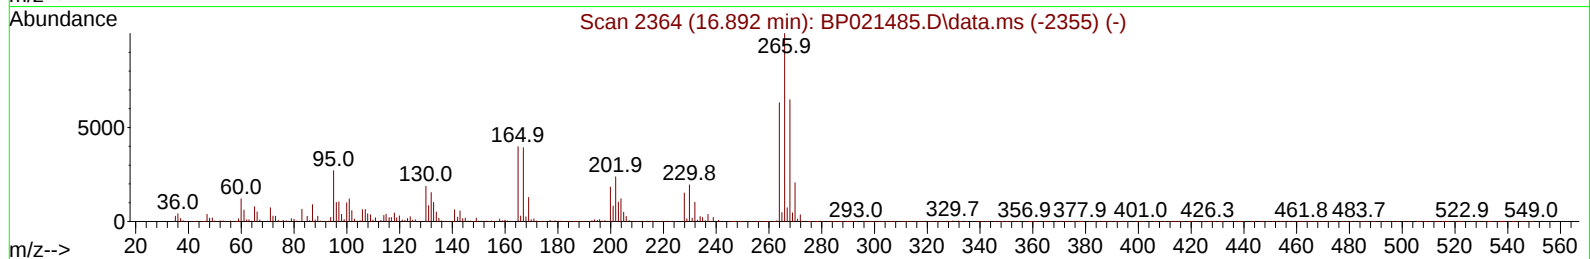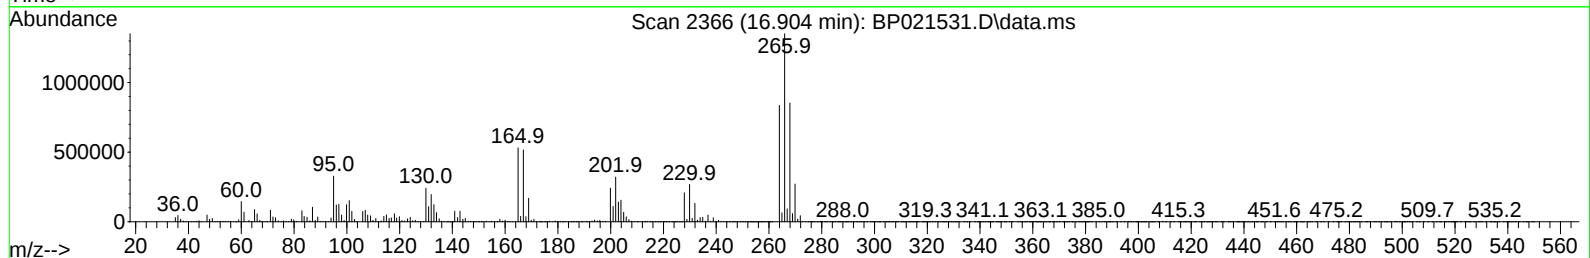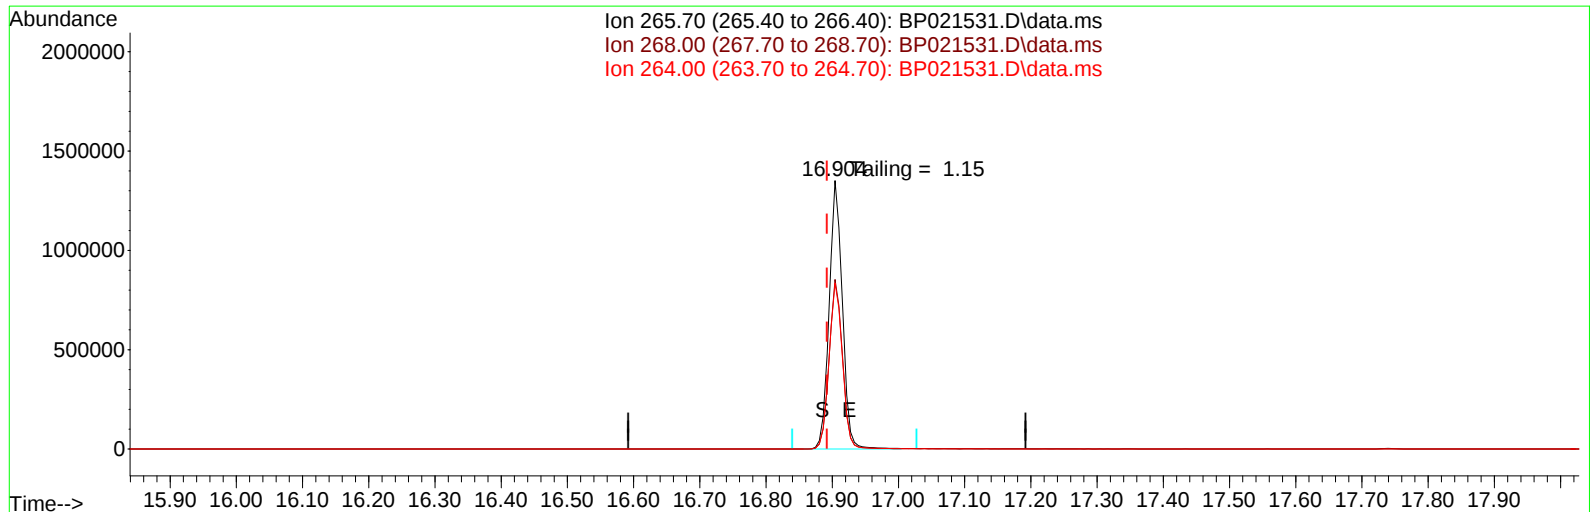

TIC: BP021531.D\data.ms

(70) Pentachlorophenol (C)

16.904min (+ 0.012) 1554275.02 ng




response 1878016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.14
264.00	63.10	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081624\
Data File : BP021531.D
Acq On : 16 Aug 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 16 11:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 00:00:30 2024
Response via : Initial Calibration

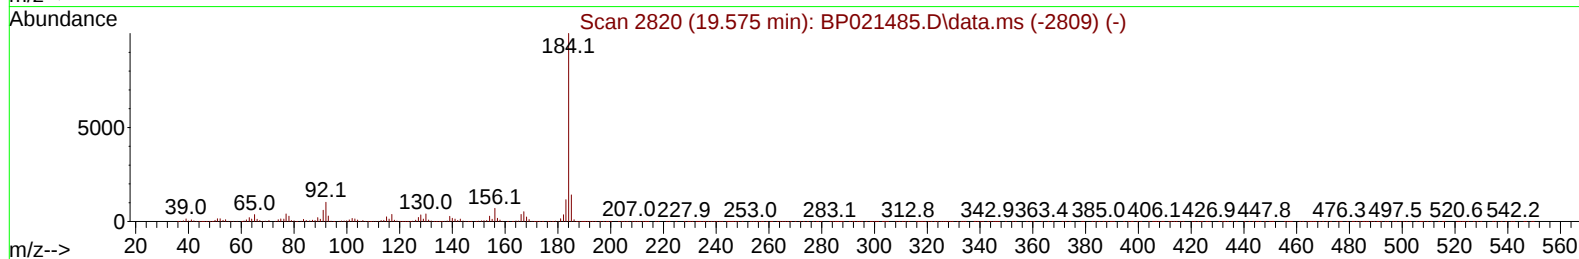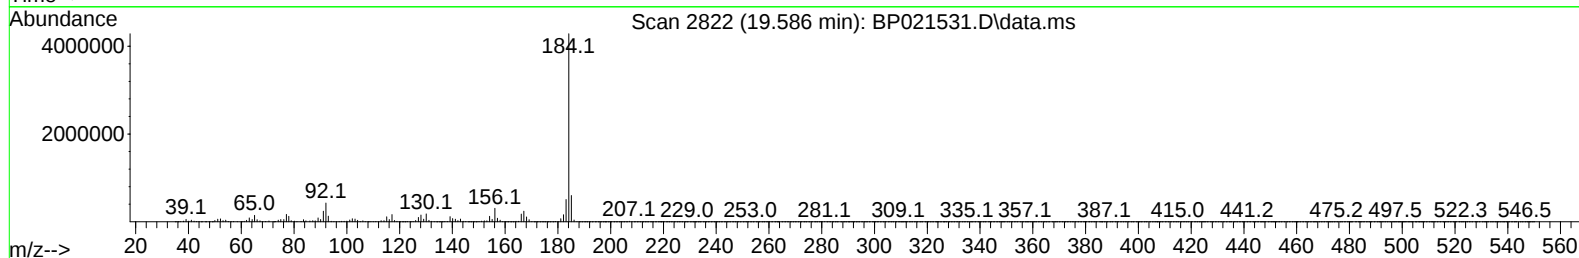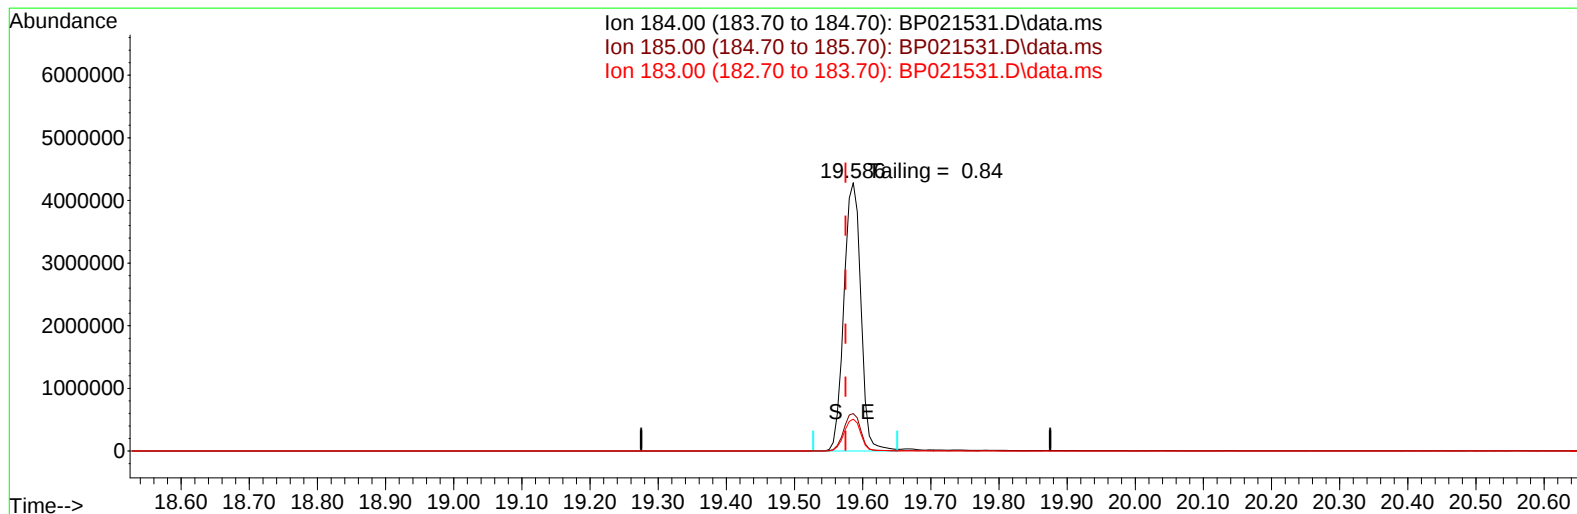

TIC: BP021531.D\data.ms

(77) Benzidine

19.586min (+ 0.011) -20.00 ng

response 7414128

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.97
183.00	11.60	11.88
0.00	0.00	0.00