


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081720\
 Data File : BP002994.D
 Acq On : 17 Aug 2020 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 14:07:35 2020

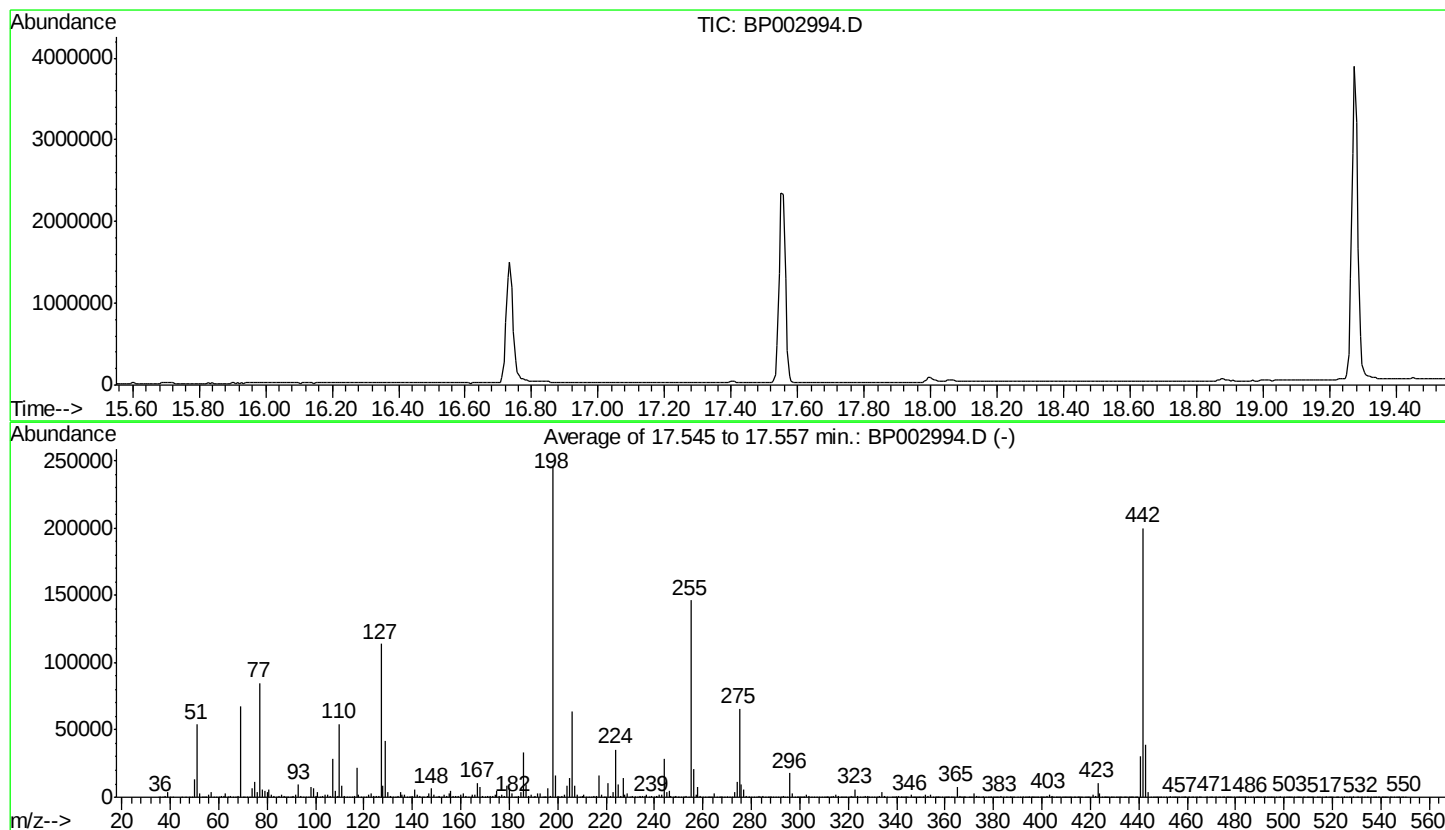

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.0	54095	PASS
68	69	0.00	2	1.9	1265	PASS
69	198	0.00	100	27.5	67719	PASS
70	69	0.00	2	0.4	284	PASS
127	198	10	80	46.2	113709	PASS
197	198	0.00	2	0.3	809	PASS
198	198	100	100	100.0	246272	PASS
199	198	5	9	6.8	16658	PASS
275	198	10	60	26.7	65864	PASS
365	198	1	100	3.3	8106	PASS
441	198	0.01	100	12.2	30080	PASS
442	198	50	100	81.2	199882	PASS
443	442	15	24	19.5	38949	PASS