
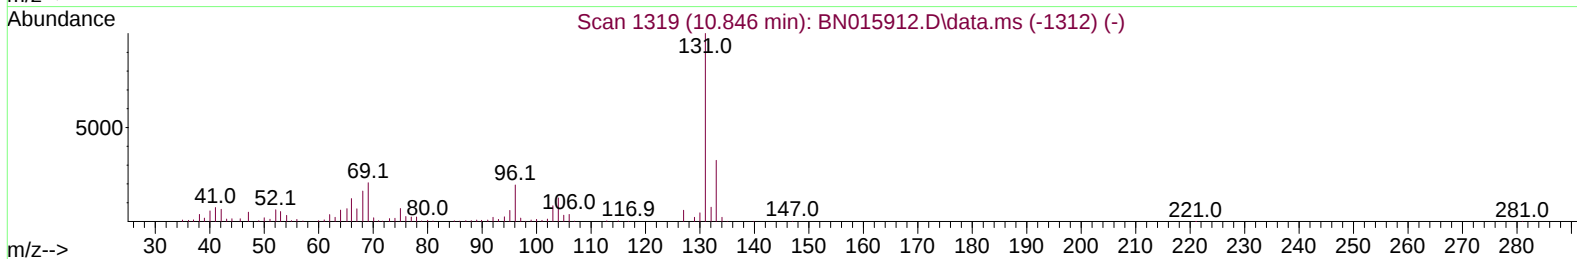
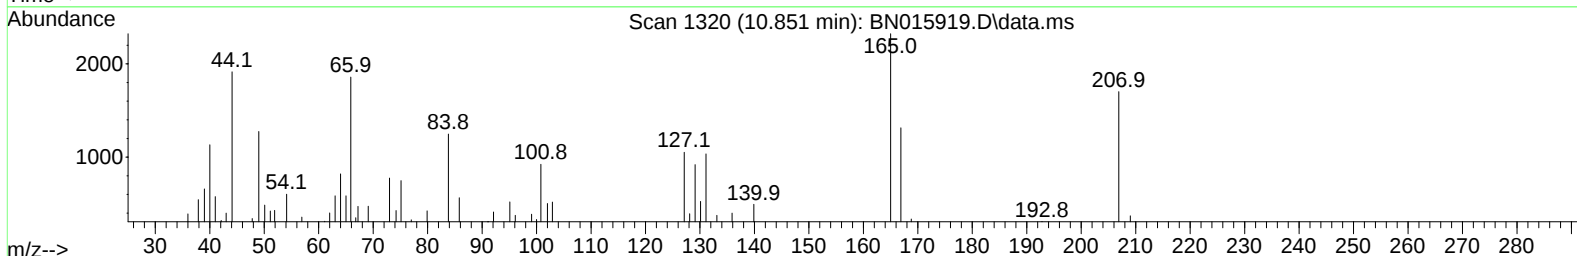


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081721\
Data File : BN015919.D
Acq On : 18 Aug 2021 03:50
Operator : CG/JU
Sample : M3355-03MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Aug 18 04:40:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 17 09:43:53 2021
Response via : Initial Calibration

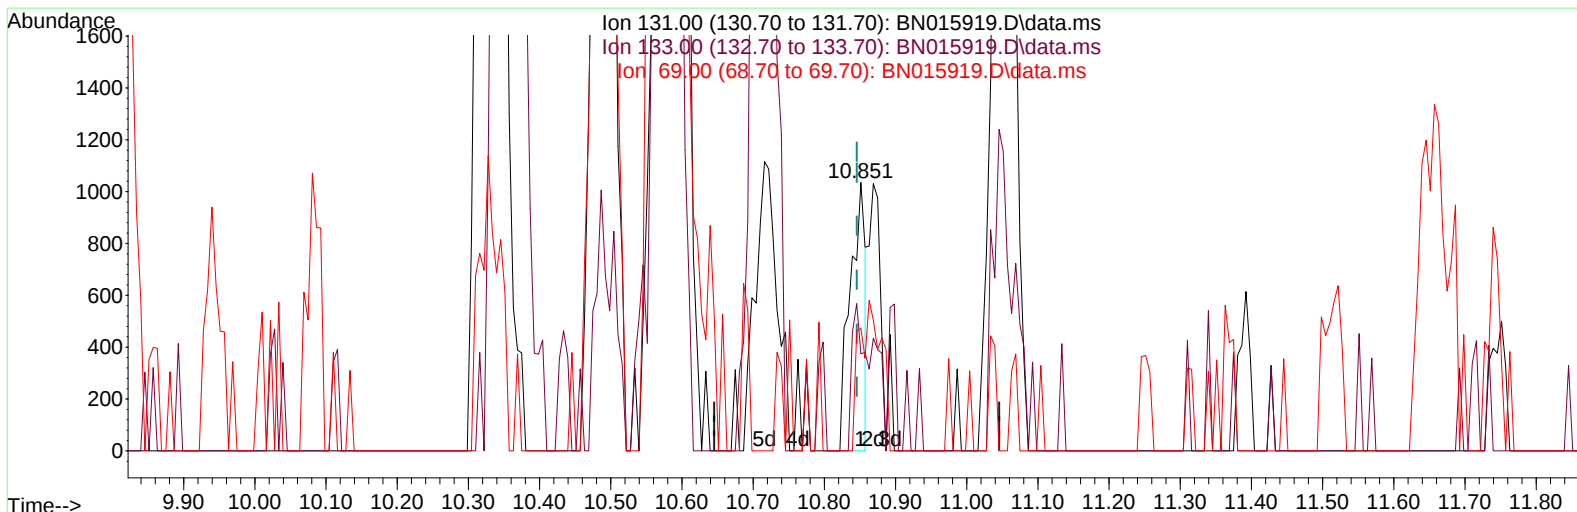

TIC: BN015919.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.851min (+ 0.006) 0.06 ng/u1

response 1520

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.40	36.23
69.00	21.40	45.70#
0.00	0.00	0.00